

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030117\
 Data File : BM009061.D
 Acq On : 01 Mar 2017 21:24
 Operator : SJ/MA
 Sample : I1988-17
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DABT1

Quant Time: Mar 02 03:56:15 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM022317.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 02 03:54:18 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.90	152	189752	20.00	ng/ul	0.00
18) Naphthalene-d8	10.70	136	716875	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.53	164	432299	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.28	188	1021419	20.00	ng/ul	0.00
75) Chrysene-d12	21.45	240	1289965	20.00	ng/ul	0.00
83) Perylene-d12	23.80	264	1259726	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.36	96	23016	4.87	ng/uL	0.00
5) Phenol-d5	7.05	99	432698	25.16	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.23	67	329716	26.77	ng/ul	0.00
9) 2-Chlorophenol-d4	7.42	132	297201	25.94	ng/ul	0.00
13) 4-Methylphenol-d8	8.59	113	324386	25.69	ng/ul	0.00
19) Nitrobenzene-d5	9.06	128	148152	28.88	ng/ul	0.00
22) 2-Nitrophenol-d4	9.78	143	149695	27.04	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.31	165	297284	25.58	ng/ul	0.00
29) 4-Chloroaniline-d4	10.83	131	380585	31.07	ng/ul	0.00
43) Dimethylphthalate-d6	13.94	166	954690	32.80	ng/ul	0.00
46) Acenaphthylene-d8	14.23	160	1158617	32.41	ng/ul	0.00
51) 4-Nitrophenol-d4	14.72	143	138120	27.17	ng/ul	0.00
57) Fluorene-d10	15.53	176	862572	31.74	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.64	200	130056	21.16	ng/ul	0.00
70) Anthracene-d10	17.38	188	1422150	29.41	ng/ul	0.00
76) Pyrene-d10	19.67	212	1702493	30.28	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.65	264	1750421	30.60	ng/ul	0.00


Target Compounds						Qvalue
44) Dimethylphthalate	13.99	163	442327	15.19	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030117\
Data File : BM009061.D
Acq On : 01 Mar 2017 21:24
Operator : SJ/MA
Sample : I1988-17
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DABT1

Quant Time: Mar 02 03:56:15 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM022317.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 02 03:54:18 2017
Response via : Initial Calibration

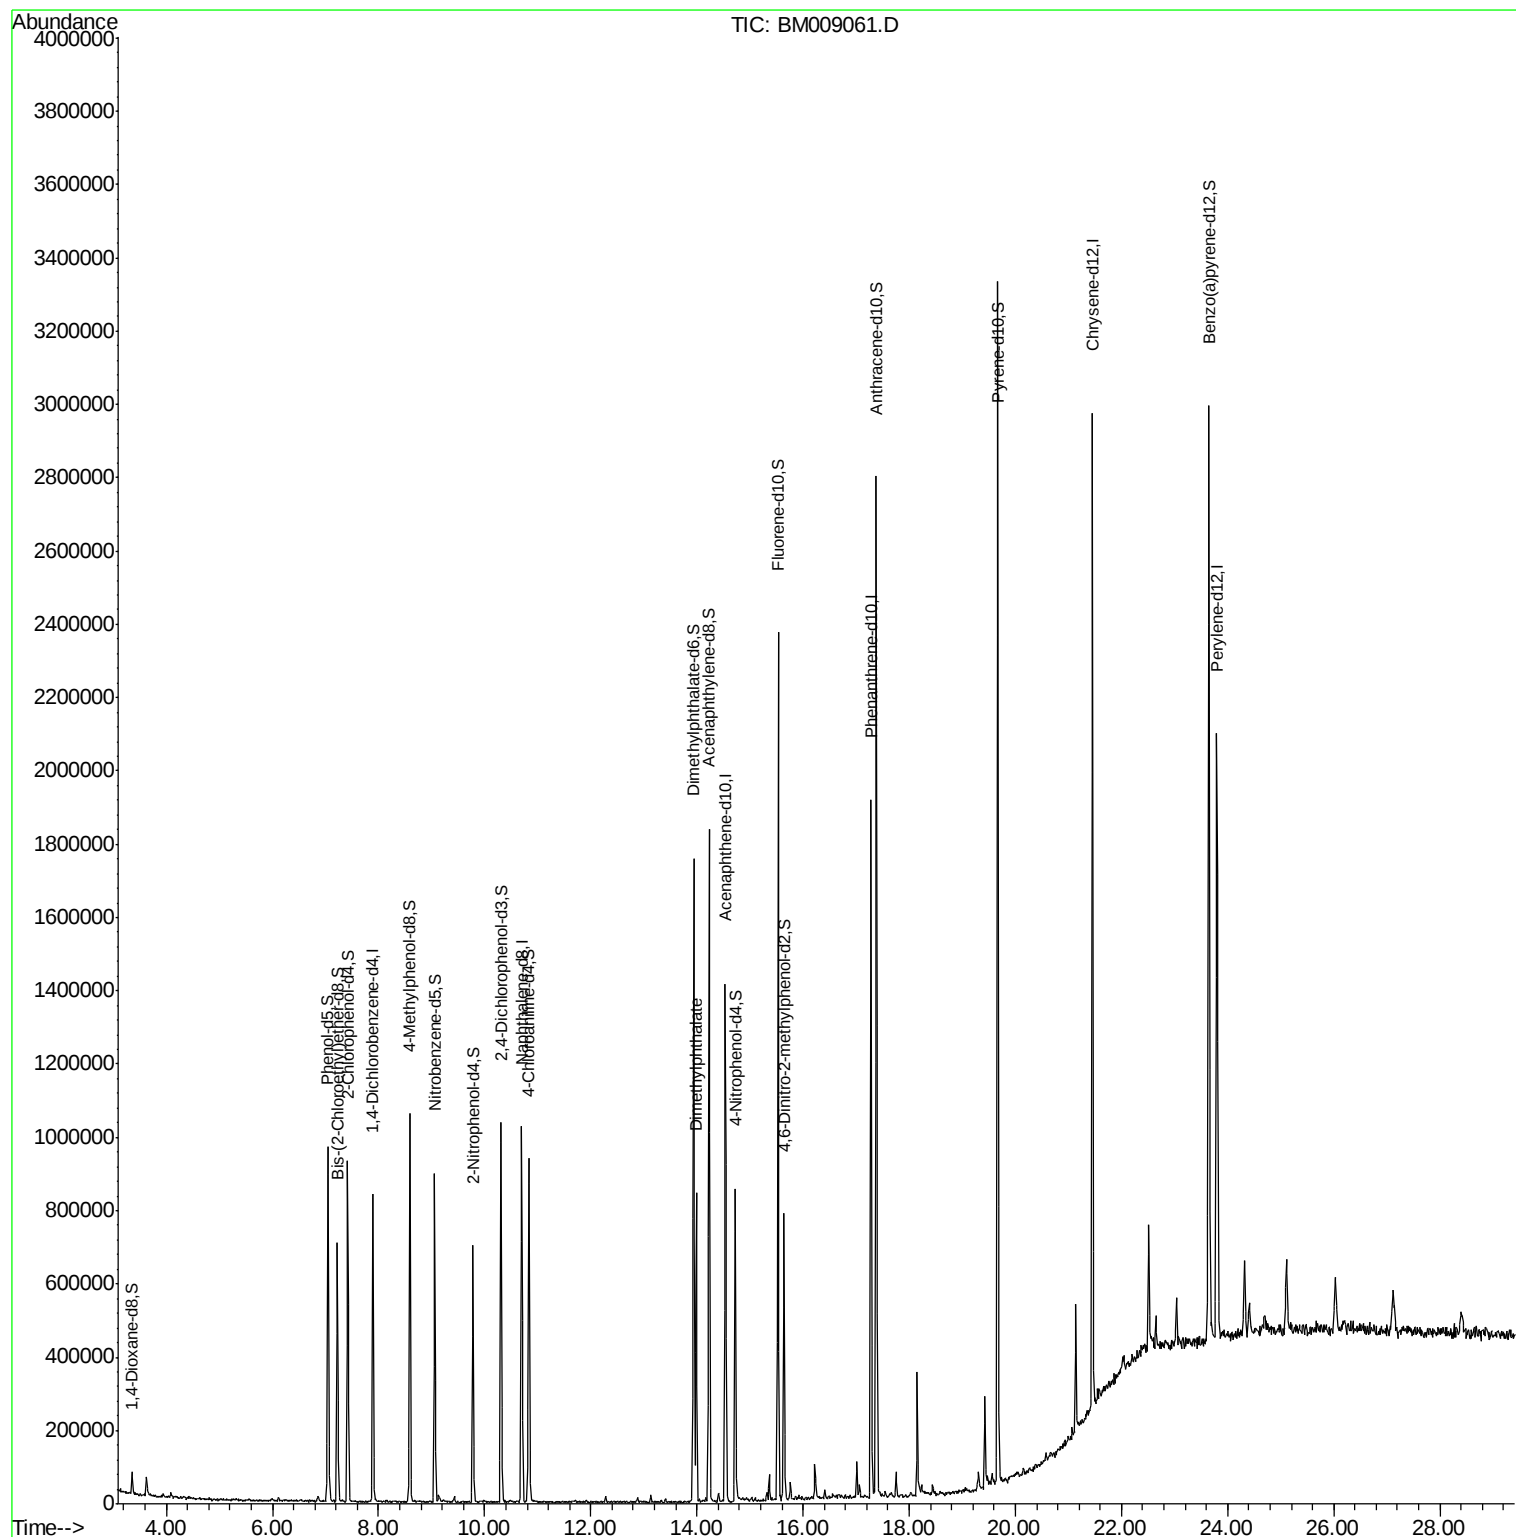

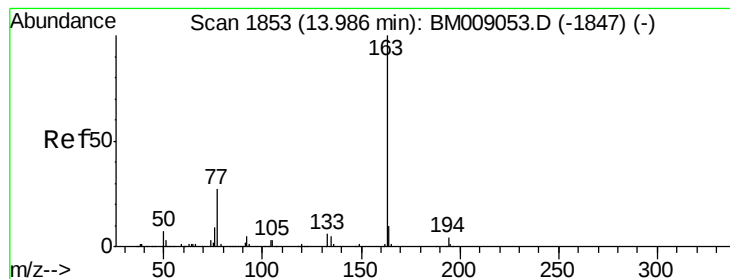

#44

Dimethylphthalate

Concen: 15.19 ng/ul

RT: 13.99 min Scan# 1853

Delta R.T. 0.00 min

Lab File: BM009061.D

Acq: 01 Mar 2017 21:24

Instrument :

BNA_M

ClientSampleId :

DABT1



Tgt Ion:163 Resp: 442327

Ion Ratio Lower Upper

163 100

194 4.1 3.0 4.6

164 11.0 8.6 12.8

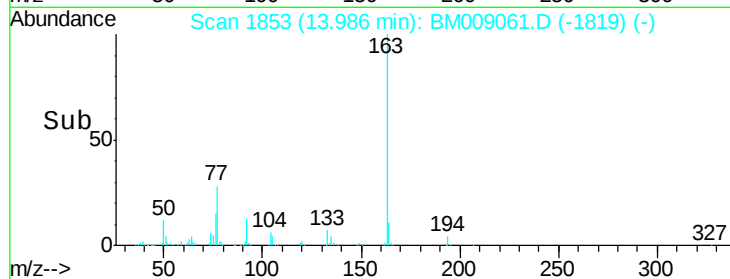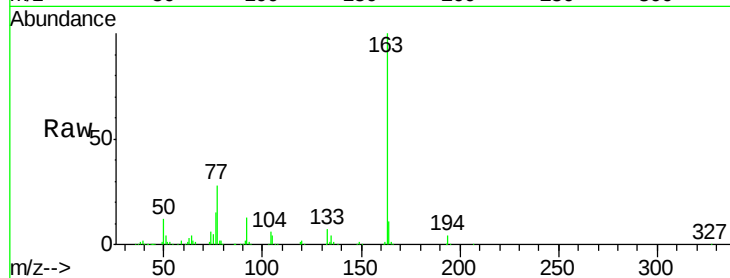

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

