

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030117\
 Data File : BM009063.D
 Acq On : 01 Mar 2017 22:38
 Operator : SJ/MA
 Sample : I1988-19
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DABT3

Quant Time: Mar 02 03:56:30 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM022317.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 02 03:54:18 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.90	152	189572	20.00	ng/ul	0.00
18) Naphthalene-d8	10.70	136	744136	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.53	164	444412	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.28	188	1049650	20.00	ng/ul	0.00
75) Chrysene-d12	21.45	240	1309530	20.00	ng/ul	0.00
83) Perylene-d12	23.80	264	1226810	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.36	96	21275	4.51	ng/uL	0.00
5) Phenol-d5	7.05	99	423775	24.66	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.22	67	311183	25.29	ng/ul	0.00
9) 2-Chlorophenol-d4	7.42	132	287088	25.08	ng/ul	0.00
13) 4-Methylphenol-d8	8.59	113	287815	22.81	ng/ul	0.00
19) Nitrobenzene-d5	9.06	128	135863	25.52	ng/ul	0.00
22) 2-Nitrophenol-d4	9.78	143	148331	25.82	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.31	165	289469	24.00	ng/ul	0.00
29) 4-Chloroaniline-d4	10.83	131	342449	26.93	ng/ul	0.00
43) Dimethylphthalate-d6	13.94	166	903036	30.18	ng/ul	0.00
46) Acenaphthylene-d8	14.23	160	1115410	30.35	ng/ul	0.00
51) 4-Nitrophenol-d4	14.72	143	125442	24.01	ng/ul	0.00
57) Fluorene-d10	15.53	176	837622	29.98	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.64	200	115200	18.24	ng/ul	0.00
70) Anthracene-d10	17.38	188	1340987	26.98	ng/ul	0.00
76) Pyrene-d10	19.67	212	1583488	27.74	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.65	264	1538690	27.62	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.99	163	429367	14.34	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030117\
Data File : BM009063.D
Acq On : 01 Mar 2017 22:38
Operator : SJ/MA
Sample : I1988-19
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
DABT3

Quant Time: Mar 02 03:56:30 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM022317.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 02 03:54:18 2017
Response via : Initial Calibration

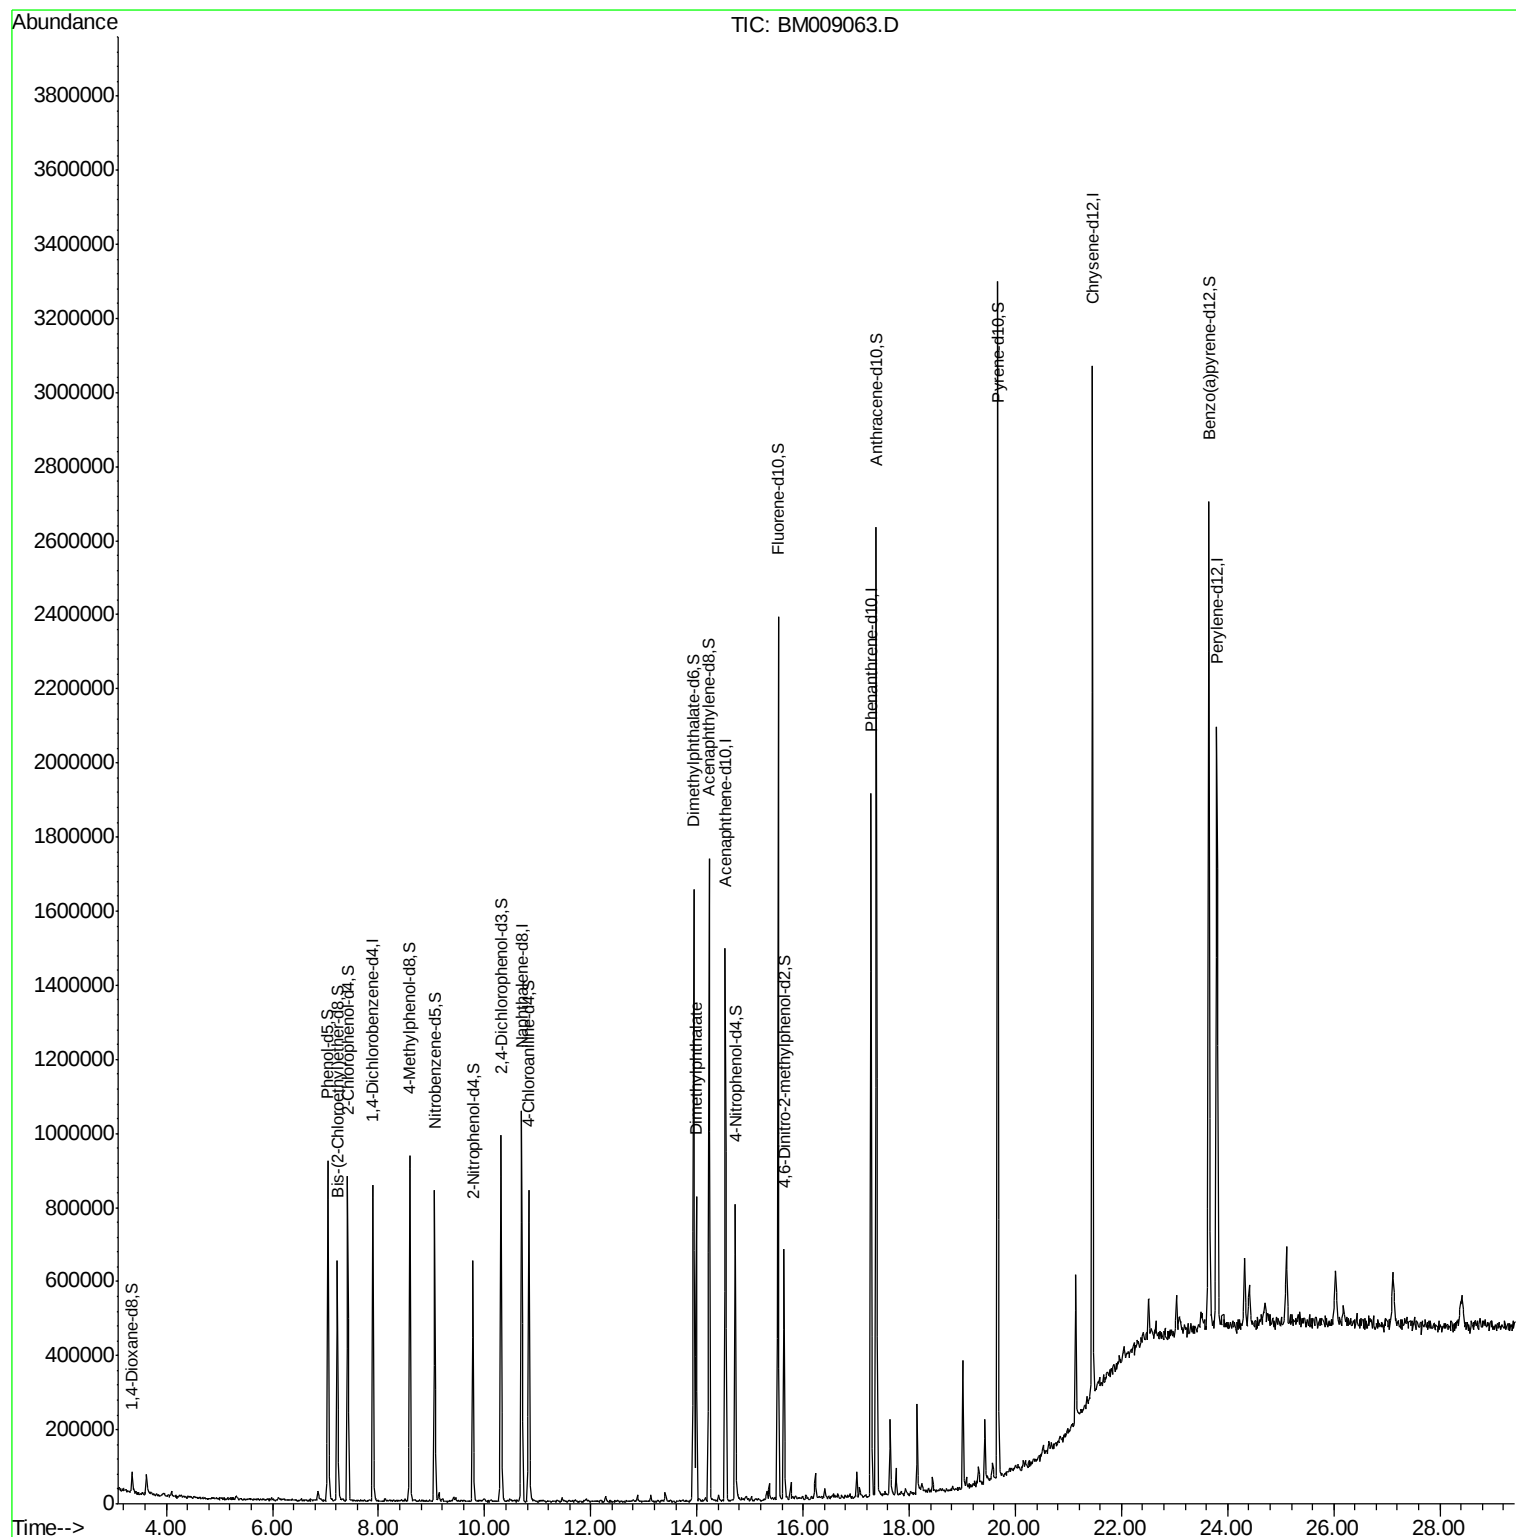

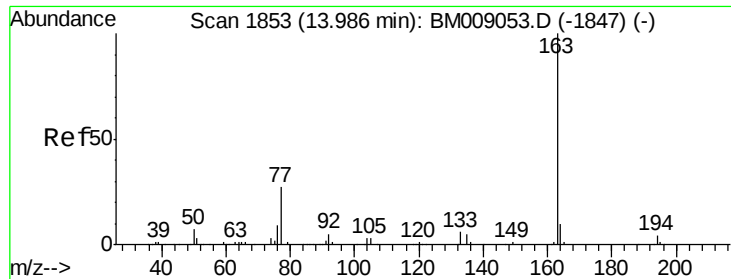

#44

Dimethylphthalate

Concen: 14.34 ng/ul

RT: 13.99 min Scan# 1853

Delta R.T. -0.00 min

Lab File: BM009063.D


Acq: 01 Mar 2017 22:38

Instrument :

BNA_M

ClientSampleId :

DABT3

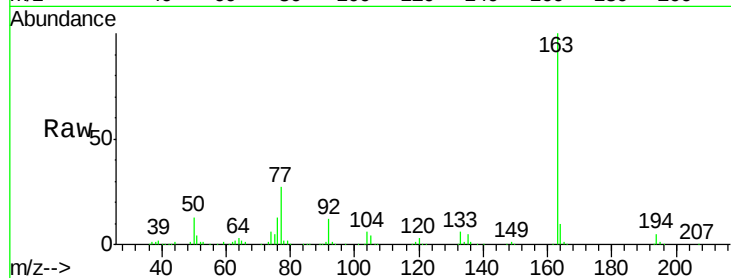

Tgt Ion:	163	Resp:	429367
Ion	Ratio	Lower	Upper
163	100		
194	4.6	3.0	4.6
164	9.6	8.6	12.8

