

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030117\
 Data File : BM009045.D
 Acq On : 01 Mar 2017 11:35
 Operator : SJ/MA
 Sample : PB97222BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK22

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM022317.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.357	42	46	53	rVB	70513	93155	1.92%	0.182%
2	7.051	667	674	682	rBV	1023931	1594723	32.90%	3.113%
3	7.228	698	704	714	rBV	745116	1149566	23.72%	2.244%
4	7.428	731	738	746	rBV	981610	1538731	31.74%	3.003%
5	7.898	811	818	826	rBV	740948	1154395	23.81%	2.253%
6	8.592	929	936	945	rBV	1128116	1809547	37.33%	3.532%
7	9.063	1007	1016	1026	rBV	939737	1549054	31.96%	3.024%
8	9.781	1131	1138	1146	rBV	755795	1249336	25.77%	2.439%
9	10.310	1221	1228	1241	rBV	1103459	1851107	38.19%	3.613%
10	10.698	1287	1294	1303	rVB	896886	1536701	31.70%	3.000%
11	10.839	1311	1318	1326	rBV	1043905	1806115	37.26%	3.525%
12	13.939	1834	1845	1855	rBV	1844012	2607710	53.80%	5.090%
13	14.233	1887	1895	1901	rBV	1982904	2893154	59.69%	5.647%
14	14.539	1941	1947	1955	rVB2	1304572	1951209	40.25%	3.809%
15	14.721	1972	1978	1994	rBV	938468	1403611	28.96%	2.740%
16	15.527	2109	2115	2128	rVB	2611292	3753104	77.43%	7.326%
17	15.645	2128	2135	2147	rBV	814348	1117219	23.05%	2.181%
18	17.280	2407	2413	2420	rBV	1644859	2381635	49.13%	4.649%
19	17.380	2424	2430	2439	rBV2	2870675	4131145	85.22%	8.064%
20	19.309	2753	2758	2762	rBV	36264	49424	1.02%	0.096%
21	19.668	2814	2819	2828	rBV	3543058	4846775	99.99%	9.460%
22	21.450	3117	3122	3127	rBV	2408801	3060224	63.13%	5.973%
23	23.650	3489	3496	3506	rVB2	2488112	4847352	100.00%	9.462%
24	23.803	3515	3522	3529	rBV	1452002	2856825	58.94%	5.576%


Sum of corrected areas: 51231817

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030117\
Data File : BM009045.D
Acq On : 01 Mar 2017 11:35
Operator : SJ/MA
Sample : PB97222BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK22

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM022317.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

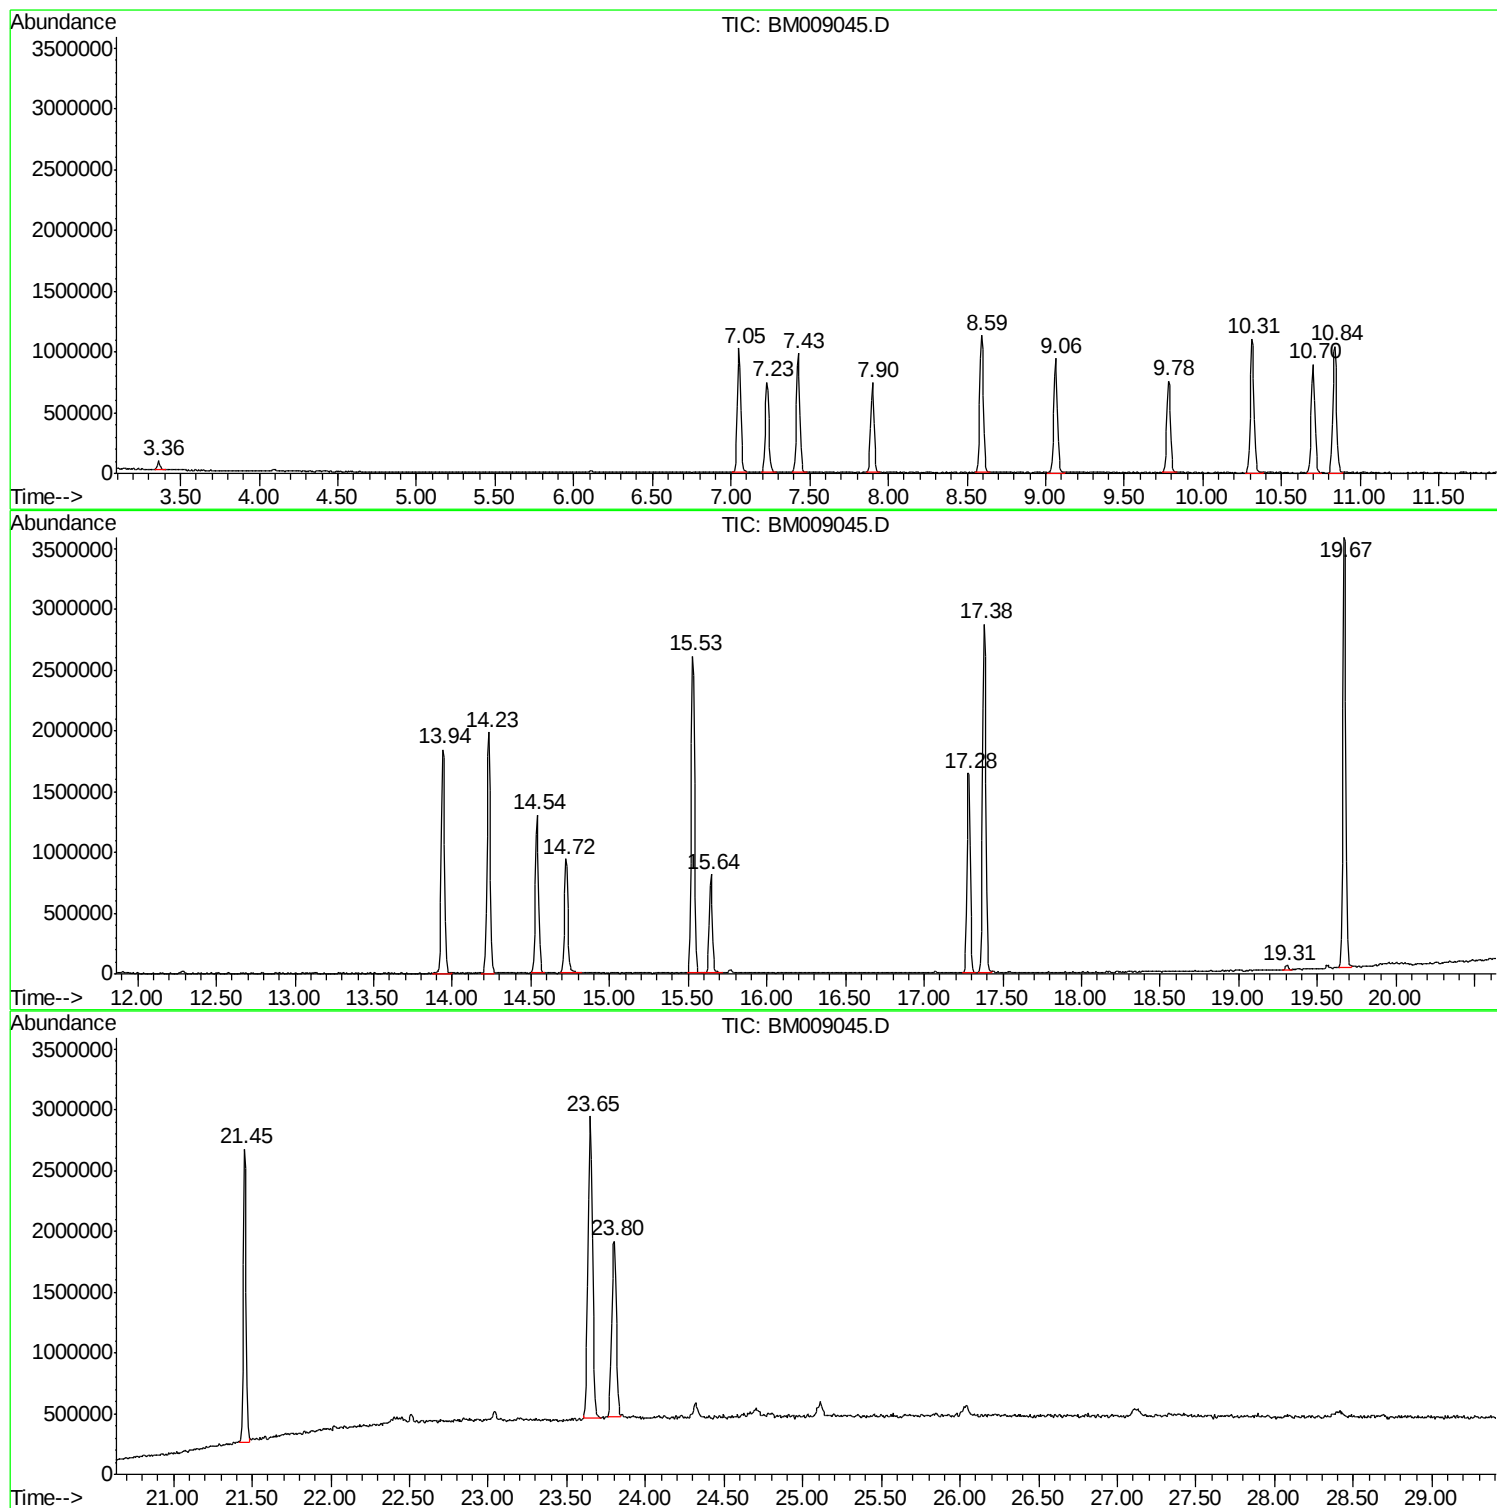

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030117\
Data File : BM009045.D
Acq On : 01 Mar 2017 11:35
Operator : SJ/MA
Sample : PB97222BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK22

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM022317.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030117\
Data File : BM009045.D
Acq On : 01 Mar 2017 11:35
Operator : SJ/MA
Sample : PB97222BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK22

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM022317.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc