

Data Path : Z:\HPCHEM1\BNA_M\Data\BM030118\

Data File : BM014445.D

Acq On : 01 Mar 2018 22:35

Operator : SJ/JU

Sample : J1678-11

Misc :

ALS Vial : 9 Sample Multiplier: 1

Quant Time: Mar 02 11:20:35 2018

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM021418.M

Quant Title : SVOA CALIBRATION

QLast Update : Thu Mar 01 03:03:26 2018

Response via : Initial Calibration

Instrument :

BNA_M



ClientSampleId :

BE5W1

Manual Integrations
APPROVED

Sohil

3/2/2018 3:32:05 PM

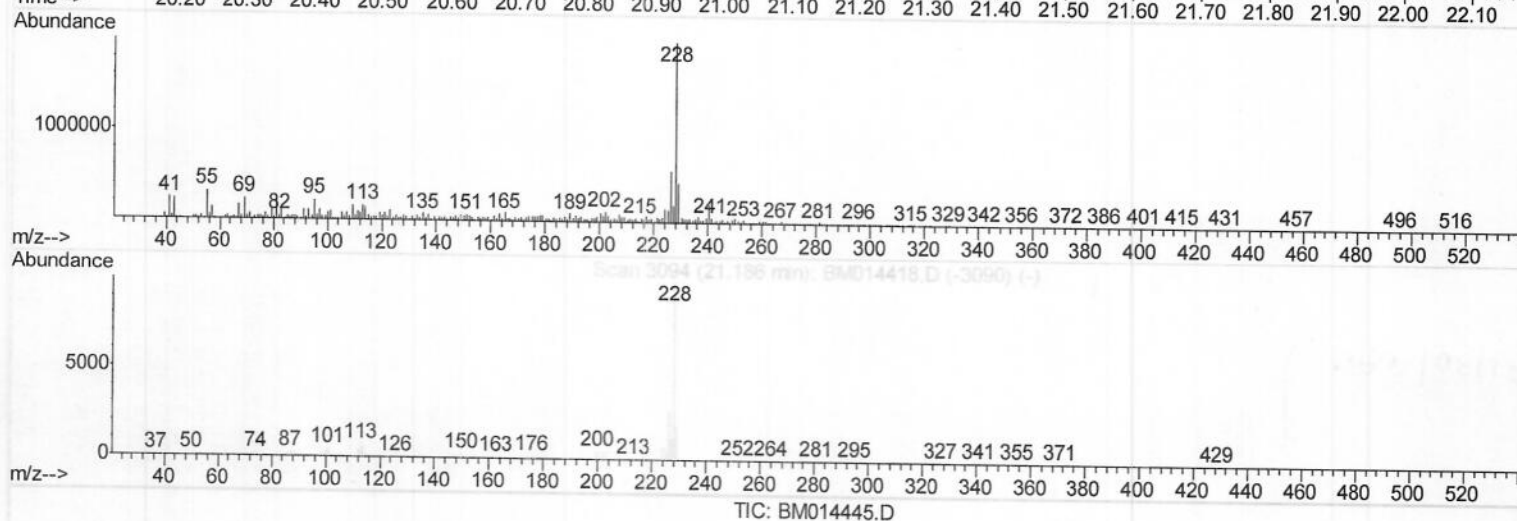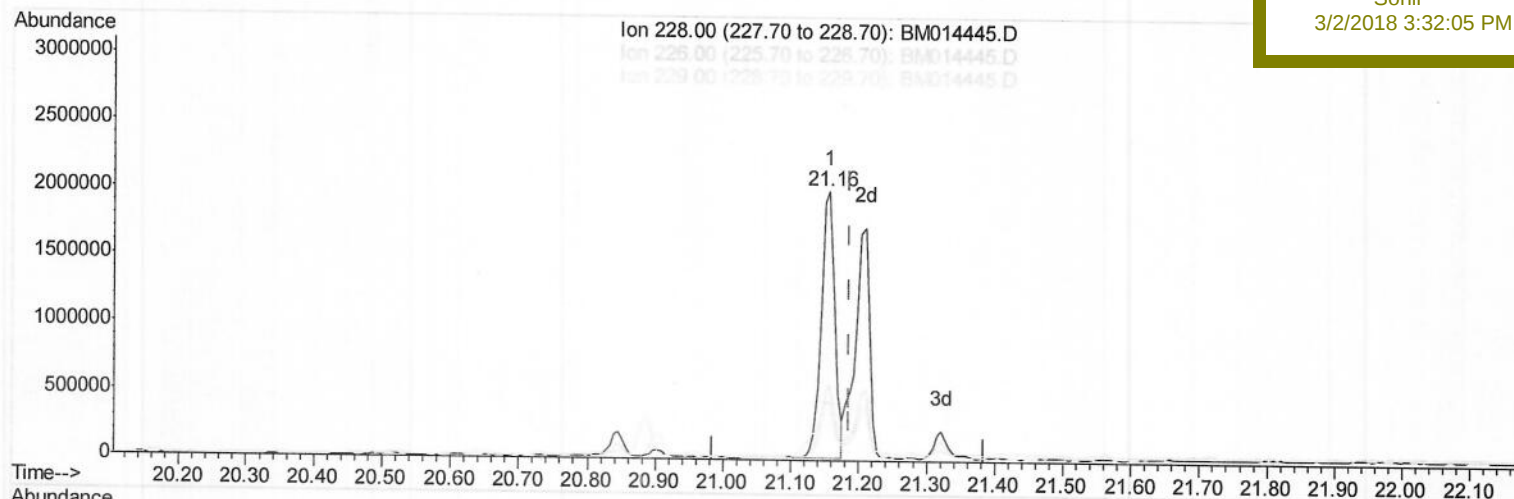

(82) Chrysene

21.156min (-0.029) 70.56ng/ul

response 2741090

Ion	Exp%	Act%
228.00	100	100
226.00	29.30	28.51
229.00	19.40	22.03
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM030118\
 Data File : BM014445.D
 Acq On : 01 Mar 2018 22:35
 Operator : SJ/JU
 Sample : J1678-11
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Quant Time: Mar 02 11:20:35 2018
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM021418.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 01 03:03:26 2018
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 BE5W1

Manual Integrations
 APPROVED

Sohil
 3/2/2018 3:32:05 PM

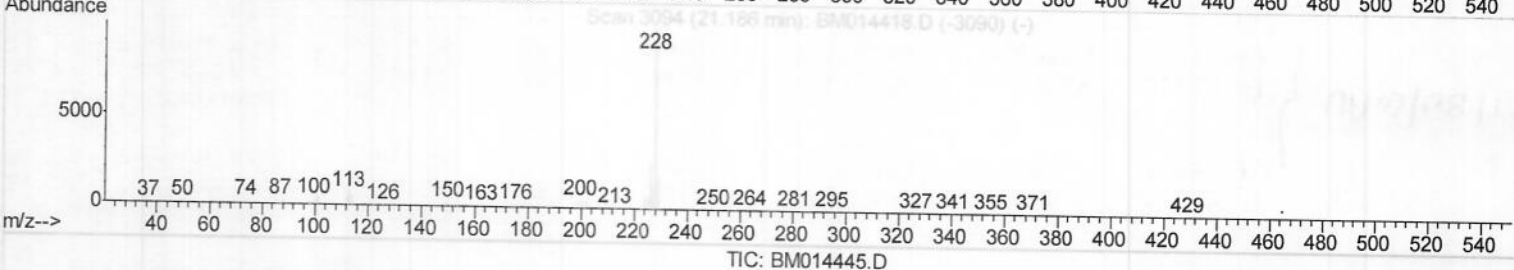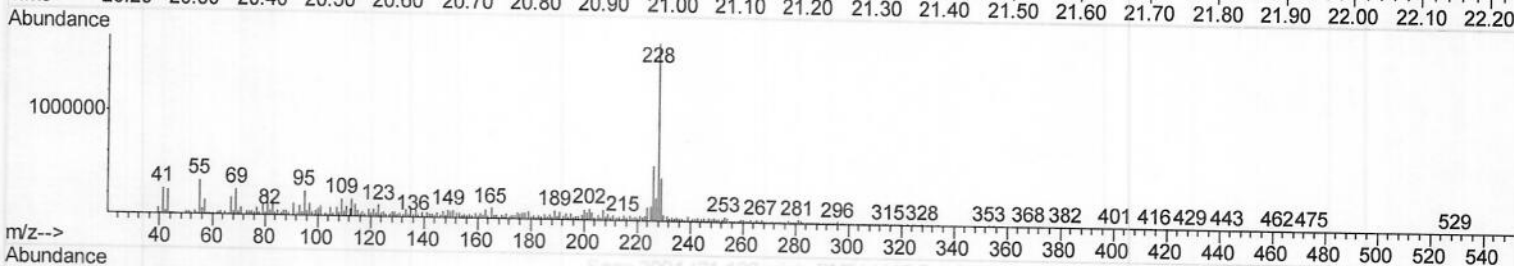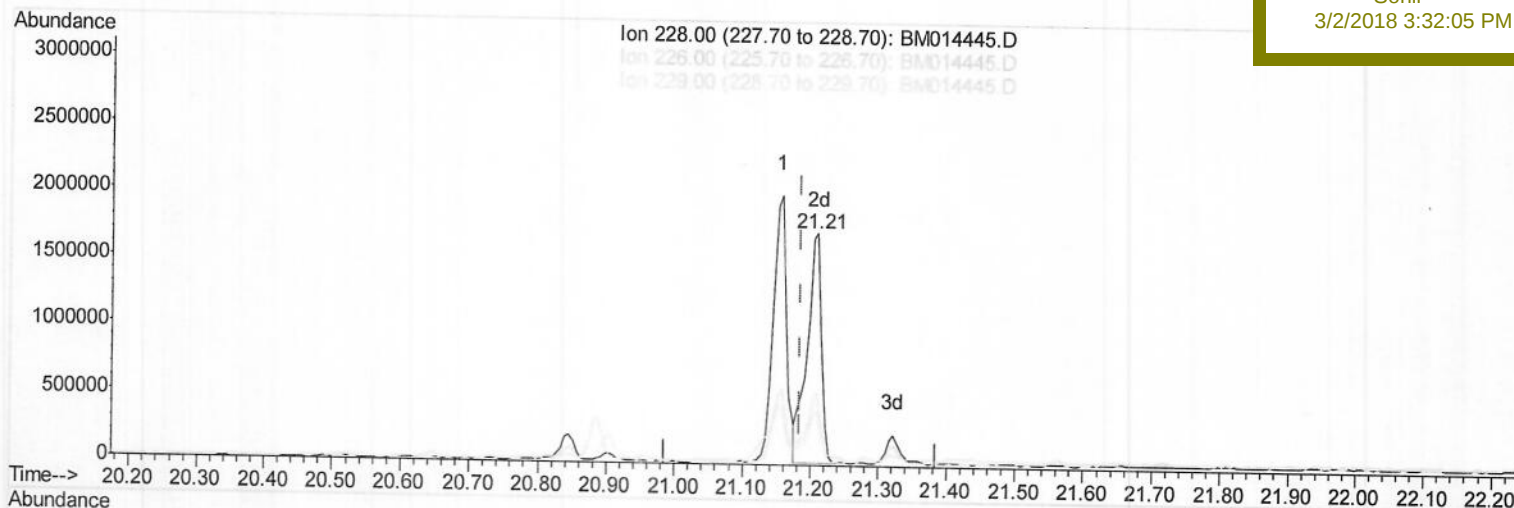

(82) Chrysene

21.209min (+0.024) 65.46ng/ul m) JU 03/02/18

response 2543181

Ion	Exp%	Act%
228.00	100	100
226.00	29.30	31.09
229.00	19.40	23.98#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_M\Data\BM030118\

Data File : BM014445.D

Acq On : 01 Mar 2018 22:35

Operator : SJ/JU

Sample : J1678-11

Misc :

ALS Vial : 9 Sample Multiplier: 1

Quant Time: Mar 02 11:20:35 2018

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM021418.M

Quant Title : SVOA CALIBRATION

QLast Update : Thu Mar 01 03:03:26 2018

Response via : Initial Calibration

Instrument :

BNA_M




ClientSampleId :

BE5W1

Manual Integrations
APPROVED

Sohil

3/2/2018 3:32:05 PM

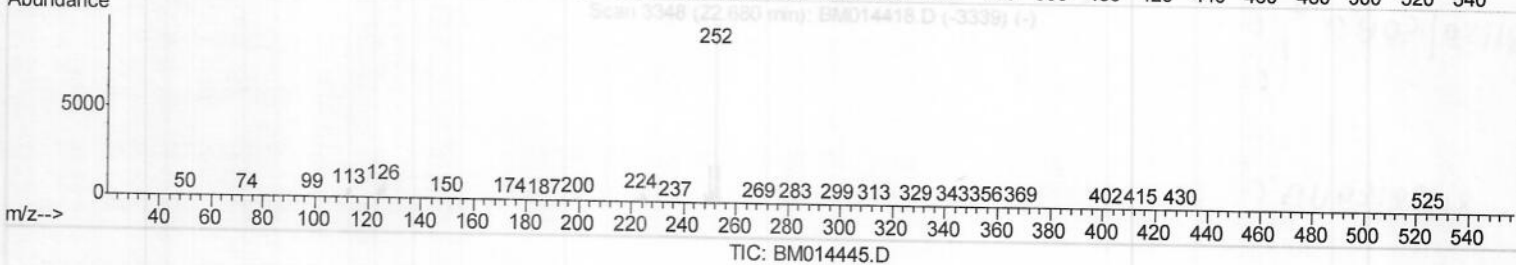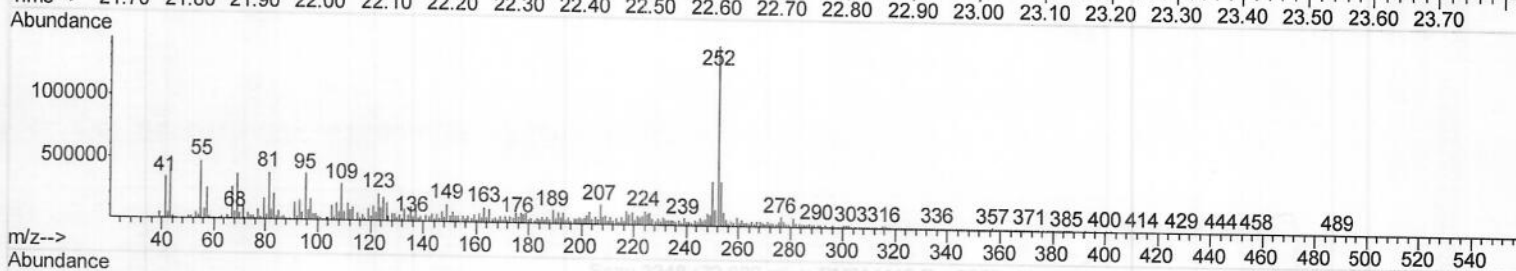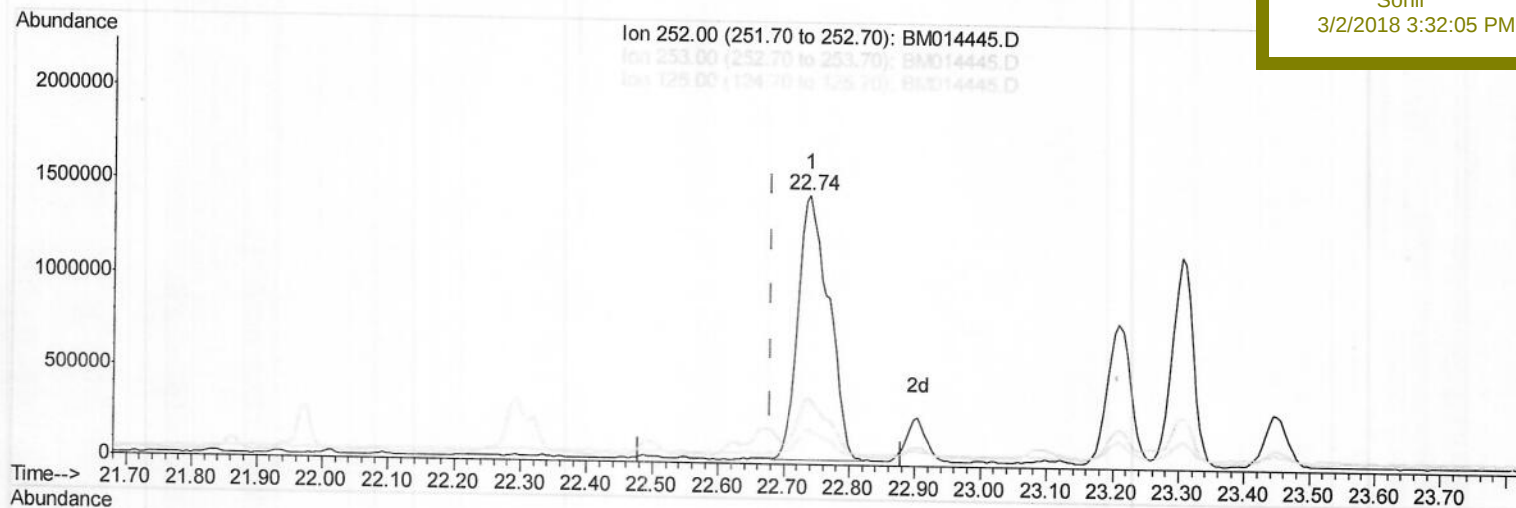

(85) Benzo(b)fluoranthene

22.739min (+0.059) 107.12ng/ul

response 4688667

Ion Exp% Act%

252.00 100 100

253.00 22.40 25.00

125.00 4.50 13.26#

0.00 0.00 0.00

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA_M\Data\BM030118\

Data File : BM014445.D

Acq On : 01 Mar 2018 22:35

Operator : SJ/JU

Sample : J1678-11

Misc :

ALS Vial : 9 Sample Multiplier: 1

Quant Time: Mar 02 11:20:35 2018

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM021418.M

Quant Title : SVOA CALIBRATION

QLast Update : Thu Mar 01 03:03:26 2018

Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :



BE5W1

Manual Integrations

APPROVED

Sohil

3/2/2018 3:32:05 PM

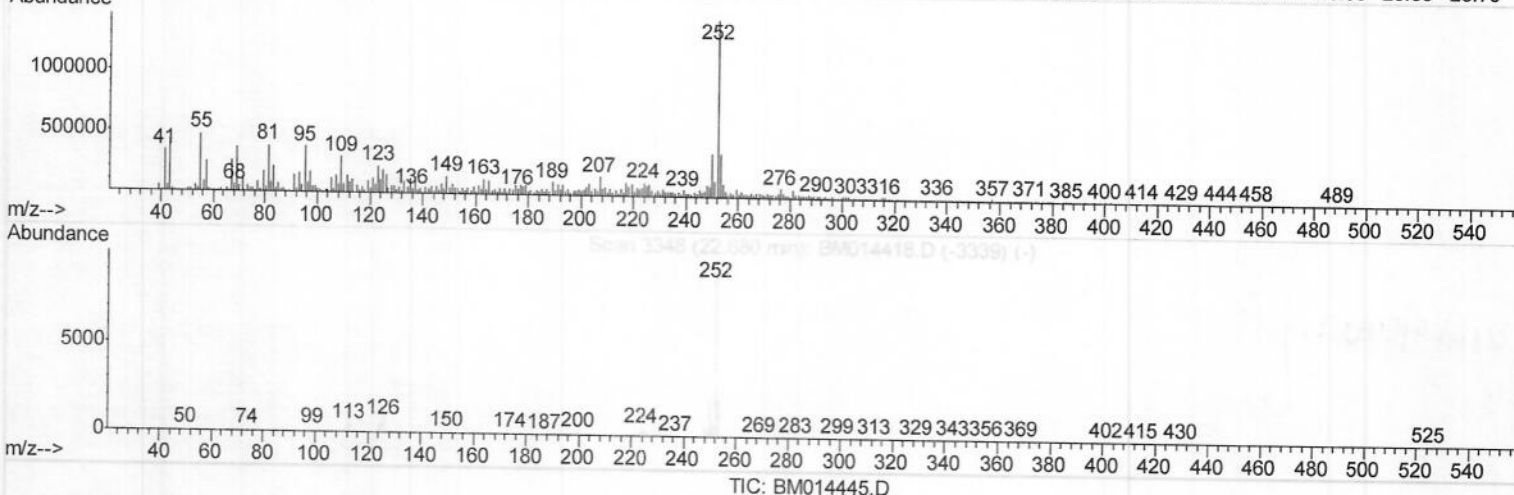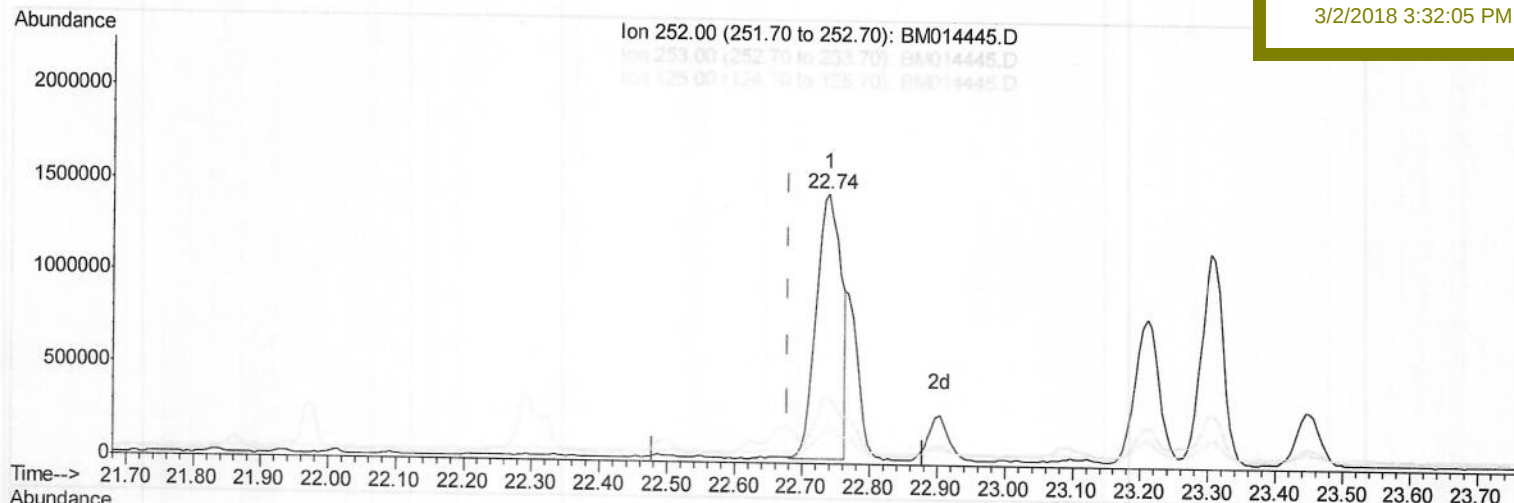

(85) Benzo(b)fluoranthene

22.739min (+0.059) 84.18ng/ul m>JU 03/09/18

response 3684628

Ion	Exp%	Act%
252.00	100	100
253.00	22.40	25.00
125.00	4.50	13.26#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\Data\BM030118\
 Data File : BM014445.D
 Acq On : 01 Mar 2018 22:35
 Operator : SJ/JU
 Sample : J1678-11
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Quant Time: Mar 02 11:20:35 2018
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM021418.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 01 03:03:26 2018
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 BE5W1

Manual Integrations
 APPROVED

Sohil
 3/2/2018 3:32:05 PM

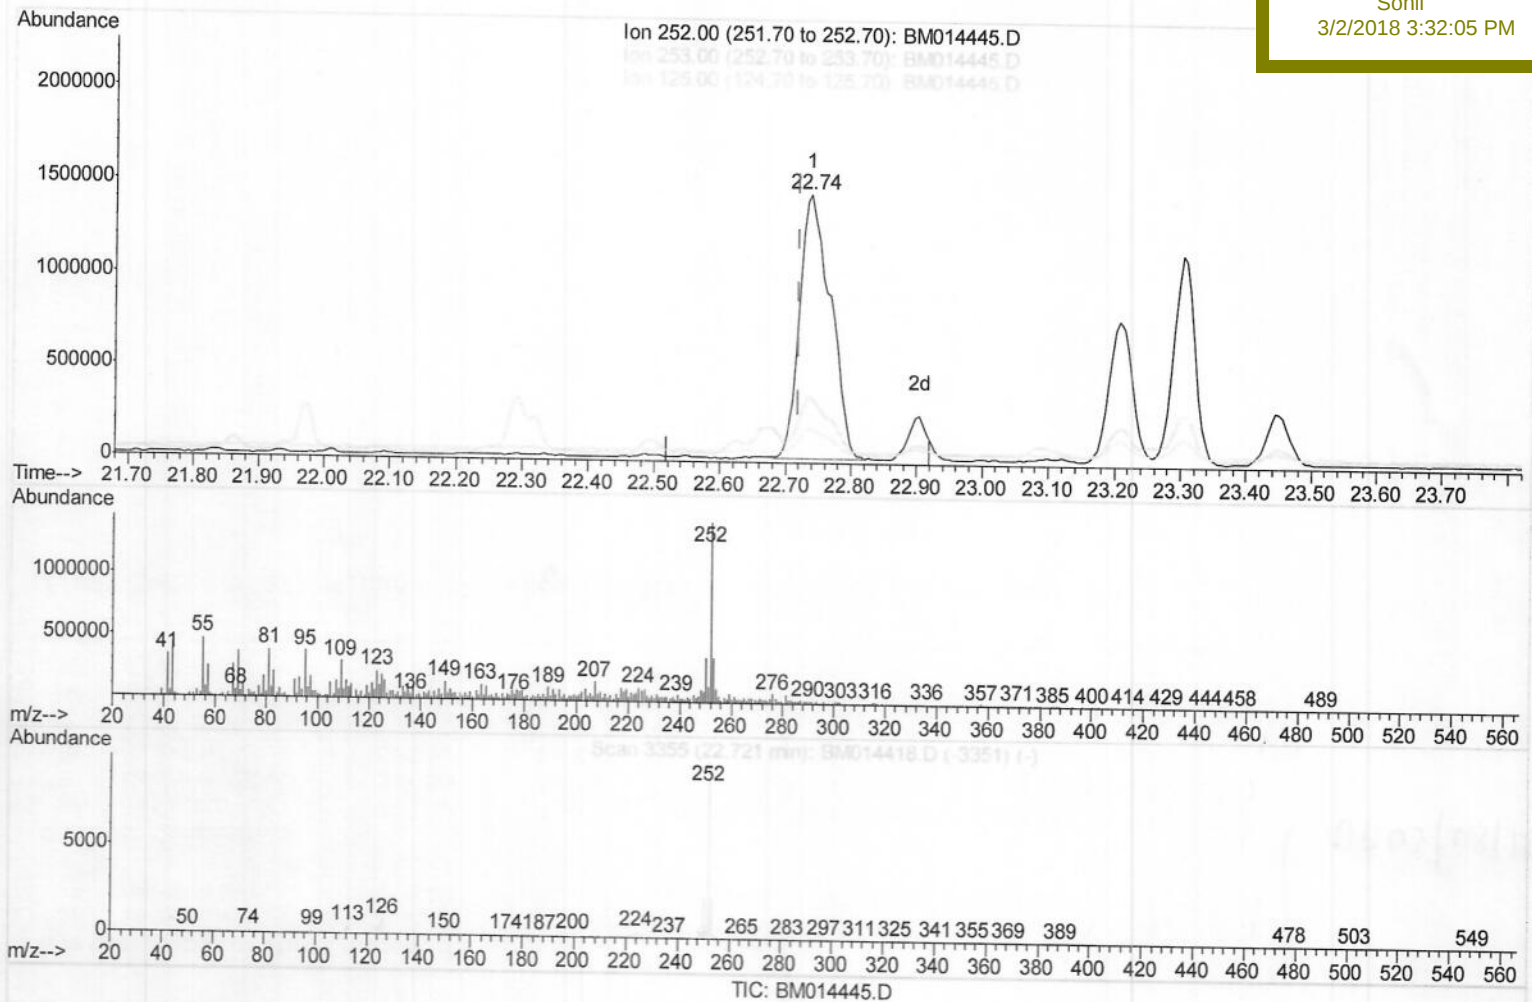

(86) Benzo(k)fluoranthene

22.739min (+0.018) 112.67ng/ul

response 4688667

Ion Exp% Act%

252.00 100 100

253.00 21.40 25.00

125.00 4.30 13.26#

0.00 0.00 0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM030118\
 Data File : BM014445.D
 Acq On : 01 Mar 2018 22:35
 Operator : SJ/JU
 Sample : J1678-11
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Quant Time: Mar 02 11:20:35 2018
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM021418.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 01 03:03:26 2018
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 BE5W1

Manual Integrations
 APPROVED

Sohil
 3/2/2018 3:32:05 PM

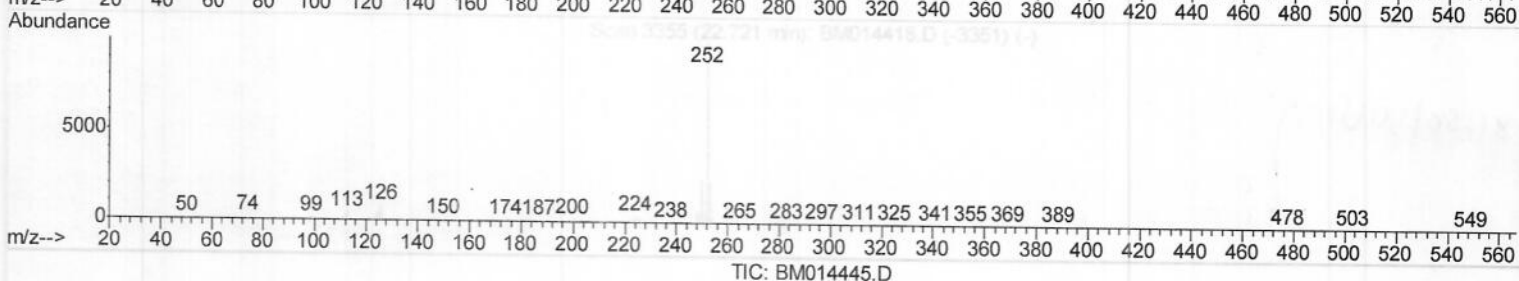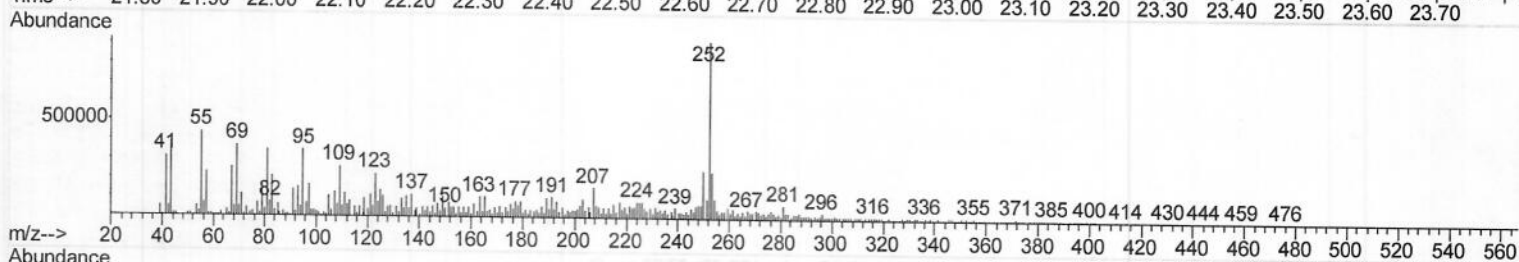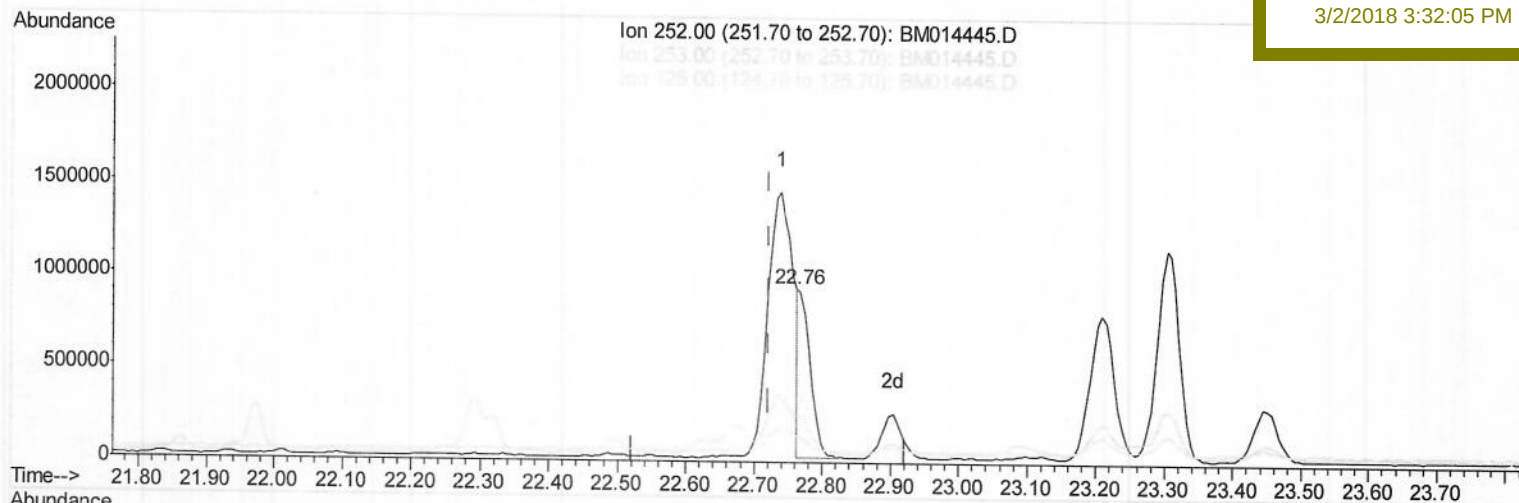

(86) Benzo(k)fluoranthene

22.762min (+0.041) 24.65ng/ul m 500309118

response 1025889

Ion	Exp%	Act%
252.00	100	100
253.00	21.40	26.37#
125.00	4.30	15.38#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_M\Data\BM030118\

Data File : BM014445.D

Acq On : 01 Mar 2018 22:35

Operator : SJ/JU

Sample : J1678-11

Misc :

ALS Vial : 9 Sample Multiplier: 1

Quant Time: Mar 02 11:20:35 2018

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM021418.M

Quant Title : SVOA CALIBRATION

QLast Update : Thu Mar 01 03:03:26 2018

Response via : Initial Calibration

Instrument :

BNA_M


ClientSampleId :

BE5W1

Manual Integrations
APPROVED

Sohil

3/2/2018 3:32:05 PM

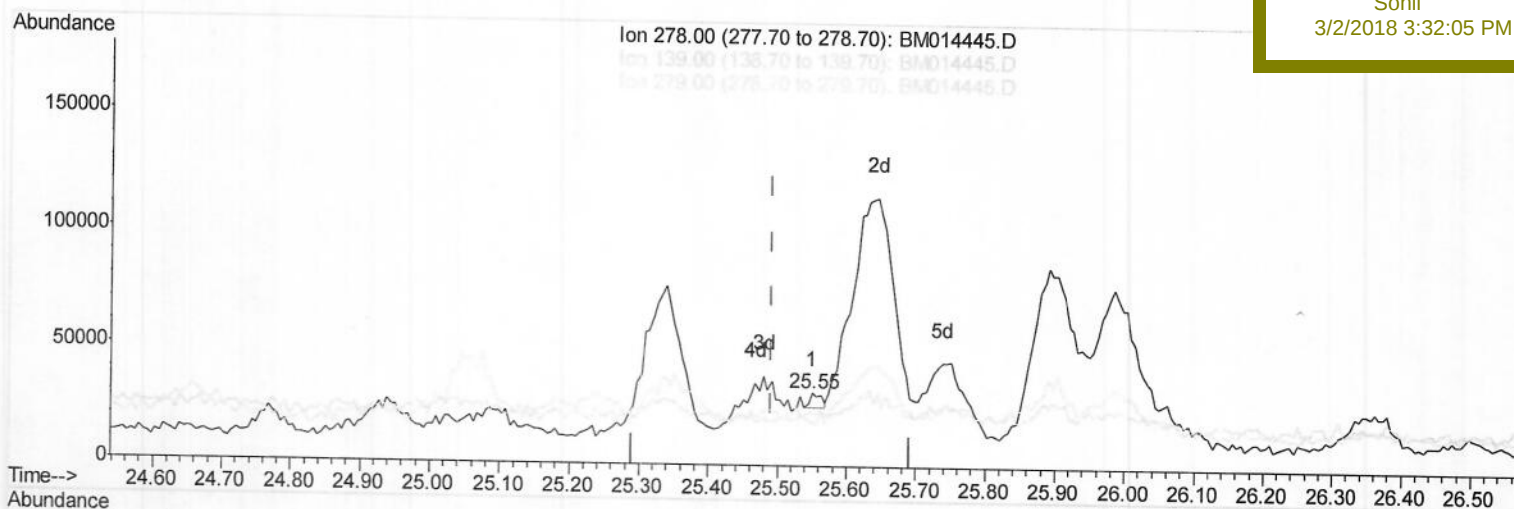

(90) Dibenzo(a,h)anthracene

25.550min (+0.059) 0.20ng/ul

response 6458

Ion Exp% Act%

278.00 100 100

139.00 7.30 61.30#

279.00 23.20 76.26#

0.00 0.00 0.00

Data Path : Z:\HPCHEM1\BNA_M\Data\BM030118\

Data File : BM014445.D

Acq On : 01 Mar 2018 22:35

Operator : SJ/JU

Sample : J1678-11

Misc :

ALS Vial : 9 Sample Multiplier: 1

Quant Time: Mar 02 11:20:35 2018

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM021418.M

Quant Title : SVOA CALIBRATION

QLast Update : Thu Mar 01 03:03:26 2018

Response via : Initial Calibration

Instrument :

BNA_M




ClientSampleId :

BE5W1

Manual Integrations
APPROVED

Sohil

3/2/2018 3:32:05 PM

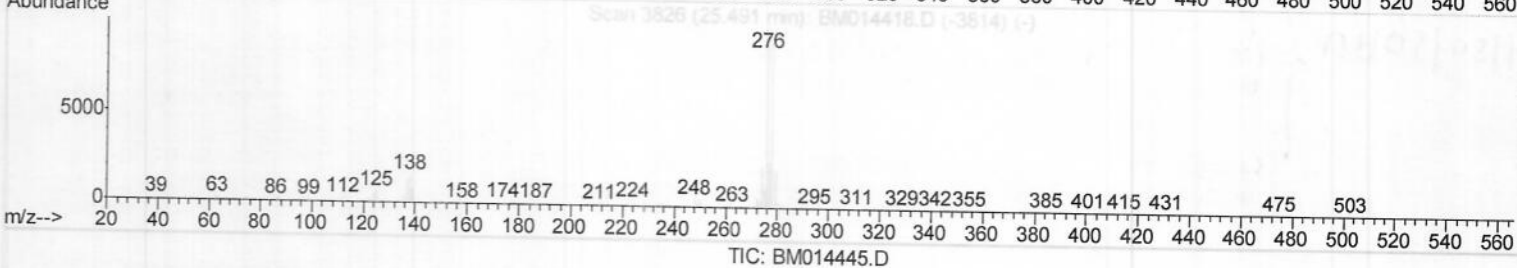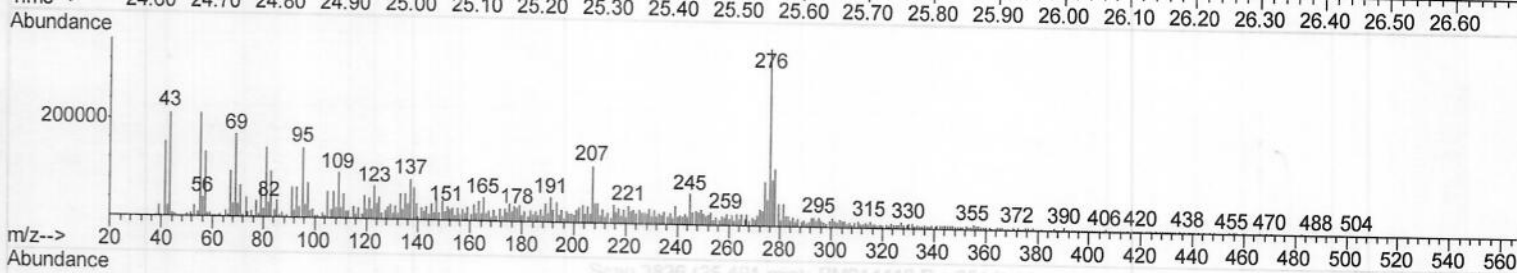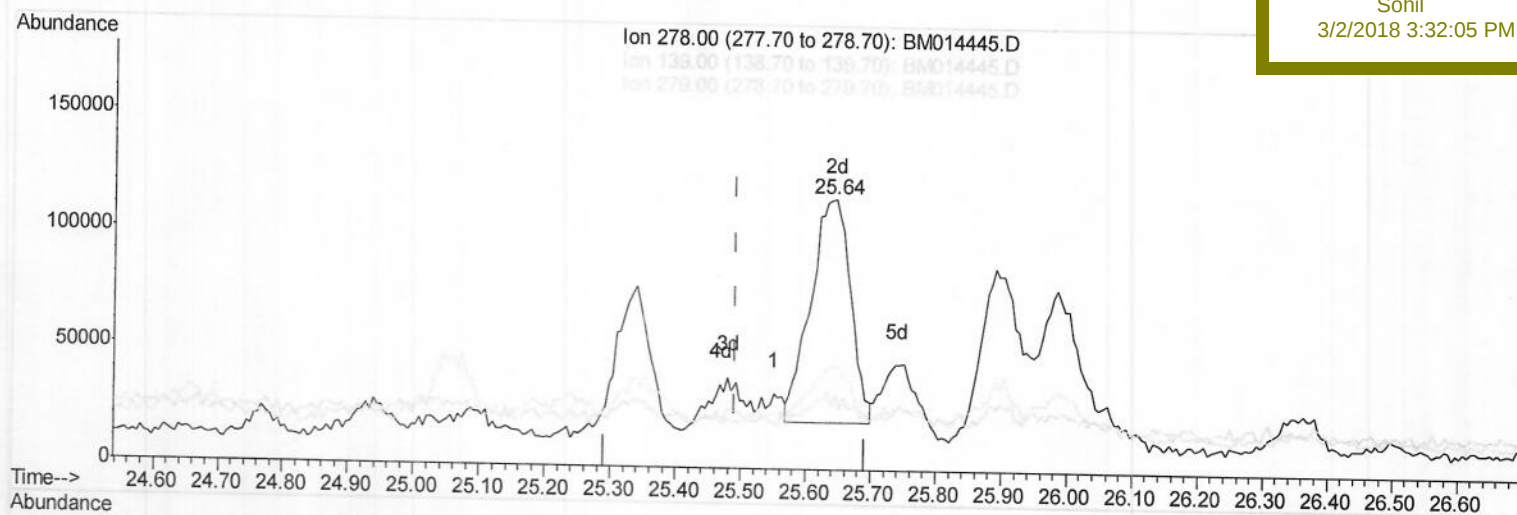

(90) Dibenzo(a,h)anthracene

25.644min (+0.153) 12.88ng/ul m 5 J1678-11

response 406190

Ion Exp% Act%

278.00 100 100

139.00 7.30 27.95#

279.00 23.20 38.29#

0.00 0.00 0.00

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA M\DATA\BM030118\
 Data File : BM014445.D
 Acq On : 01 Mar 2018 22:35
 Operator : SJ/JU
 Sample : J1678-11
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 Client Sample Id :
 BE5W1

Quant Time: Mar 08 14:09:19 2018
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM021418.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 01 03:03:26 2018
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Sohil
 3/2/2018 3:32:05 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.51	152	57333	20.00	ng/ul	0.00
18) Naphthalene-d8	10.28	136	300405	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.17	164	222655	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.94	188	602168	20.00	ng/ul	0.00
75) Chrysene-d12	21.17	240	667255	20.00	ng/ul	0.02
83) Perylene-d12	23.40	264	653692	20.00	ng/ul	0.08

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.08	96	3970	2.96	ng/uL	0.00
5) Phenol-d5	6.72	99	169324	34.94	ng/ul	0.00
7) Bis-(2-Chloroethyl) ether-d	6.86	67	87483	29.82	ng/ul	0.00
9) 2-Chlorophenol-d4	7.06	132	136991	36.87	ng/ul	0.00
13) 4-Methylphenol-d8	8.25	113	151189	35.66	ng/ul	0.00
19) Nitrobenzene-d5	8.67	128	69991	31.53	ng/ul	0.00
22) 2-Nitrophenol-d4	9.39	143	80526	35.05	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.93	165	165299	34.73	ng/ul	0.00
29) 4-Chloroaniline-d4	10.46	131	58320	12.44	ng/ul	0.01
43) Dimethylphthalate-d6	13.60	166	600862	32.68	ng/ul	0.00
46) Acenaphthylene-d8	13.86	160	835108	36.83	ng/ul	0.00
51) 4-Nitrophenol-d4	14.46	143	85166	33.55	ng/ul	0.02
57) Fluorene-d10	15.18	176	619308	37.59	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.35	200	15347	4.25	ng/ul	0.01
70) Anthracene-d10	17.04	188	1098167	37.80	ng/ul	0.00
76) Pyrene-d10	19.36	212	1241275	36.07	ng/ul	0.01
87) Benzo(a)pyrene-d12	23.26	264	1152321	36.22	ng/ul	0.07

Target Compounds						
28) Naphthalene	10.33	128	45183	2.928	ng/ul#	96
34) 2-Methylnaphthalene	11.96	142	18713	1.593	ng/ul	92
44) Dimethylphthalate	13.65	163	100295	5.532	ng/ul	98
47) Acenaphthylene	13.89	152	167084	7.797	ng/ul	99
49) Acenaphthene	14.23	153	108623	7.198	ng/ul	97
53) Dibenzofuran	14.58	168	73684	3.256	ng/ul	88
58) Fluorene	15.23	166	133805	6.850	ng/ul	99
69) Phenanthrene	16.98	178	2947933	84.968	ng/ul	99
71) Anthracene	17.07	178	706207	20.240	ng/ul	99
72) Carbazole	17.36	167	286387	9.761	ng/ul	97
73) Di-n-butylphthalate	17.92	149	2693110	71.151	ng/ul	99
74) Fluoranthene	19.02	202	5995776	144.648	ng/ul#	92
77) Pyrene	19.39	202	5047594	113.828	ng/ul#	91
80) Benzo(a)anthracene	21.16	228	2741090	65.823	ng/ul	95
82) Chrysene	21.21	228	2543181m	65.465	ng/ul	
85) Benzo(b)fluoranthene	22.74	252	3684628m	84.181	ng/ul	
86) Benzo(k)fluoranthene	22.76	252	1025889m	24.652	ng/ul	
88) Benzo(a)pyrene	23.30	252	2534696	64.804	ng/ul#	92
89) Indeno(1,2,3-cd)pyrene	25.66	276	1489899	39.255	ng/ul#	90
90) Dibenzo(a,h)anthracene	25.64	278	406190m	12.880	ng/ul	
91) Benzo(a,h,i)perylene	26.34	276	1243596	40.447	ng/ul#	88

JV03109108

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA M\DATA\BM030118\
Data File : BM014445.D
Acq On : 01 Mar 2018 22:35
Operator : SJ/JU
Sample : J1678-11
Misc :
ALS Vial : 9 Sample Multiplier: 1

Quant Time: Mar 08 14:09:19 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM021418.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 01 03:03:26 2018
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
BE5W1

Manual Integrations
APPROVED

Sohil
3/2/2018 3:32:05 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)

(#) = qualifier out of range (m) = manual integration (+) = signals summed						

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA M\DATA\BM030118\

Data File : BM014445.D

Acq On : 01 Mar 2018 22:35

Operator : SJ/JU

Sample : J1678-11

Misc :

ALS Vial : 9 Sample Multiplier: 1

Quant Time: Mar 08 14:09:19 2018

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM021418.M

Quant Title : SVOA CALIBRATION

QLast Update : Thu Mar 01 03:03:26 2018

Response via : Initial Calibration

Instrument :

BNA_M


Client Sampled :

BE5W1

Manual Integrations
APPROVED

Sohil

3/2/2018 3:32:05 PM

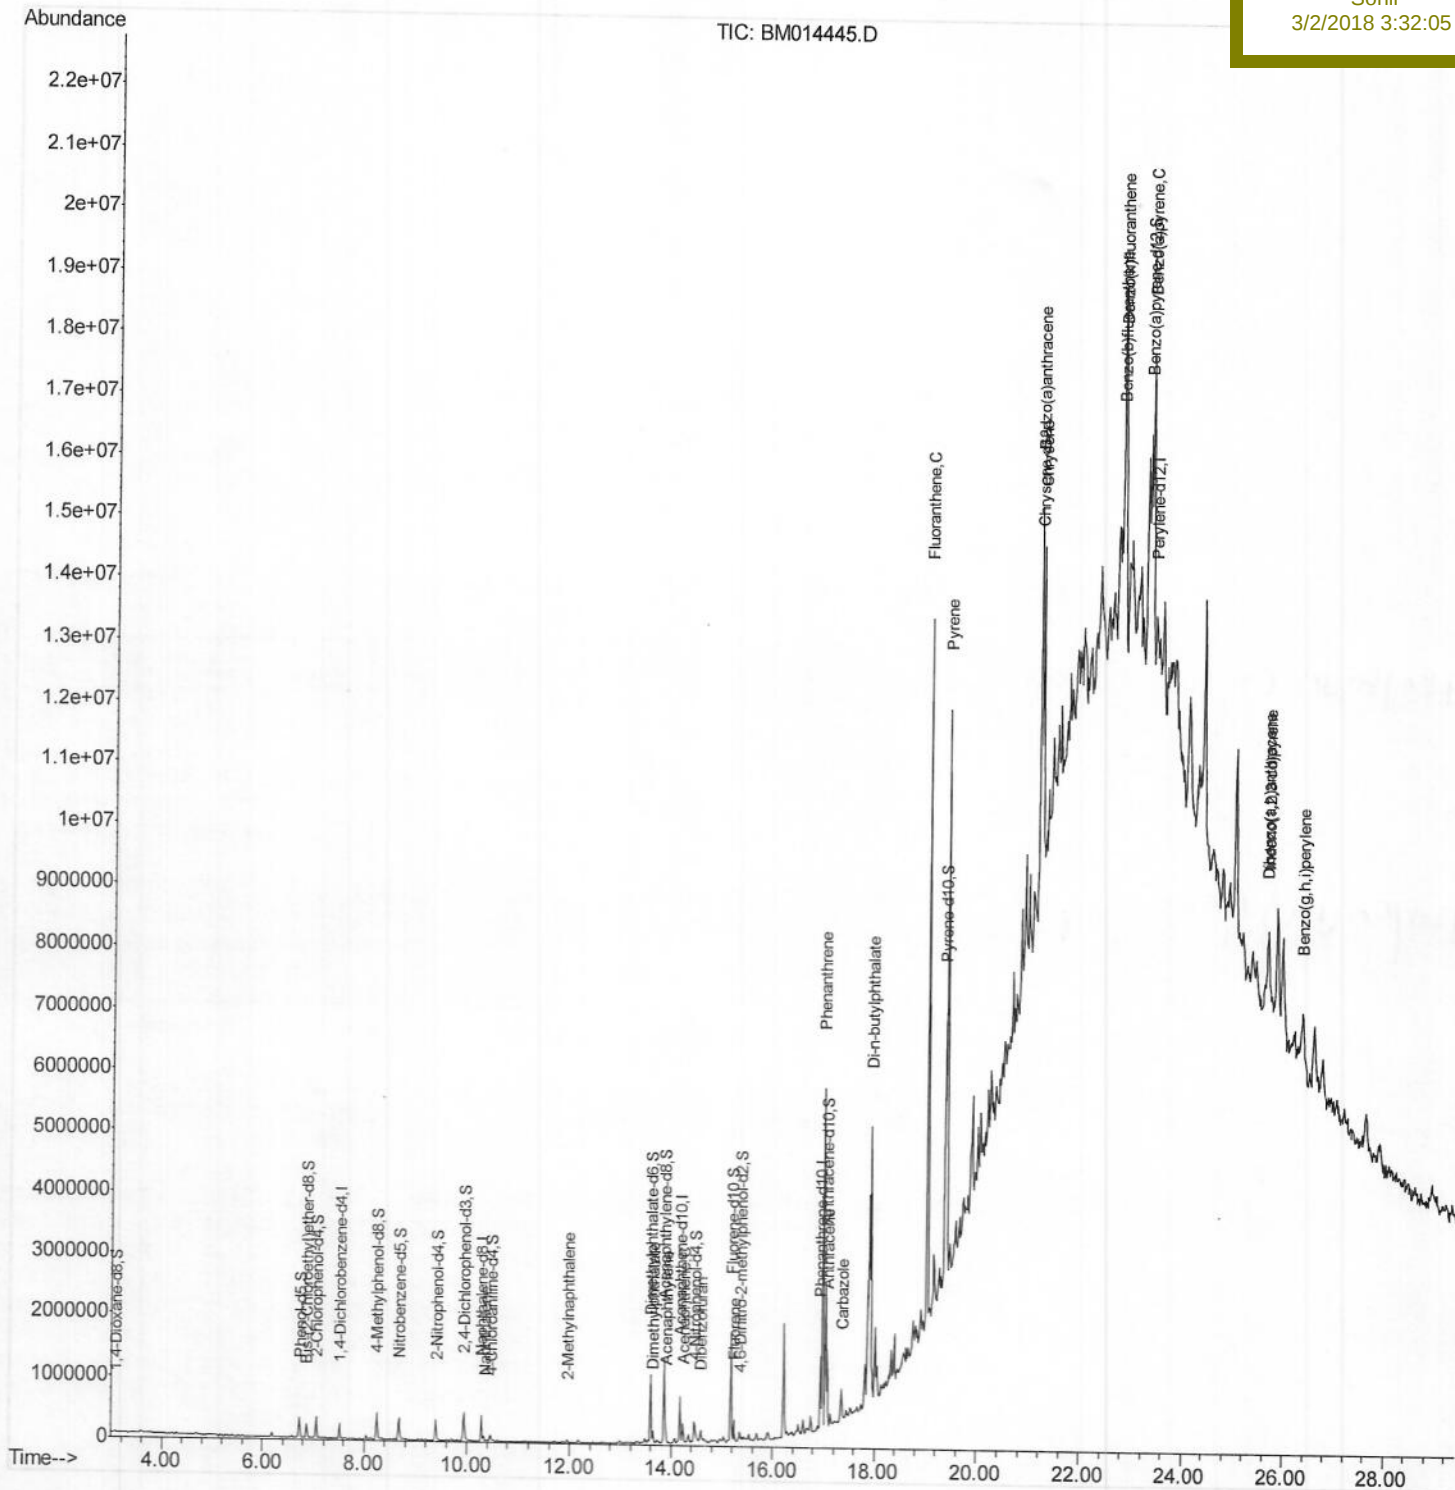

SOM-EPA-BM021418.M Thu Mar 08 14:10:05 2018

Page: 3