


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM030121\
Data File : BM028960.D
Acq On : 01 Mar 2021 12:13
Operator : CG/JU
Sample : M1482-08
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBGM6

Manual Integrations
APPROVED

mohammad
3/1/2021 4:33:22 PM

Quant Time: Mar 01 12:53:10 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM020521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 01 10:25:15 2021
Response via : Initial Calibration

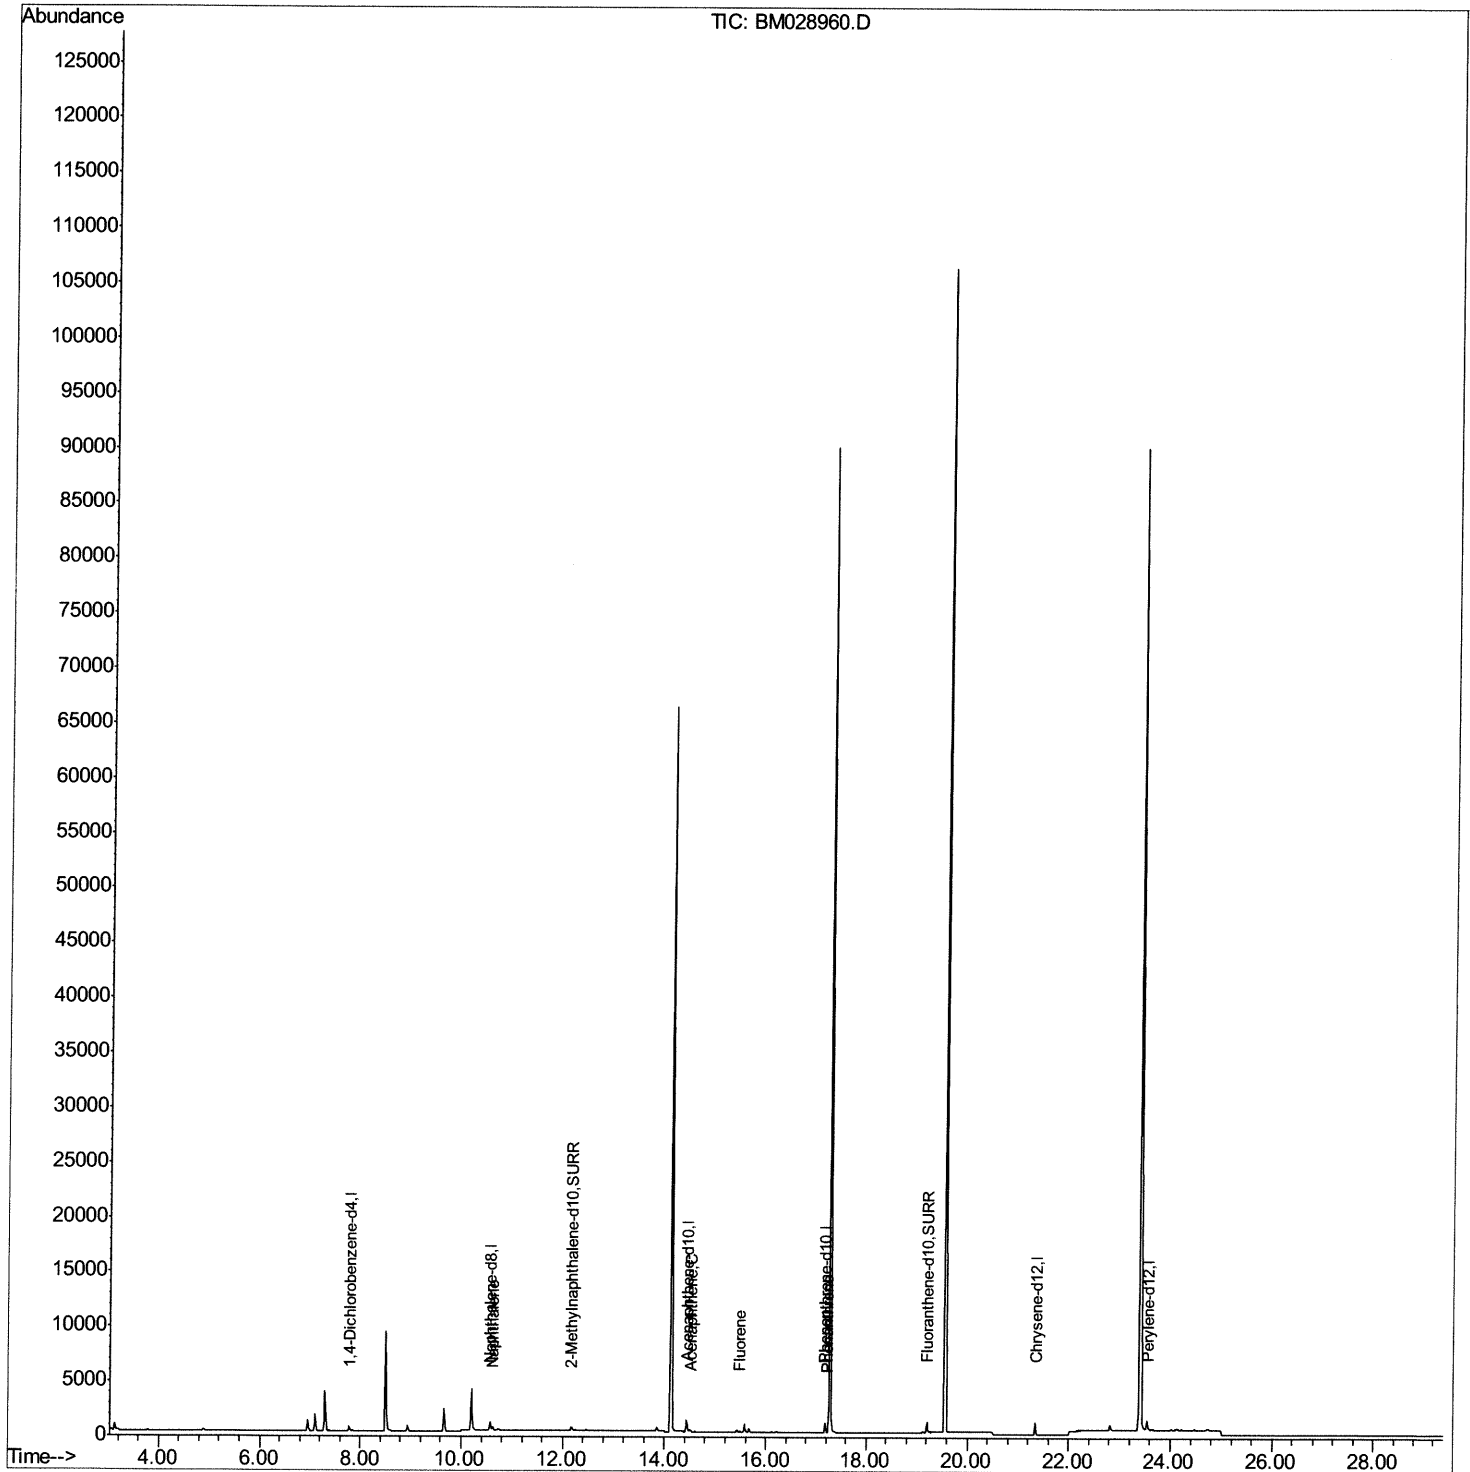

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM030121\
 Data File : BM028960.D
 Acq On : 01 Mar 2021 12:13
 Operator : CG/JU
 Sample : M1482-08
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampleId :
 DBG6

Manual Integrations
APPROVED

mohammad
 3/1/2021 4:33:22 PM

Quant Time: Mar 01 12:51:52 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM020521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 01 10:25:15 2021
 Response via : Initial Calibration

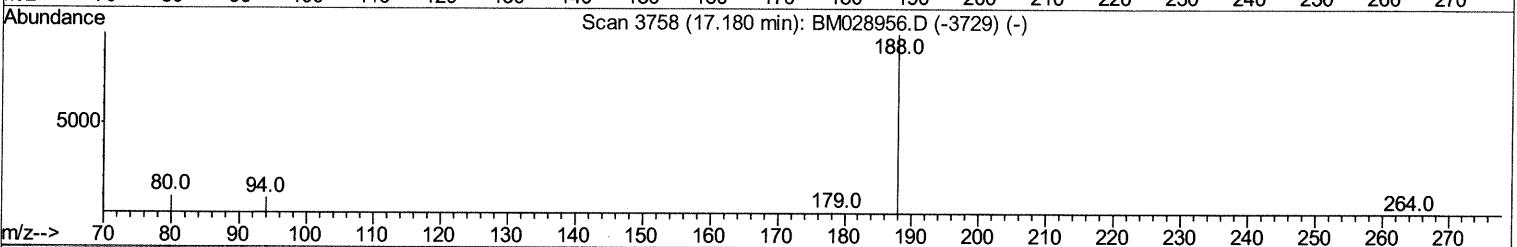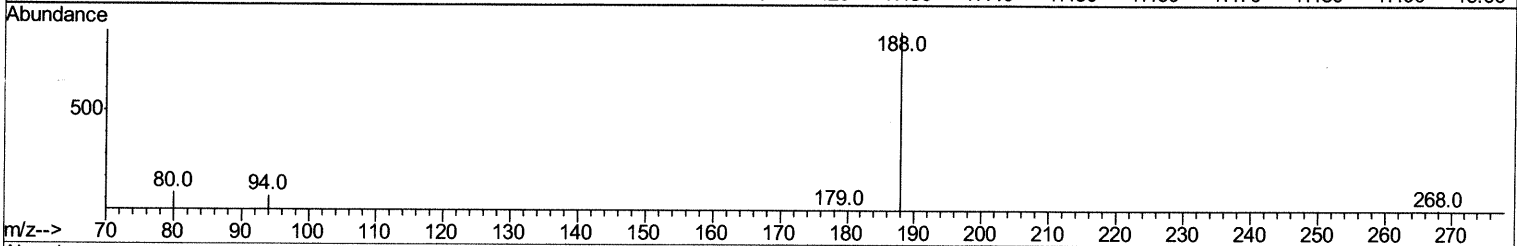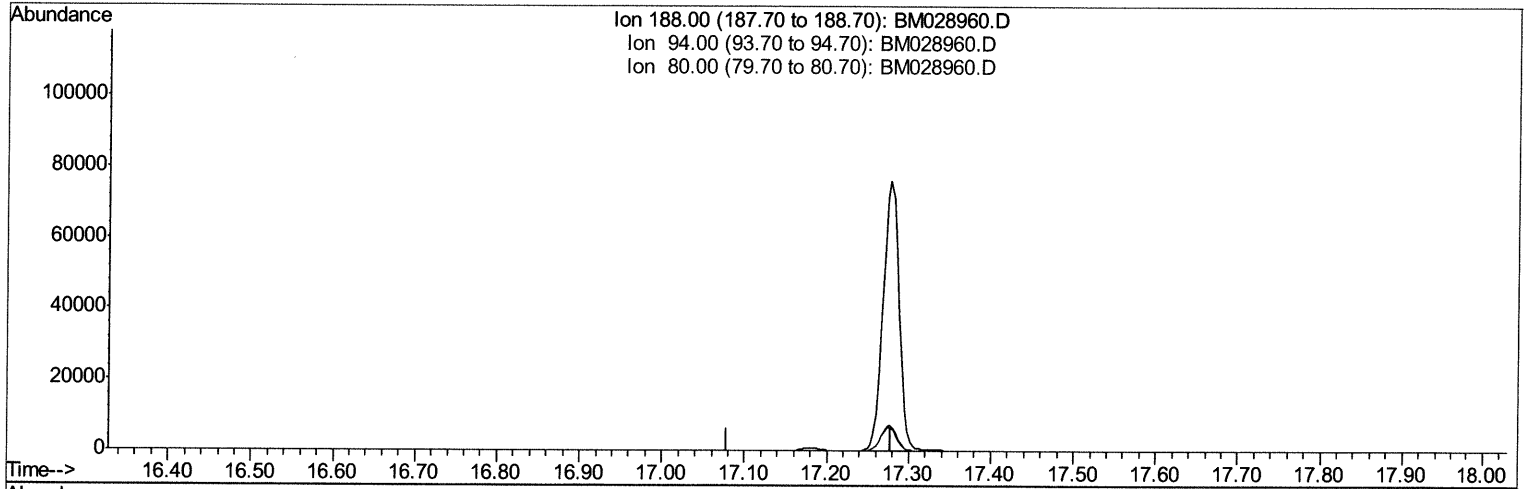

TIC: BM028960.D

(10) Phenanthrene-d10 (I)

17.180min (-17.180) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	13.50	0.00#
80.00	14.00	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM030121\
Data File : BM028960.D
Acq On : 01 Mar 2021 12:13
Operator : CG/JU
Sample : M1482-08
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBGM6

Manual Integrations
APPROVED

mohammad
3/1/2021 4:33:22 PM

Quant Time: Mar 01 12:51:52 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM020521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 01 10:25:15 2021
Response via : Initial Calibration

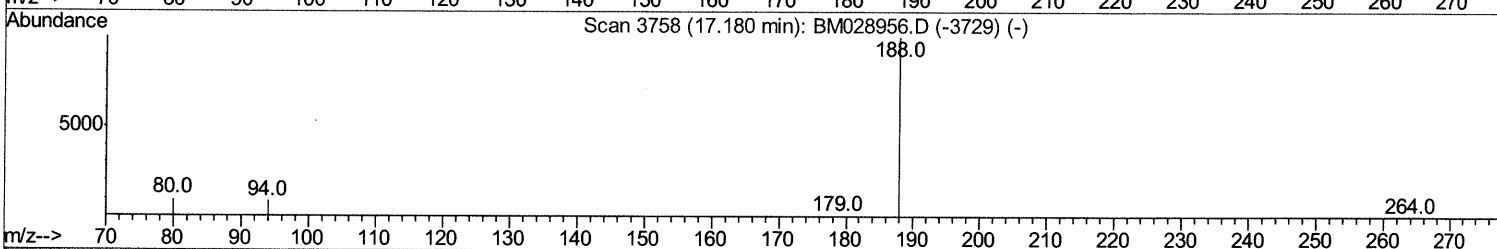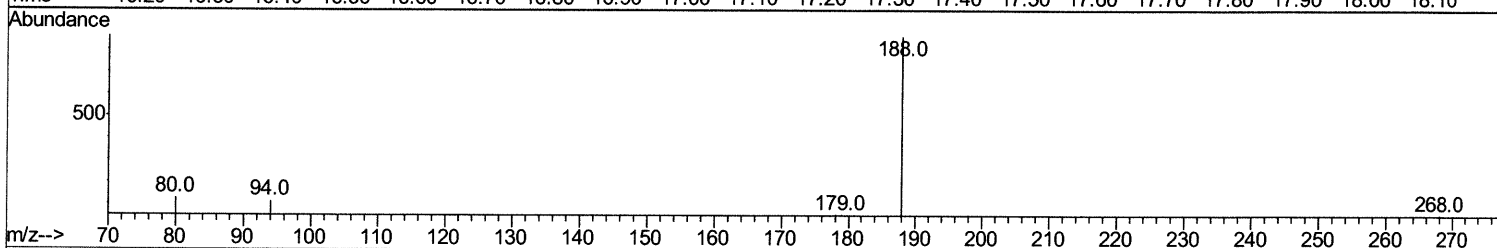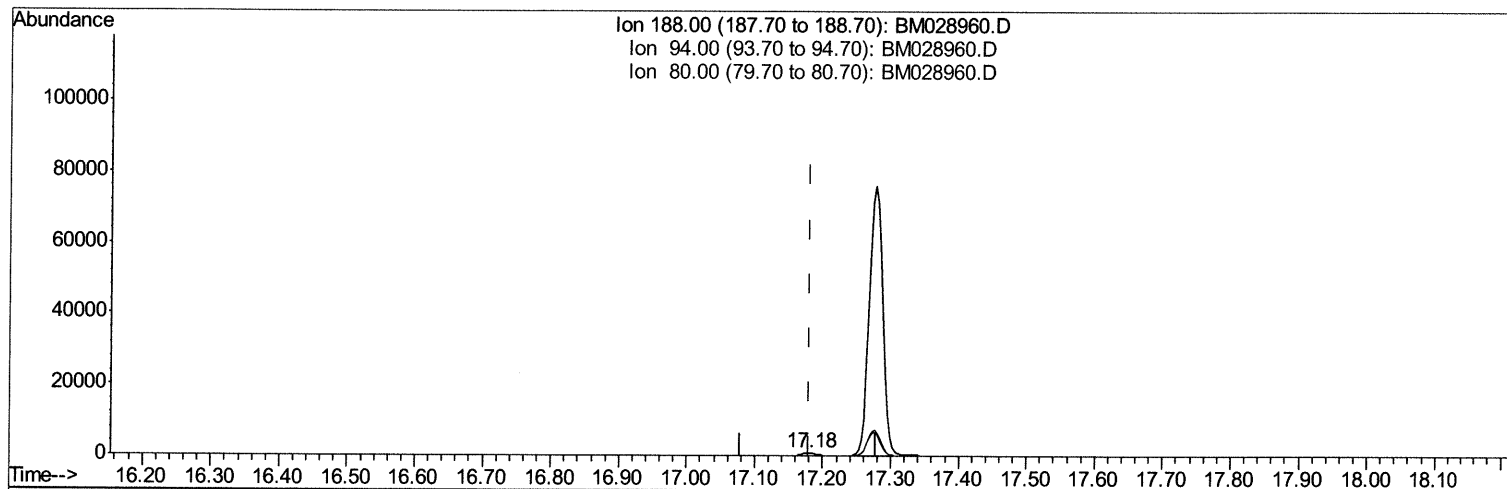

TIC: BM028960.D

(10) Phenanthrene-d10 (I)

17.180min (+0.000) 0.40ng/ul m 02/02/21 JU

response 1260

Ion	Exp%	Act%
188.00	100	100
94.00	13.50	12.89
80.00	14.00	14.40
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM030121\
 Data File : BM028960.D
 Acq On : 01 Mar 2021 12:13
 Operator : CG/JU
 Sample : M1482-08
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBG M6

Manual Integrations
 APPROVED

mohammad
 3/1/2021 4:33:22 PM

Quant Time: Mar 01 12:53:10 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM020521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 01 10:25:15 2021
 Response via : Initial Calibration

Internal Standards	R.T.	Q Ion	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	7.79	152	259	0.40	ng/ul	0.00
2) Naphthalene-d8	10.58	136	1069	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.44	164	599	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.18	188	1260m>	0.40	ng/ul>	0.00
16) Chrysene-d12	21.35	240	1060	0.40	ng/ul	0.00
20) Perylene-d12	23.54	264	1130	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.17	152	498	0.33	ng/ul	0.00
14) Fluoranthene-d10	19.20	212	1092	0.34	ng/ul	0.00
Target Compounds						
3) Naphthalene	10.63	128	392	0.147	ng/ul#	67
8) Acenaphthene	14.50	153	123	0.063	ng/ul#	91
9) Fluorene	15.49	166	67	0.031	ng/ul#	83
12) Phenanthrene	17.22	178	102	0.029	ng/ul#	30

(#) = qualifier out of range (m) = manual integration (+) = signals summed