


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM030121\
 Data File : BM028955.D
 Acq On : 01 Mar 2021 09:10
 Operator : CG/JU
 Sample : DFTPP38
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP38

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM020521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 01 10:25:15 2021

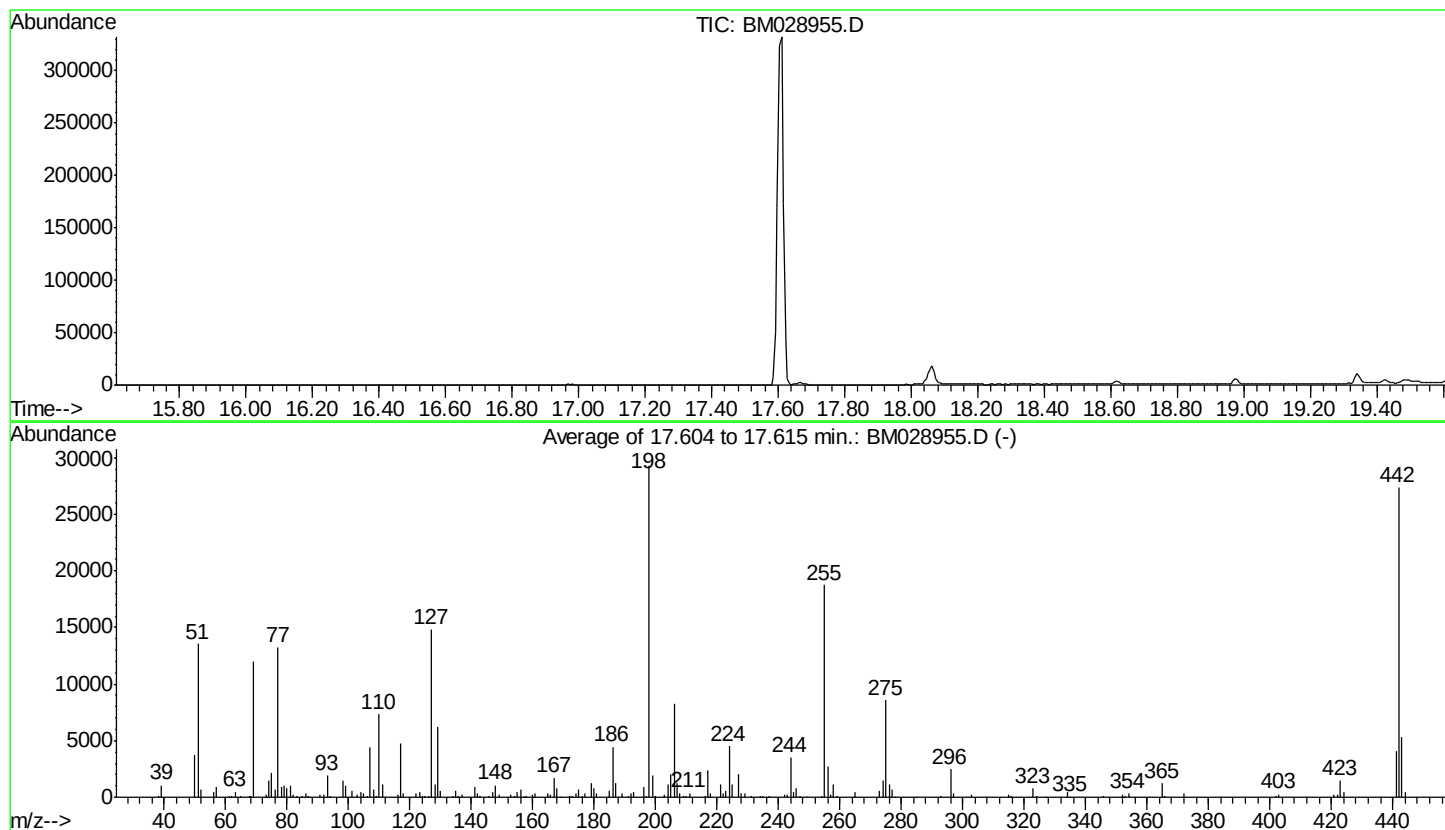

AutoFind: Scans 2485, 2486, 2487; Background Corrected with Scan 2479

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.3	13570	PASS
68	69	0.00	2	1.0	123	PASS
69	198	0.00	100	41.1	12042	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.4	14774	PASS
197	198	0.00	2	0.3	77	PASS
198	198	100	100	100.0	29309	PASS
199	198	5	9	6.6	1925	PASS
275	198	10	60	29.3	8590	PASS
365	198	1	100	4.2	1219	PASS
441	198	0.01	100	13.9	4085	PASS
442	198	50	100	93.3	27338	PASS
443	442	15	24	19.3	5289	PASS

m/z	Abundance
43.90	220.0

Instrument :
BNA_M
ClientSampleId :
DFTPP38

m/z	Abundance
38.00	281.0
39.10	1297.0
44.00	224.0
50.00	4954.0
51.00	17944.0
52.00	914.0
56.00	523.0
57.00	1232.0
61.00	209.0
62.00	255.0
63.00	610.0
65.00	247.0
68.20	370.0
69.00	15967.0
73.00	314.0
74.00	1980.0
75.00	2733.0
76.00	950.0
77.10	17056.0
78.00	1198.0
79.00	1346.0
80.00	895.0
81.00	1329.0
82.00	368.0
83.00	257.0
84.90	193.0
86.00	407.0
87.00	201.0
90.90	363.0
91.90	376.0
93.00	2278.0
94.00	195.0
98.00	1886.0
99.00	1328.0
101.00	763.0
103.00	317.0
104.00	484.0
105.00	466.0
106.00	189.0
107.00	5395.0
108.00	861.0
109.10	220.0
110.00	9304.0
111.00	1506.0
116.00	295.0
117.00	5990.0
117.90	404.0
122.00	417.0
123.00	635.0
123.90	247.0
125.00	233.0
127.00	18256.0
128.00	1550.0
129.00	7695.0
129.90	677.0
133.90	178.0
135.00	678.0
135.90	278.0
137.00	289.0
141.00	1174.0
142.00	388.0
142.90	217.0
145.90	194.0
147.00	604.0
148.00	1321.0
149.00	251.0
153.00	387.0
153.90	277.0
154.90	538.0
156.00	818.0
156.90	154.0
157.90	176.0
159.90	292.0
160.90	479.0
164.90	445.0
165.90	277.0
167.00	2068.0
167.90	867.0
169.00	166.0
171.90	170.0
172.90	260.0
174.00	517.0
175.00	760.0
176.00	189.0
176.90	392.0
178.90	1386.0
179.90	975.0
180.90	410.0
185.00	783.0
186.00	5303.0
187.00	1538.0
189.00	332.0

Instrument :
BNA_M
ClientSampleId :
DFTPP38

190.90	216.0
192.00	473.0
193.00	492.0
196.00	900.0
197.90	34640.0
198.90	2262.0
199.90	184.0
202.90	306.0
204.00	1287.0
205.00	2411.0
206.00	9564.0
207.00	1504.0
208.00	405.0
208.90	160.0
210.10	167.0
210.90	385.0
216.10	185.0
216.90	2581.0
217.90	384.0
221.00	1323.0
221.90	333.0
223.00	672.0
224.00	5329.0
225.00	1292.0
227.00	2267.0
228.00	400.0
229.00	460.0
230.90	176.0
233.90	197.0
237.00	290.0
241.90	254.0
242.90	257.0
244.00	3835.0
245.00	542.0
245.90	845.0
246.90	183.0
254.10	230.0
255.00	21376.0
256.00	3121.0
256.90	288.0
258.00	1244.0
264.90	462.0
272.90	582.0
274.00	1613.0
275.00	9285.0
276.00	1319.0
276.90	783.0
292.90	207.0
296.00	2799.0
296.90	443.0
303.00	302.0
314.90	289.0
316.00	199.0
323.00	778.0
324.00	170.0
334.00	484.0
345.90	161.0
352.00	246.0
353.00	156.0
353.90	225.0
365.00	1123.0
365.90	164.0
372.00	340.0
402.00	169.0
403.00	209.0
421.00	193.0
421.90	172.0
423.00	1266.0
424.00	431.0
441.00	3763.0
442.00	24248.0
443.00	4852.0
444.00	465.0

Instrument :
BNA_M
ClientSampleId :
DFTPP38

m/z	Abundance
38.00	235.0
39.00	1296.0
44.00	188.0
50.00	4228.0
51.00	15614.0
52.00	800.0
56.00	513.0
57.00	1014.0
60.90	215.0
61.90	229.0
63.00	644.0
65.00	227.0
67.90	254.0
69.00	13895.0
73.10	253.0
74.00	1634.0
75.00	2490.0
76.10	778.0
77.10	15590.0
78.00	1028.0
79.00	1283.0
80.00	970.0
81.00	1177.0
81.90	317.0
83.00	234.0
84.90	211.0
86.00	387.0
90.90	299.0
91.90	360.0
93.00	2347.0
98.00	1780.0
99.00	1295.0
101.00	687.0
102.90	248.0
104.00	475.0
104.90	451.0
107.00	5433.0
108.00	695.0
109.00	191.0
110.00	8806.0
111.00	1241.0
111.90	156.0
116.00	312.0
117.00	5683.0
118.00	365.0
122.00	371.0
123.00	489.0
124.00	224.0
124.90	168.0
126.20	231.0
127.00	17800.0
128.00	1242.0
129.00	7260.0
129.90	575.0
133.90	260.0
135.00	615.0
135.90	189.0
136.90	302.0
140.90	997.0
142.00	360.0
143.00	226.0
145.90	172.0
147.00	522.0
148.00	1189.0
149.00	220.0
153.00	339.0
154.00	210.0
155.00	487.0
156.00	742.0
157.90	172.0
160.00	322.0
160.90	505.0
164.90	437.0
165.90	271.0
167.00	2113.0
168.00	1012.0
172.00	222.0
173.00	242.0
173.90	428.0
175.00	814.0
176.00	233.0
177.00	351.0
178.90	1514.0
180.00	974.0
180.90	442.0
185.00	675.0
186.00	5282.0
187.00	1422.0
188.00	165.0
189.00	396.0
191.00	178.0
192.00	432.0

Instrument :
BNA_M
ClientSampleId :
DFTPP38

193.00	551.0
195.90	1087.0
197.00	231.0
197.90	35080.0
198.90	2433.0
200.00	245.0
203.00	340.0
204.00	1374.0
205.00	2359.0
206.00	10040.0
207.00	1470.0
208.00	368.0
209.00	177.0
210.00	202.0
211.00	466.0
216.00	198.0
217.00	2819.0
217.90	329.0
221.00	1295.0
221.80	414.0
223.00	564.0
224.00	5345.0
225.00	1420.0
227.00	2584.0
228.00	343.0
228.90	464.0
231.00	181.0
233.90	151.0
234.90	207.0
237.00	195.0
242.00	285.0
243.00	334.0
244.00	4169.0
245.00	581.0
245.90	938.0
246.90	224.0
249.00	167.0
255.00	22456.0
256.00	3302.0
257.00	237.0
258.00	1376.0
259.00	274.0
264.90	578.0
273.00	734.0
274.00	1855.0
275.00	10243.0
276.00	1242.0
276.90	865.0
278.00	157.0
285.00	181.0
292.90	175.0
296.00	2915.0
296.90	440.0
302.90	311.0
314.90	327.0
315.90	160.0
323.00	912.0
324.00	199.0
327.00	156.0
334.00	588.0
335.00	156.0
345.90	215.0
352.00	262.0
352.90	172.0
353.90	390.0
365.00	1455.0
366.00	235.0
372.00	427.0
401.90	243.0
403.00	366.0
421.00	267.0
422.00	305.0
423.00	1852.0
423.90	494.0
441.00	4945.0
442.00	33640.0
443.00	6565.0
443.90	571.0

Instrument :
BNA_M
ClientSampleId :
DFTPP38

m/z	Abundance
39.00	534.0
44.00	184.0
50.00	2173.0
51.10	7152.0
52.00	331.0
55.90	233.0
56.90	460.0
63.00	233.0
69.00	6265.0
73.10	204.0
74.00	849.0
75.00	1189.0
75.90	343.0
77.00	6962.0
78.00	434.0
79.00	601.0
79.90	352.0
81.00	542.0
81.90	165.0
86.00	228.0
91.00	178.0
93.00	1080.0
98.00	915.0
98.90	578.0
100.90	307.0
104.00	246.0
105.00	241.0
107.00	2386.0
108.00	397.0
110.00	3799.0
111.00	661.0
115.90	182.0
117.00	2692.0
118.00	189.0
121.90	203.0
122.90	277.0
127.00	8266.0
127.90	732.0
129.00	3562.0
130.00	295.0
135.00	321.0
136.90	196.0
141.00	559.0
142.00	167.0
147.00	304.0
148.00	636.0
148.90	153.0
155.00	340.0
156.00	394.0
159.90	151.0
161.00	204.0
164.90	255.0
167.00	1074.0
167.90	498.0
174.00	229.0
174.90	445.0
176.80	191.0
178.90	808.0
180.00	540.0
181.00	263.0
185.00	375.0
186.00	2673.0
187.00	814.0
189.00	167.0
191.90	293.0
193.00	357.0
195.90	591.0
197.90	18208.0
198.90	1080.0
203.00	170.0
204.00	702.0
205.00	1216.0
206.00	5309.0
207.00	848.0
208.00	239.0
211.00	218.0
216.90	1631.0
217.90	228.0
221.00	737.0
221.90	210.0
222.90	314.0
224.00	2850.0
225.00	800.0
227.00	1312.0
228.00	194.0
229.00	265.0
242.00	201.0
244.00	2404.0
245.00	321.0
246.00	497.0
255.00	12508.0
256.00	1748.0

Instrument :
BNA_M
ClientSampleId :
DFTPP38

256.90	189.0
257.90	801.0
265.00	364.0
273.00	386.0
274.00	1059.0
275.00	6244.0
276.00	783.0
276.90	557.0
296.00	1691.0
297.00	230.0
303.00	220.0
314.90	190.0
323.00	629.0
334.00	337.0
351.90	223.0
354.00	252.0
364.90	1080.0
371.90	330.0
403.00	163.0
420.90	191.0
422.00	173.0
423.00	1235.0
424.00	342.0
441.00	3548.0
442.00	24128.0
443.00	4451.0
443.90	371.0

Instrument :
BNA_M
ClientSampleId :
DFTPP38