

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030122\
 Data File : BM034101.D
 Acq On : 01 Mar 2022 10:39
 Operator : CG/JU
 Sample : PB142783BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK783

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022822.M
 Title : SVOA CALIBRATION

Signal : TIC: BM034101.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.372	20	23	28	rVB	39578	47139	1.48%	0.143%
2	3.790	90	94	108	rBV	482655	700007	21.96%	2.123%
3	4.143	150	154	160	rVB	9497	13647	0.43%	0.041%
4	7.060	646	650	655	rBV7	1651	4074	0.13%	0.012%
5	7.142	658	664	676	rVB	550056	844873	26.51%	2.563%
6	7.313	687	693	705	rVV	393261	634188	19.90%	1.924%
7	7.525	722	729	738	rVB	566991	908895	28.52%	2.757%
8	7.995	801	809	816	rBV	506101	780376	24.49%	2.367%
9	8.695	921	928	937	rBV	680369	1049652	32.94%	3.184%
10	9.154	999	1006	1017	rBV	520109	817863	25.66%	2.481%
11	9.883	1121	1130	1138	rBV	436260	692047	21.71%	2.099%
12	10.425	1215	1222	1232	rBV	691603	1123758	35.26%	3.409%
13	10.813	1279	1288	1295	rBV	600443	999608	31.36%	3.032%
14	10.936	1301	1309	1319	rBV	644046	1061808	33.32%	3.221%
15	12.107	1507	1508	1515	rVB7	2522	3685	0.12%	0.011%
16	12.395	1551	1557	1564	rBV3	9806	17996	0.56%	0.055%
17	13.024	1659	1664	1672	rBV5	3820	6693	0.21%	0.020%
18	14.036	1830	1836	1843	rBV	1270140	1695517	53.20%	5.143%
19	14.324	1878	1885	1894	rBV	1356925	1952716	61.27%	5.923%
20	14.630	1930	1937	1949	rBV	919541	1362592	42.75%	4.133%
21	14.801	1959	1966	1976	rBV	500988	727123	22.82%	2.205%
22	15.442	2071	2075	2082	rVB8	2832	5881	0.18%	0.018%
23	15.618	2099	2105	2115	rBV	1708318	2445604	76.74%	7.418%
24	15.724	2117	2123	2135	rBV	505154	676053	21.21%	2.051%
25	15.860	2140	2146	2154	rVB4	6904	12108	0.38%	0.037%
26	17.154	2364	2366	2372	rVB3	3442	4058	0.13%	0.012%
27	17.371	2397	2403	2410	rBV	1179092	1597670	50.13%	4.846%
28	17.471	2413	2420	2431	rBV	1895858	2644220	82.97%	8.020%
29	19.324	2731	2735	2741	rVV3	24661	34916	1.10%	0.106%
30	19.395	2743	2747	2752	rVB	20024	27225	0.85%	0.083%
31	19.759	2803	2809	2814	rBV	2283284	3056142	95.89%	9.270%
32	21.542	3107	3112	3122	rBV	1413352	1859605	58.35%	5.640%
33	23.836	3495	3502	3511	rVB2	1639107	3187027	100.00%	9.667%
34	23.994	3522	3529	3541	rVB2	955261	1974433	61.95%	5.989%

Sum of corrected areas: 32969199

Instrument :

BNA_M

ClientSampleId :




SBLK783

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030122\
Data File : BM034101.D
Acq On : 01 Mar 2022 10:39
Operator : CG/JU
Sample : PB142783BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK783

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

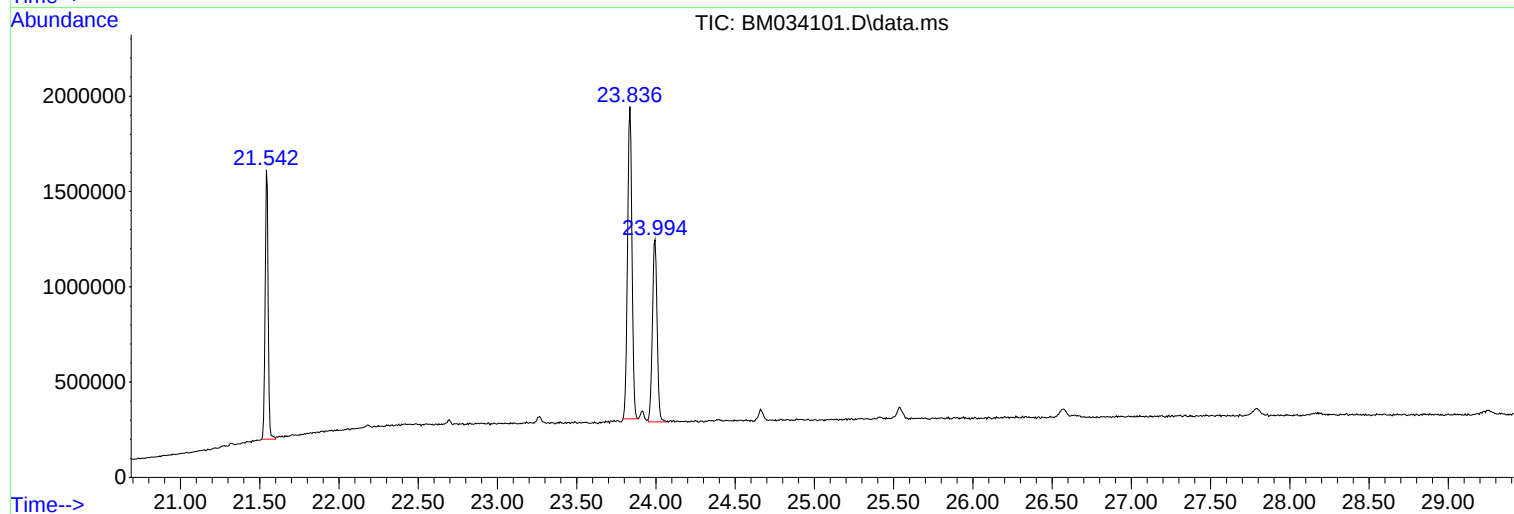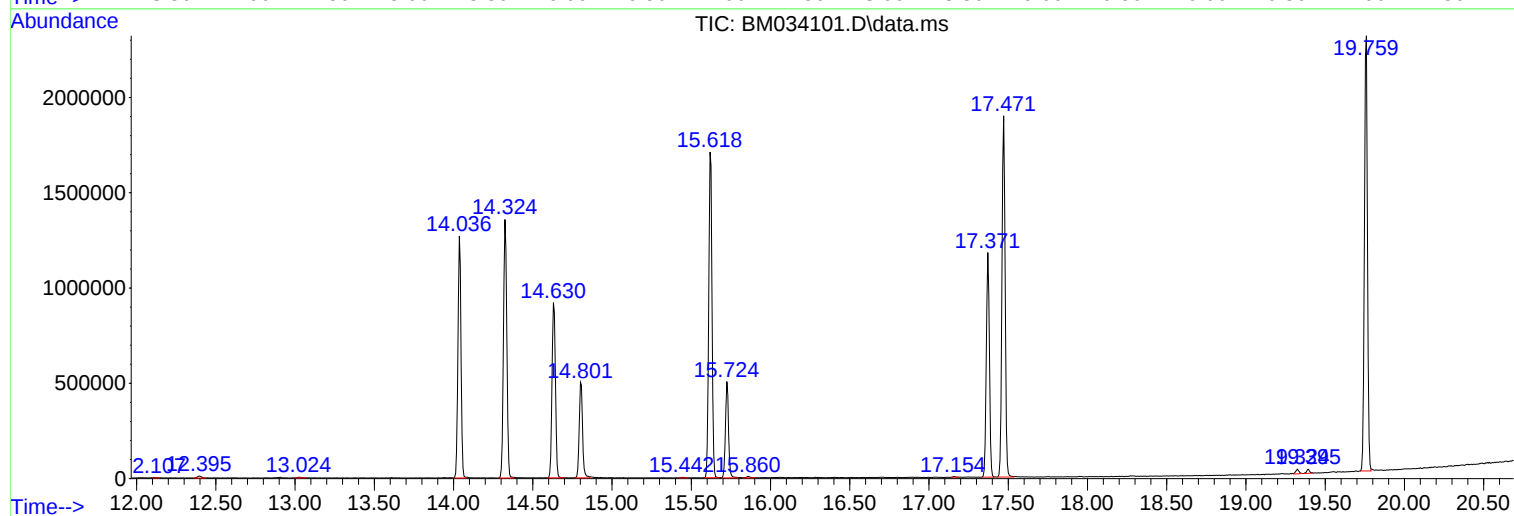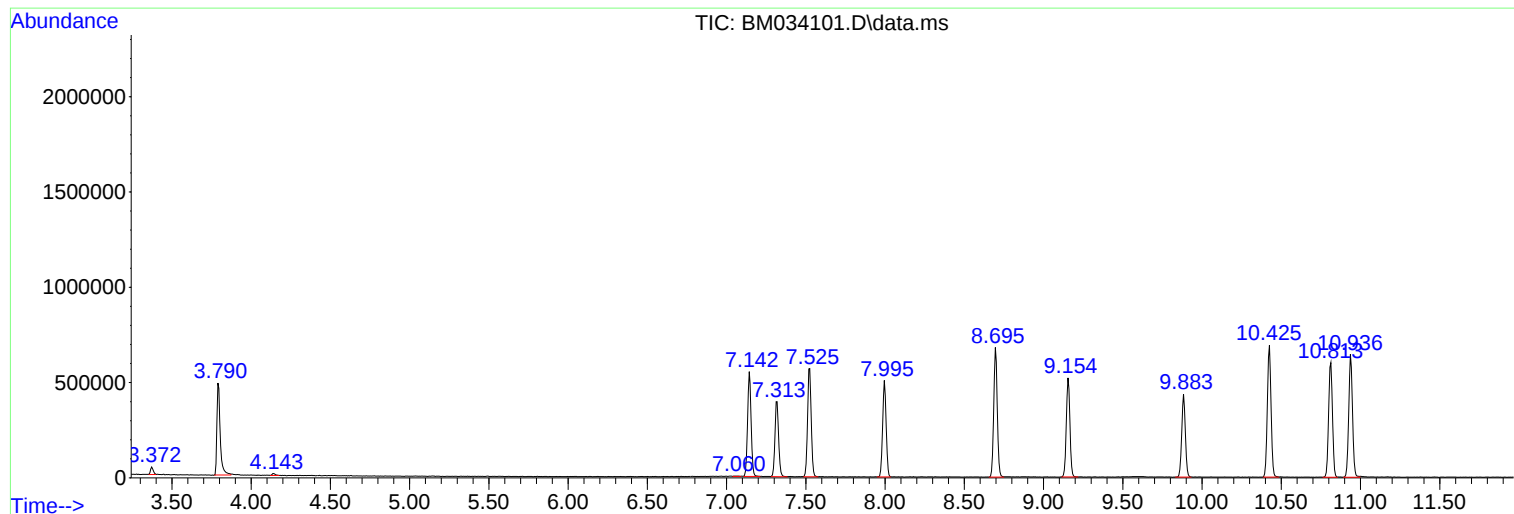

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030122\
Data File : BM034101.D
Acq On : 01 Mar 2022 10:39
Operator : CG/JU
Sample : PB142783BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK783

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030122\
Data File : BM034101.D
Acq On : 01 Mar 2022 10:39
Operator : CG/JU
Sample : PB142783BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK783

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc