

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030122\
 Data File : BM034103.D
 Acq On : 01 Mar 2022 12:24
 Operator : CG/JU
 Sample : PB142782BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK782

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022822.M
 Title : SVOA CALIBRATION

Signal : TIC: BM034103.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.372	19	23	33	rVB	45873	59836	1.72%	0.163%
2	3.790	90	94	106	rBV	568997	794921	22.83%	2.159%
3	4.137	150	153	160	rVB	11908	15986	0.46%	0.043%
4	7.143	657	664	673	rVB	614712	956106	27.46%	2.597%
5	7.319	687	694	701	rBV	452178	710540	20.40%	1.930%
6	7.525	721	729	739	rBV	645037	1025278	29.44%	2.784%
7	7.995	803	809	819	rVB	558569	871992	25.04%	2.368%
8	8.695	921	928	939	rBV	738847	1186384	34.07%	3.222%
9	9.154	999	1006	1019	rVB	579231	932894	26.79%	2.534%
10	9.884	1122	1130	1140	rBV	495222	790709	22.71%	2.147%
11	10.425	1215	1222	1232	rBV	791766	1285679	36.92%	3.492%
12	10.813	1279	1288	1296	rBV	677137	1127155	32.37%	3.061%
13	10.936	1302	1309	1326	rBV	723983	1213470	34.85%	3.296%
14	12.395	1550	1557	1563	rVB	12552	20837	0.60%	0.057%
15	12.854	1623	1635	1648	rVB7	6266	26594	0.76%	0.072%
16	12.978	1651	1656	1657	rBV4	6085	9065	0.26%	0.025%
17	13.601	1759	1762	1766	rBV3	2475	3882	0.11%	0.011%
18	13.930	1811	1818	1820	rBV5	4722	8588	0.25%	0.023%
19	14.042	1830	1837	1850	rBV	1364571	1922019	55.19%	5.220%
20	14.324	1879	1885	1895	rBV	1527997	2228549	64.00%	6.052%
21	14.548	1913	1923	1927	rBV6	3043	6145	0.18%	0.017%
22	14.636	1931	1938	1949	rVB	1047024	1555751	44.68%	4.225%
23	14.807	1954	1967	1981	rBV	583083	821275	23.58%	2.230%
24	15.442	2066	2075	2080	rBV5	9019	16102	0.46%	0.044%
25	15.624	2099	2106	2117	rBV	1976003	2781473	79.88%	7.554%
26	15.724	2117	2123	2132	rBV	532383	750639	21.56%	2.039%
27	15.866	2142	2147	2151	rVB3	8790	12820	0.37%	0.035%
28	16.071	2177	2182	2184	rVV4	3100	4504	0.13%	0.012%
29	16.701	2286	2289	2293	rVB4	3093	3971	0.11%	0.011%
30	17.054	2346	2349	2354	rBV5	2211	3549	0.10%	0.010%
31	17.165	2364	2368	2372	rBV5	2837	4565	0.13%	0.012%
32	17.248	2379	2382	2385	rBV4	4471	4841	0.14%	0.013%
33	17.371	2396	2403	2413	rBV	1243120	1762122	50.60%	4.786%
34	17.471	2413	2420	2436	rVV	2121296	2919232	83.83%	7.928%
35	18.265	2552	2555	2559	rBV4	6458	9414	0.27%	0.026%
36	18.901	2661	2663	2667	rBV5	3385	4225	0.12%	0.011%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030122\
Data File : BM034103.D
Acq On : 01 Mar 2022 12:24
Operator : CG/JU
Sample : PB142782BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK782

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022822.M
Title : SVOA CALIBRATION

37	19.324	2731	2735	2740	rBV2	24409	36259	1.04%	0.098%
38	19.395	2744	2747	2752	rVB	22538	30105	0.86%	0.082%
39	19.759	2803	2809	2822	rBV	2570889	3339547	95.90%	9.070%
40	21.548	3108	3113	3125	rBV	1550945	1980288	56.87%	5.378%
41	23.842	3495	3503	3511	rBV2	1758878	3482251	100.00%	9.457%
42	24.000	3523	3530	3539	rVB2	1009574	2101913	60.36%	5.708%




Sum of corrected areas: 36821475

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030122\
Data File : BM034103.D
Acq On : 01 Mar 2022 12:24
Operator : CG/JU
Sample : PB142782BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK782

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

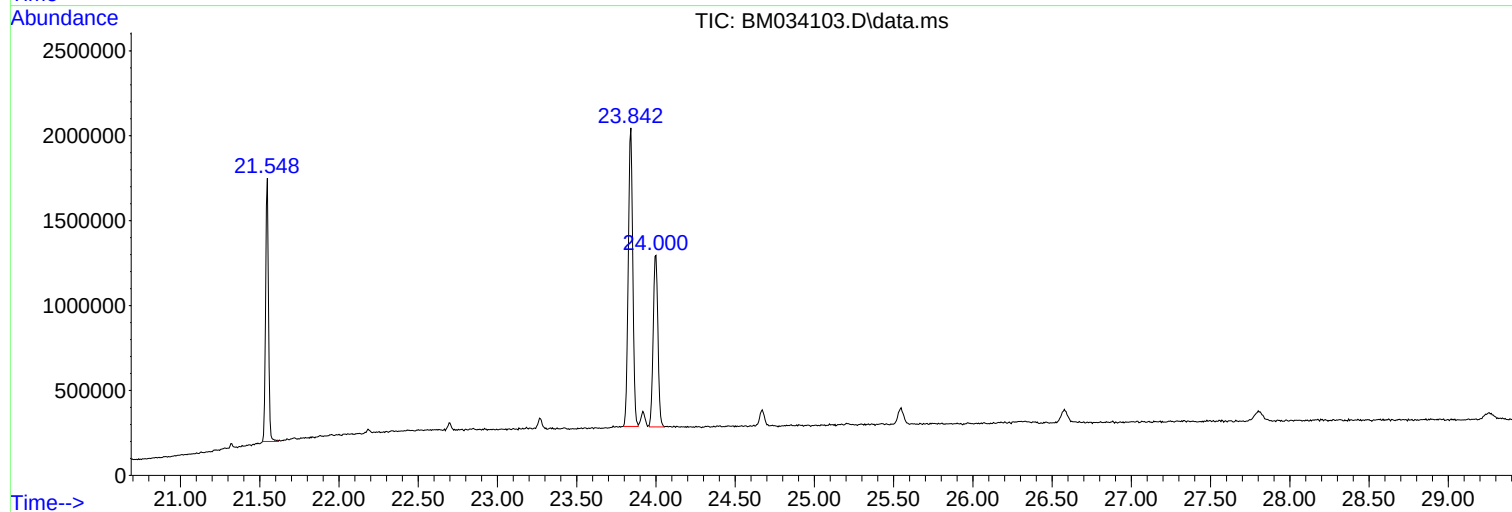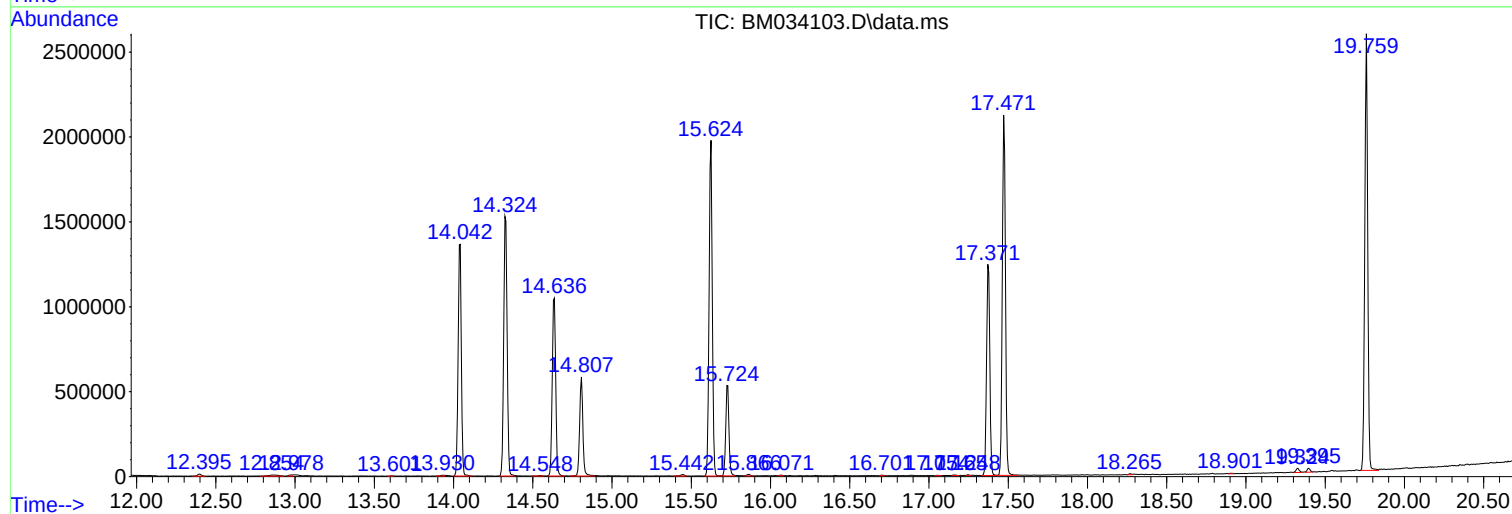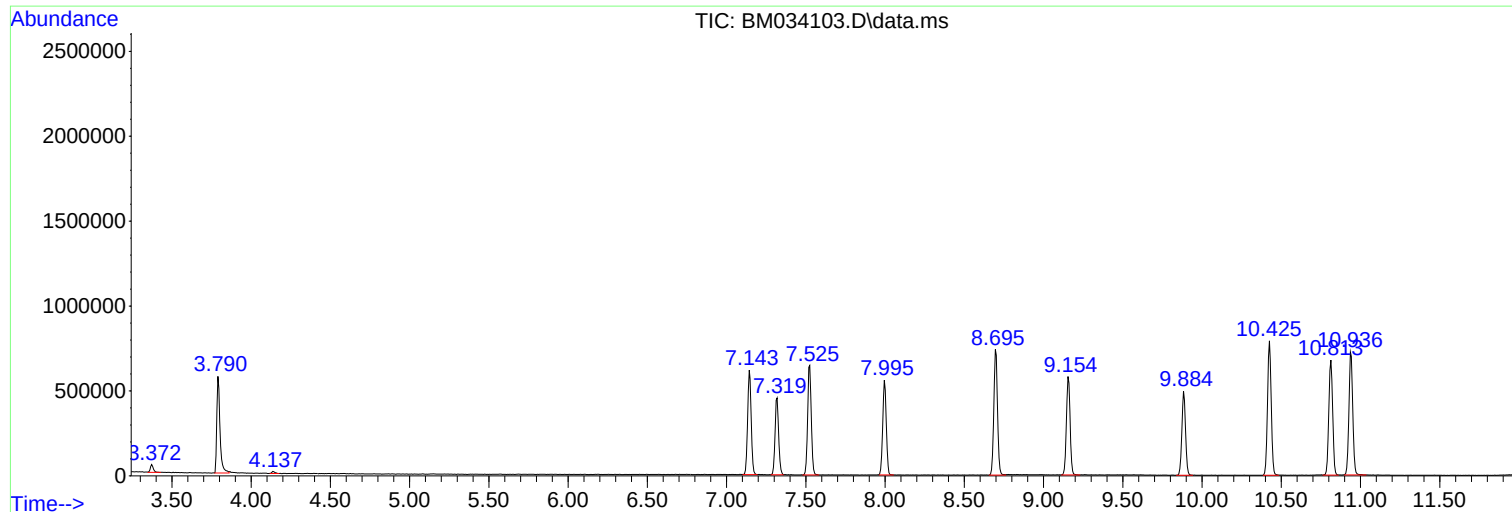

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030122\
Data File : BM034103.D
Acq On : 01 Mar 2022 12:24
Operator : CG/JU
Sample : PB142782BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK782

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030122\
Data File : BM034103.D
Acq On : 01 Mar 2022 12:24
Operator : CG/JU
Sample : PB142782BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK782

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc