

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030122\
 Data File : BM034107.D
 Acq On : 01 Mar 2022 15:46
 Operator : CG/JU
 Sample : N1676-05
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022822.M
 Title : SVOA CALIBRATION

Signal : TIC: BM034107.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.137	151	153	161	rVB4	9536	14346	0.76%	0.174%
2	5.719	420	422	427	rVB4	1420	1911	0.10%	0.023%
3	5.848	439	444	449	rVB7	1552	3589	0.19%	0.043%
4	6.872	614	618	620	rBV4	1470	2084	0.11%	0.025%
5	6.966	632	634	637	rVB3	2074	1965	0.10%	0.024%
6	7.995	802	809	817	rVB	467518	741045	39.11%	8.979%
7	9.025	981	984	986	rBV4	1873	2146	0.11%	0.026%
8	10.813	1281	1288	1296	rVV	542928	911423	48.10%	11.043%
9	11.383	1382	1385	1388	rVB5	1298	1921	0.10%	0.023%
10	12.013	1487	1492	1493	rBV4	2453	2972	0.16%	0.036%
11	12.042	1495	1497	1501	rVB4	1562	1991	0.11%	0.024%
12	12.871	1629	1638	1639	rBV6	5905	10062	0.53%	0.122%
13	13.001	1654	1660	1662	rBV3	5779	11357	0.60%	0.138%
14	13.083	1671	1674	1677	rBV4	1294	1936	0.10%	0.023%
15	13.930	1814	1818	1826	rBV6	4886	9860	0.52%	0.119%
16	14.083	1838	1844	1851	rVB7	3371	7062	0.37%	0.086%
17	14.371	1887	1893	1900	rVB3	4159	6579	0.35%	0.080%
18	14.548	1918	1923	1926	rBV6	2637	3632	0.19%	0.044%
19	14.636	1931	1938	1949	rVV	839674	1226825	64.74%	14.865%
20	14.771	1956	1961	1965	rVB4	2253	3282	0.17%	0.040%
21	15.442	2069	2075	2079	rBV5	5436	9024	0.48%	0.109%
22	15.636	2104	2108	2112	rBV6	4367	6192	0.33%	0.075%
23	15.918	2153	2156	2158	rBV4	1545	1912	0.10%	0.023%
24	15.971	2162	2165	2168	rBV4	2238	2647	0.14%	0.032%
25	16.065	2176	2181	2184	rVB4	3468	5056	0.27%	0.061%
26	16.701	2285	2289	2293	rBV6	4022	5200	0.27%	0.063%
27	17.012	2338	2342	2343	rBV4	1949	2230	0.12%	0.027%
28	17.159	2362	2367	2372	rBV5	4418	8338	0.44%	0.101%
29	17.242	2378	2381	2387	rBV8	3356	4919	0.26%	0.060%
30	17.377	2397	2404	2411	rBV	1038345	1483454	78.28%	17.975%
31	17.471	2417	2420	2425	rVB4	4079	5289	0.28%	0.064%
32	18.289	2554	2559	2560	rBV4	3037	4606	0.24%	0.056%
33	21.547	3108	3113	3122	rBV	1461242	1853187	97.79%	22.455%
34	24.000	3523	3530	3539	rVB2	946089	1894999	100.00%	22.961%

Sum of corrected areas: 8253041

Instrument :

BNA_M

ClientSampleId :




SVOC-GPC-BLANK

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030122\
Data File : BM034107.D
Acq On : 01 Mar 2022 15:46
Operator : CG/JU
Sample : N1676-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

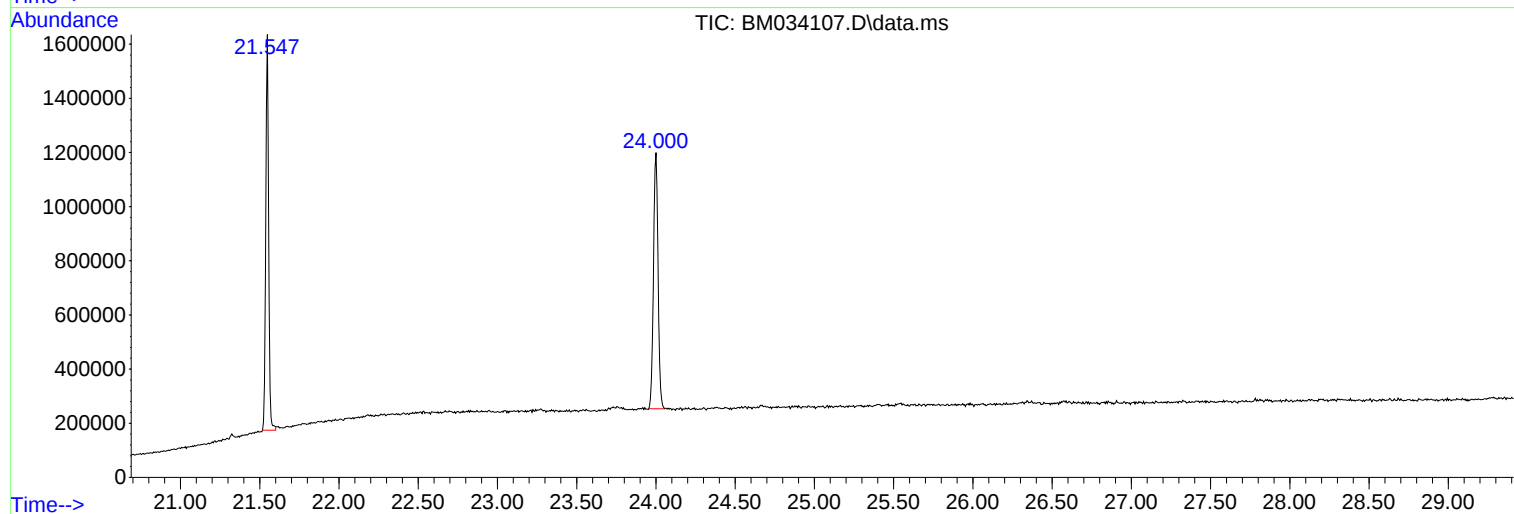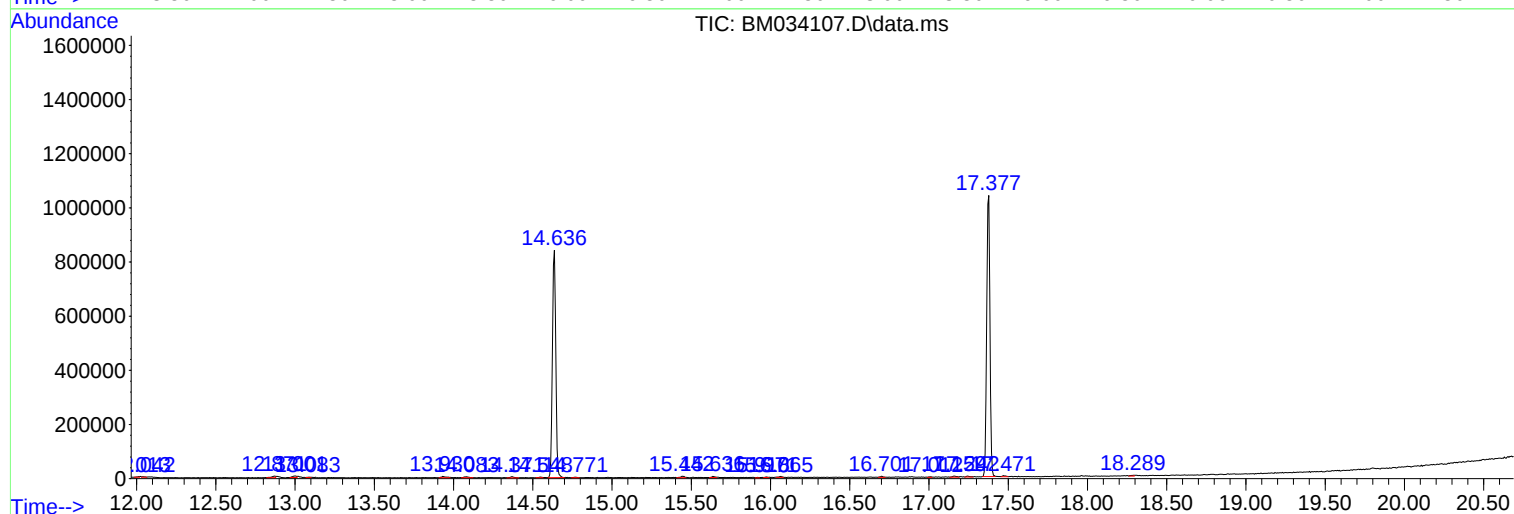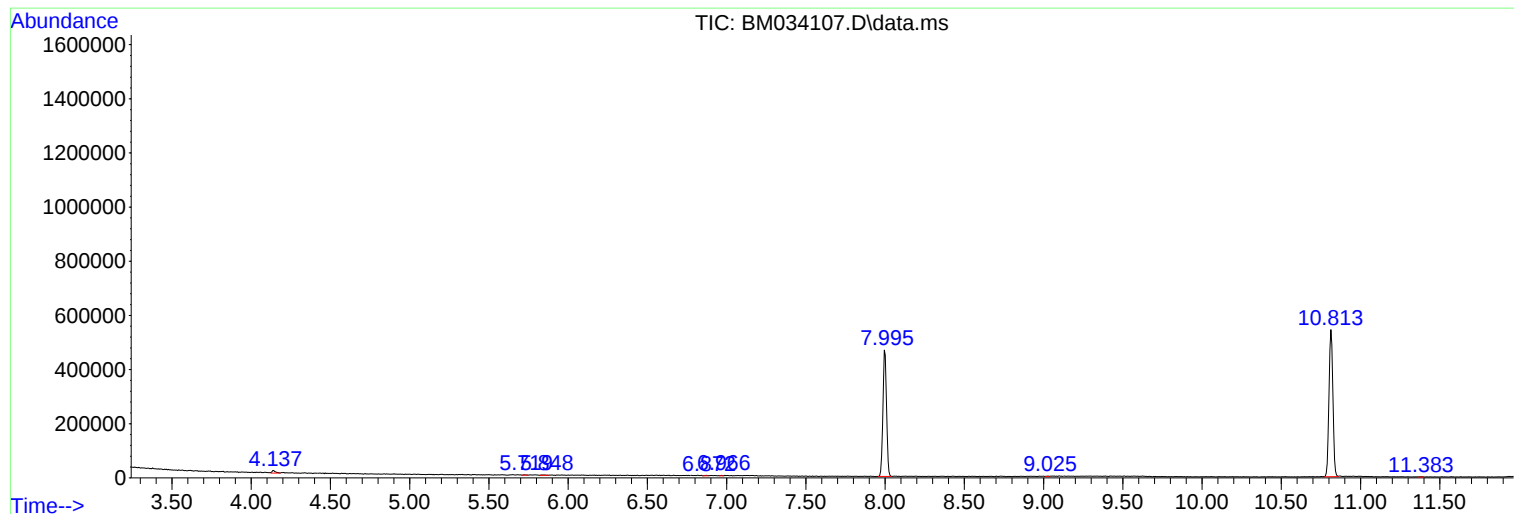

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030122\
Data File : BM034107.D
Acq On : 01 Mar 2022 15:46
Operator : CG/JU
Sample : N1676-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030122\
Data File : BM034107.D
Acq On : 01 Mar 2022 15:46
Operator : CG/JU
Sample : N1676-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc