

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030124\
 Data File : BM044473.D
 Acq On : 01 Mar 2024 16:40
 Operator : MA/JU
 Sample : PB159245BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK245

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM044473.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.128	4	7	11	rVB	33765	39429	0.90%	0.078%
2	3.175	11	15	29	rVB	489913	615793	14.02%	1.225%
3	3.404	50	54	60	rBV	70837	91752	2.09%	0.183%
4	3.828	122	126	146	rBV	827194	1361301	30.98%	2.708%
5	4.157	178	182	187	rVB3	38169	59533	1.36%	0.118%
6	4.340	211	213	219	rVV7	7046	9444	0.21%	0.019%
7	4.393	219	222	229	rVB2	19671	27709	0.63%	0.055%
8	4.545	246	248	254	rVB4	10252	15599	0.36%	0.031%
9	4.740	276	281	288	rVV	49353	72333	1.65%	0.144%
10	4.804	288	292	300	rVB2	17833	38291	0.87%	0.076%
11	5.922	477	482	486	rBV6	8101	13183	0.30%	0.026%
12	6.357	552	556	559	rBV6	6374	8446	0.19%	0.017%
13	6.569	590	592	596	rBV4	4170	4807	0.11%	0.010%
14	6.828	634	636	638	rBV3	4394	5087	0.12%	0.010%
15	7.216	695	702	710	rBV	885352	1414572	32.20%	2.814%
16	7.392	726	732	747	rBV	738130	1216679	27.69%	2.420%
17	7.575	756	763	779	rBV	881601	1446946	32.93%	2.878%
18	7.775	792	797	801	rVB7	5850	8941	0.20%	0.018%
19	8.016	834	838	839	rBV4	4220	5154	0.12%	0.010%
20	8.057	839	845	855	rVB	767825	1206513	27.46%	2.400%
21	8.304	883	887	893	rVB7	6627	9246	0.21%	0.018%
22	8.422	902	907	910	rVB7	3613	5825	0.13%	0.012%
23	8.781	961	968	981	rBV	1036837	1705613	38.82%	3.393%
24	8.963	996	999	1002	rBV5	2939	4463	0.10%	0.009%
25	9.239	1040	1046	1061	rBV	798782	1335957	30.41%	2.657%
26	9.969	1161	1170	1182	rBV	638697	1076497	24.50%	2.141%
27	10.245	1213	1217	1218	rBV4	5264	5556	0.13%	0.011%
28	10.510	1254	1262	1278	rBV	903640	1651409	37.59%	3.285%
29	10.757	1300	1304	1307	rBV6	4167	6136	0.14%	0.012%
30	10.886	1317	1326	1337	rBV	1021762	1699060	38.67%	3.380%
31	11.039	1344	1352	1367	rBV	938481	1769630	40.28%	3.520%
32	11.280	1389	1393	1395	rBV4	3509	4529	0.10%	0.009%
33	11.551	1434	1439	1442	rBV7	4348	6756	0.15%	0.013%
34	11.592	1442	1446	1447	rVB4	3832	5305	0.12%	0.011%
35	11.657	1452	1457	1460	rBV6	4957	7863	0.18%	0.016%
36	12.480	1593	1597	1606	rVB3	15203	28996	0.66%	0.058%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030124\
 Data File : BM044473.D
 Acq On : 01 Mar 2024 16:40
 Operator : MA/JU
 Sample : PB159245BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK245

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
 Title : SVOA CALIBRATION

37	13.633	1785	1793	1799	rBV2	18907	31359	0.71%	0.062%
38	14.151	1873	1881	1897	rBV	1648322	2419653	55.07%	4.813%
39	14.415	1919	1926	1937	rBV	2014995	2957669	67.32%	5.883%
40	14.486	1937	1938	1945	rVB7	3277	5243	0.12%	0.010%
41	14.721	1969	1978	1989	rBV	1490412	2116692	48.18%	4.210%
42	14.933	2007	2014	2035	rBV	404037	1010904	23.01%	2.011%
43	15.715	2140	2147	2162	rBV	2498527	3666958	83.46%	7.294%
44	15.845	2162	2169	2179	rBV	667041	980513	22.32%	1.950%
45	15.957	2185	2188	2193	rVB3	11876	17105	0.39%	0.034%
46	16.139	2215	2219	2224	rBV8	2703	5077	0.12%	0.010%
47	16.292	2242	2245	2250	rVB7	3278	5458	0.12%	0.011%
48	16.504	2276	2281	2286	rVB6	7796	12380	0.28%	0.025%
49	16.627	2297	2302	2305	rBV7	2841	5006	0.11%	0.010%
50	17.262	2406	2410	2414	rBV5	3785	6713	0.15%	0.013%
51	17.480	2439	2447	2456	rBV	1653109	2440287	55.54%	4.854%
52	17.574	2456	2463	2480	rVV2	2636783	3941173	89.71%	7.839%
53	18.233	2574	2575	2579	rBV4	4118	5672	0.13%	0.011%
54	18.780	2663	2668	2669	rBV4	2931	5022	0.11%	0.010%
55	19.439	2775	2780	2785	rBV3	30645	42894	0.98%	0.085%
56	19.503	2788	2791	2796	rVV	27268	36284	0.83%	0.072%
57	19.592	2804	2806	2807	rBV2	5134	4497	0.10%	0.009%
58	19.868	2847	2853	2862	rBV	3292624	4393460	100.00%	8.739%
59	21.674	3154	3160	3169	rBV	1678623	2362124	53.76%	4.698%
60	24.038	3554	3562	3578	rVB2	1966385	4244379	96.61%	8.442%
61	24.203	3582	3590	3604	rVB	1147356	2573318	58.57%	5.119%




Sum of corrected areas: 50274193

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030124\
Data File : BM044473.D
Acq On : 01 Mar 2024 16:40
Operator : MA/JU
Sample : PB159245BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK245

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

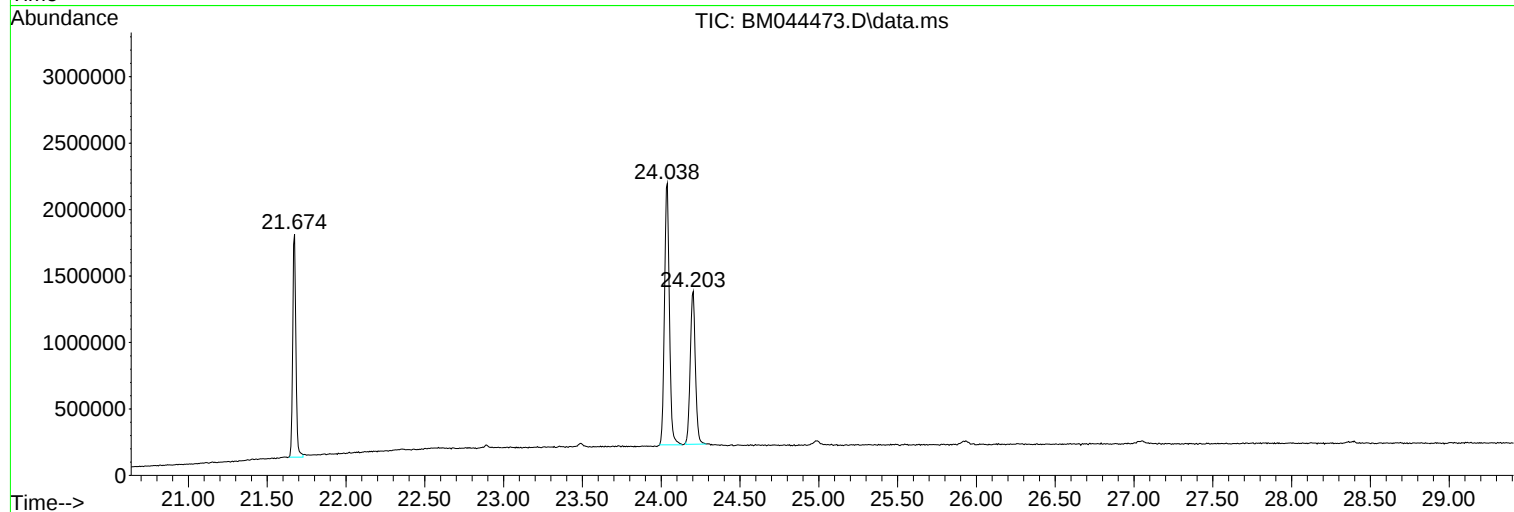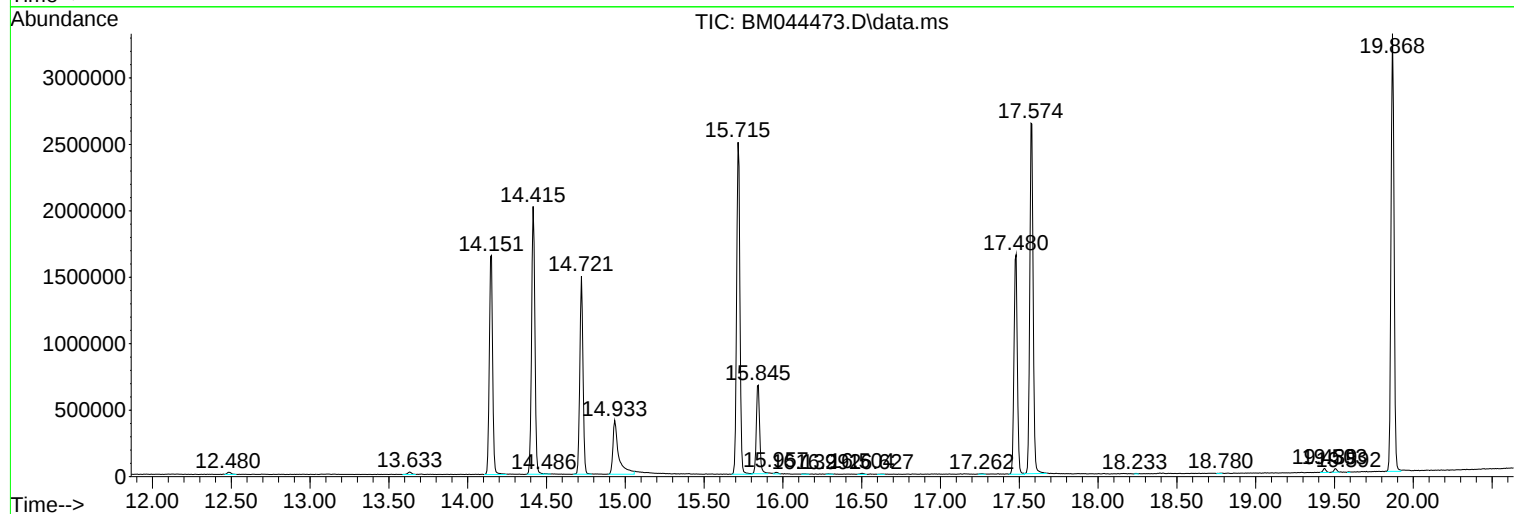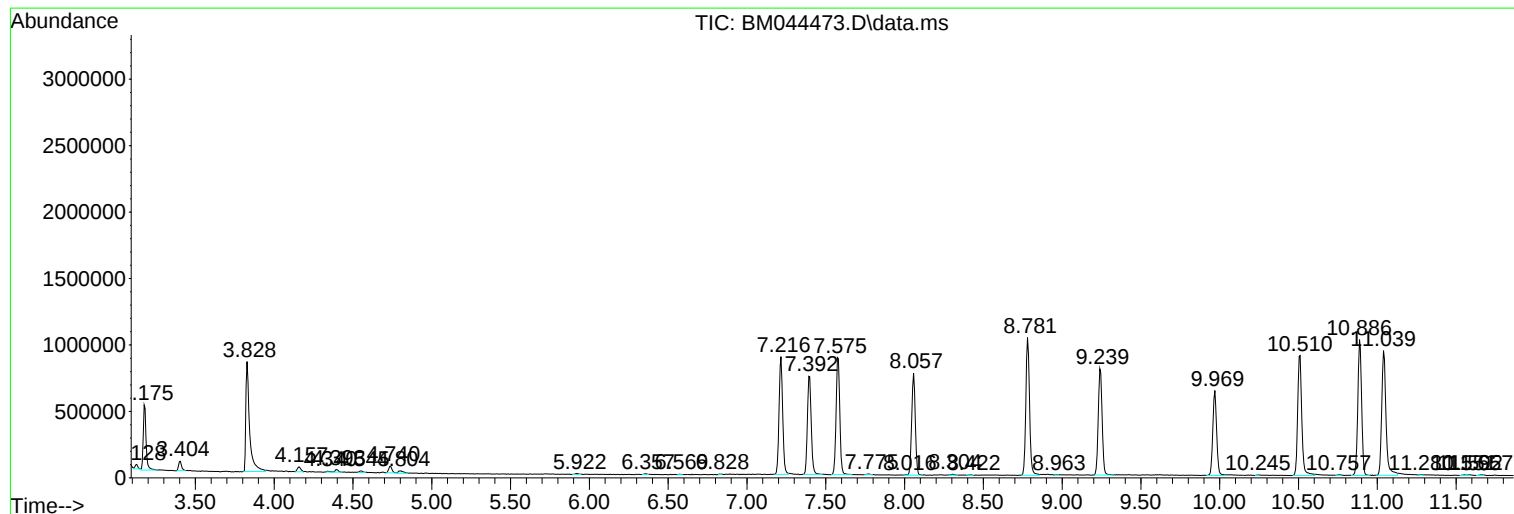

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030124\
Data File : BM044473.D
Acq On : 01 Mar 2024 16:40
Operator : MA/JU
Sample : PB159245BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK245










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Furan, tetrahydro-2-(methox... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.175	10.21 ng/ul	615793	1,4-Dichlorobenzene-d4	8.057

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Furan, tetrahydro-2-(methoxymeth...	116	C6H12O2	019354-27-9	72
2			3-Buten-2-ol, 2-methyl-	86	C5H10O	000115-18-4	72
3			3-Penten-2-ol	86	C5H10O	001569-50-2	64
4			3-Buten-2-ol, 2-methyl-	86	C5H10O	000115-18-4	59
5			Butane, 2-bromo-2-methyl-	150	C5H11Br	000507-36-8	59

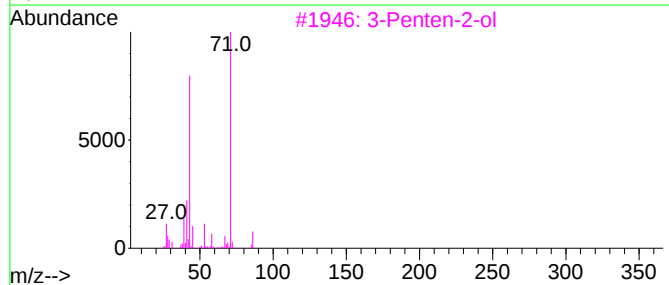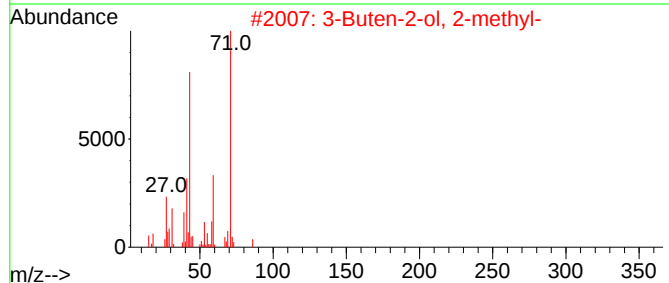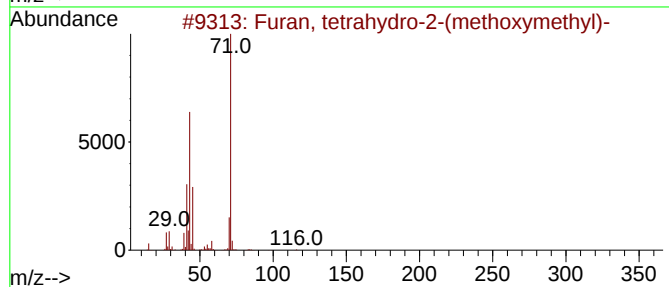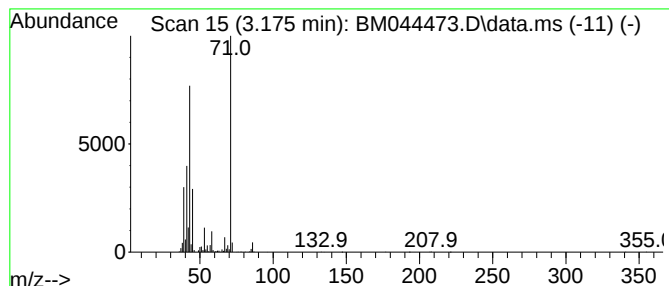

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030124\
Data File : BM044473.D
Acq On : 01 Mar 2024 16:40
Operator : MA/JU
Sample : PB159245BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK245

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Furan, tetrahyd...	3.175	10.2	ng/u1	615793	1	8.057	1206510	20.0