

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030222\
 Data File : BM034112.D
 Acq On : 02 Mar 2022 10:01
 Operator : CG/JU
 Sample : PB142853BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK853

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022822.M
 Title : SVOA CALIBRATION

Signal : TIC: BM034112.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.372	19	23	31	rVB	39446	53159	1.64%	0.149%
2	3.790	91	94	112	rBV	499588	728961	22.51%	2.047%
3	3.961	121	123	129	rBV7	2465	4489	0.14%	0.013%
4	4.143	150	154	158	rBV2	9349	13106	0.40%	0.037%
5	5.155	325	326	332	rVB4	2258	3336	0.10%	0.009%
6	7.143	658	664	673	rBV	587181	884034	27.30%	2.483%
7	7.313	687	693	704	rVB	424975	668694	20.65%	1.878%
8	7.519	722	728	737	rBV	600697	944594	29.17%	2.653%
9	7.996	802	809	818	rBV	573148	882573	27.25%	2.479%
10	8.696	921	928	937	rBV	714789	1122488	34.66%	3.152%
11	9.154	999	1006	1015	rBV	544068	880633	27.19%	2.473%
12	9.884	1122	1130	1138	rBV	468776	745613	23.02%	2.094%
13	10.425	1215	1222	1232	rBV	733913	1211270	37.40%	3.402%
14	10.807	1279	1287	1296	rBV	707701	1201854	37.11%	3.375%
15	10.937	1302	1309	1318	rBV	701025	1162840	35.91%	3.266%
16	12.395	1551	1557	1565	rVB2	12707	21031	0.65%	0.059%
17	12.901	1638	1643	1647	rBV5	2541	4329	0.13%	0.012%
18	14.036	1830	1836	1842	rBV	1458265	1916706	59.19%	5.383%
19	14.083	1842	1844	1849	rVB4	3434	4804	0.15%	0.013%
20	14.325	1878	1885	1898	rBV	1542094	2182784	67.40%	6.130%
21	14.630	1930	1937	1946	rVB	1171635	1700811	52.52%	4.776%
22	14.801	1958	1966	1986	rBV	552157	802469	24.78%	2.254%
23	15.442	2072	2075	2081	rVB5	3185	3493	0.11%	0.010%
24	15.619	2098	2105	2114	rBV	1920823	2756176	85.11%	7.740%
25	15.725	2117	2123	2137	rVV	557210	750615	23.18%	2.108%
26	15.860	2142	2146	2152	rVB3	9048	11716	0.36%	0.033%
27	16.695	2285	2288	2294	rBV6	1910	4601	0.14%	0.013%
28	17.160	2361	2367	2371	rVB3	5241	9710	0.30%	0.027%
29	17.371	2396	2403	2410	rBV	1413392	1948052	60.15%	5.471%
30	17.471	2413	2420	2432	rBV	2117954	2944219	90.91%	8.268%
31	19.324	2731	2735	2741	rVB3	23667	32723	1.01%	0.092%
32	19.389	2741	2746	2750	rBV2	23545	36556	1.13%	0.103%
33	19.760	2802	2809	2815	rBV	2357691	3238435	100.00%	9.095%
34	21.542	3107	3112	3117	rBV	1504556	1909160	58.95%	5.362%
35	23.836	3495	3502	3511	rVB	1515845	2940853	90.81%	8.259%
36	23.989	3522	3528	3537	rVB2	917710	1881481	58.10%	5.284%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030222\
Data File : BM034112.D
Acq On : 02 Mar 2022 10:01
Operator : CG/JU
Sample : PB142853BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK853

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022822.M
Title : SVOA CALIBRATION


Sum of corrected areas: 35608368

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030222\
Data File : BM034112.D
Acq On : 02 Mar 2022 10:01
Operator : CG/JU
Sample : PB142853BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK853

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

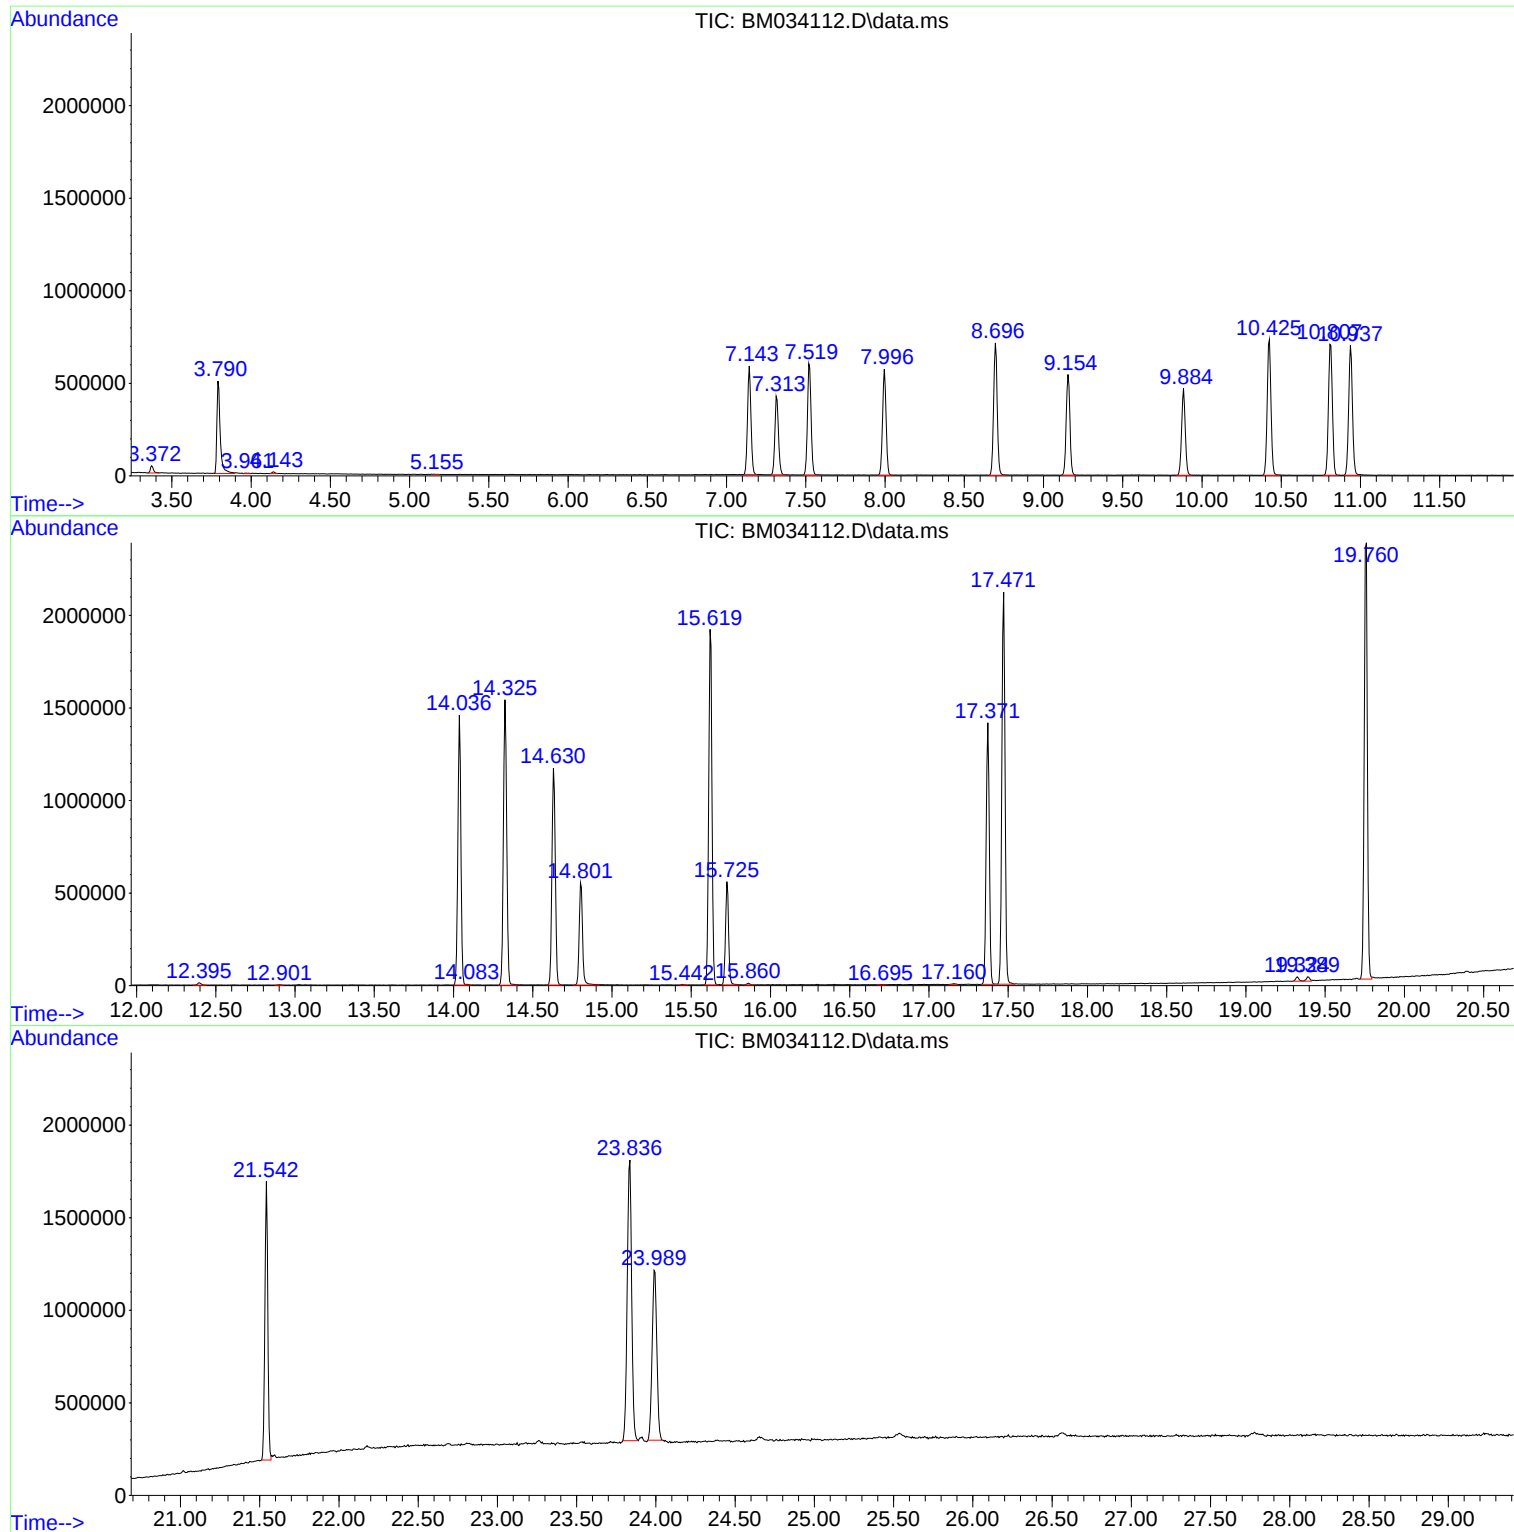

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030222\
Data File : BM034112.D
Acq On : 02 Mar 2022 10:01
Operator : CG/JU
Sample : PB142853BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK853

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030222\
Data File : BM034112.D
Acq On : 02 Mar 2022 10:01
Operator : CG/JU
Sample : PB142853BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK853

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------