

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030222\
 Data File : BM034114.D
 Acq On : 02 Mar 2022 12:50
 Operator : CG/JU
 Sample : PB142784BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK784

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022822.M
 Title : SVOA CALIBRATION

Signal : TIC: BM034114.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.373	19	23	30	rVB	36094	41781	1.51%	0.144%
2	3.790	90	94	111	rBV	427768	616136	22.33%	2.125%
3	4.137	149	153	159	rVB2	8802	12733	0.46%	0.044%
4	7.143	656	664	673	rBV	484618	749572	27.17%	2.585%
5	7.319	687	694	706	rVB	355551	561000	20.34%	1.935%
6	7.525	722	729	737	rBV	507680	806183	29.22%	2.780%
7	7.996	802	809	816	rBV	486378	772551	28.00%	2.664%
8	8.696	922	928	938	rBV	589743	930911	33.74%	3.210%
9	9.155	999	1006	1016	rBV	443388	723014	26.21%	2.494%
10	9.884	1123	1130	1142	rVB	378651	603655	21.88%	2.082%
11	10.425	1214	1222	1235	rBV	606858	992474	35.98%	3.423%
12	10.813	1277	1288	1297	rBV	582388	973421	35.28%	3.357%
13	10.937	1302	1309	1325	rBV	546654	924116	33.50%	3.187%
14	12.395	1553	1557	1562	rBV2	8899	13224	0.48%	0.046%
15	13.025	1655	1664	1668	rBV5	2995	6640	0.24%	0.023%
16	14.037	1830	1836	1843	rBV	1064996	1434701	52.01%	4.948%
17	14.084	1843	1844	1849	rVB3	3361	2991	0.11%	0.010%
18	14.325	1879	1885	1897	rBV	1144020	1648293	59.75%	5.685%
19	14.637	1931	1938	1949	rVB	862846	1290239	46.77%	4.450%
20	14.807	1960	1967	1978	rBV	422755	614134	22.26%	2.118%
21	15.625	2099	2106	2113	rBV	1463697	2078889	75.36%	7.170%
22	15.725	2118	2123	2133	rBV	402386	561939	20.37%	1.938%
23	15.866	2142	2147	2150	rBV3	6259	8666	0.31%	0.030%
24	16.701	2285	2289	2294	rBV6	1735	2931	0.11%	0.010%
25	17.160	2363	2367	2371	rBV2	3443	5122	0.19%	0.018%
26	17.248	2378	2382	2387	rBV6	1984	3689	0.13%	0.013%
27	17.372	2397	2403	2411	rBV	1049746	1481400	53.70%	5.109%
28	17.472	2414	2420	2432	rVV	1606763	2238862	81.15%	7.721%
29	18.272	2553	2556	2557	rBV2	2438	2979	0.11%	0.010%
30	19.324	2731	2735	2741	rBV3	17396	24595	0.89%	0.085%
31	19.395	2744	2747	2751	rVV	17118	21726	0.79%	0.075%
32	19.695	2796	2798	2801	rBV4	5574	6539	0.24%	0.023%
33	19.760	2803	2809	2821	rVV	1977598	2616559	94.84%	9.024%
34	21.542	3107	3112	3118	rBV	1258087	1679271	60.87%	5.791%
35	23.836	3495	3502	3510	rBV2	1415153	2758775	100.00%	9.514%
36	23.995	3522	3529	3538	rBV2	894863	1786136	64.74%	6.160%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030222\
Data File : BM034114.D
Acq On : 02 Mar 2022 12:50
Operator : CG/JU
Sample : PB142784BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK784

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022822.M
Title : SVOA CALIBRATION




Sum of corrected areas: 28995847

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030222\
Data File : BM034114.D
Acq On : 02 Mar 2022 12:50
Operator : CG/JU
Sample : PB142784BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK784

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

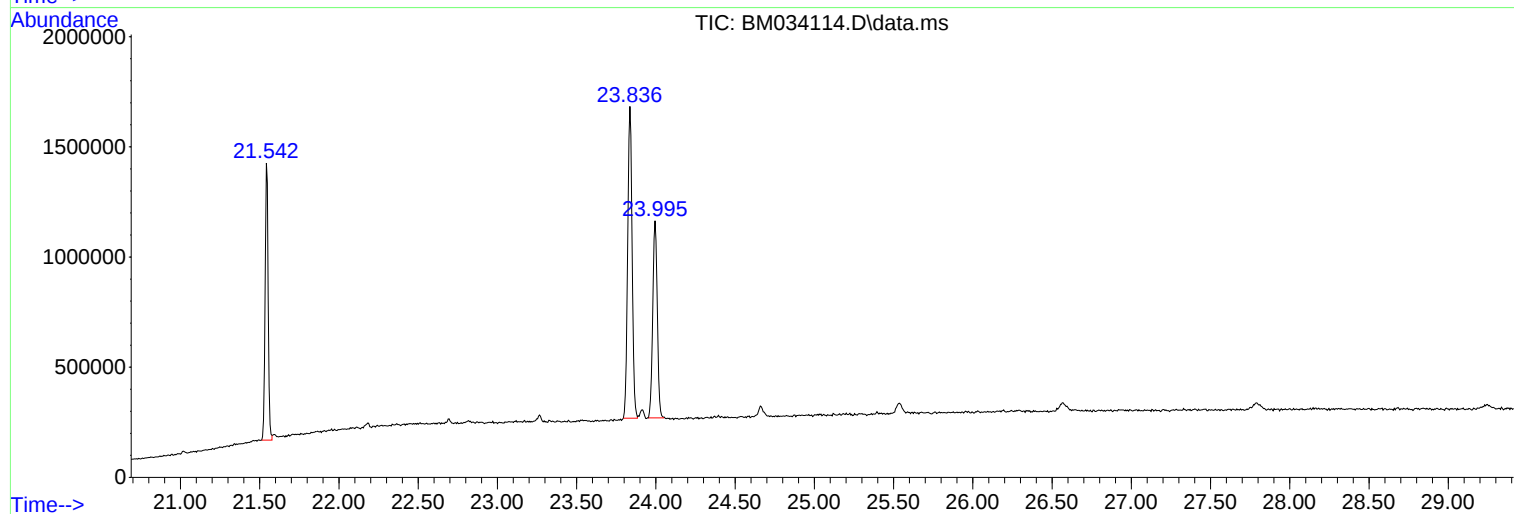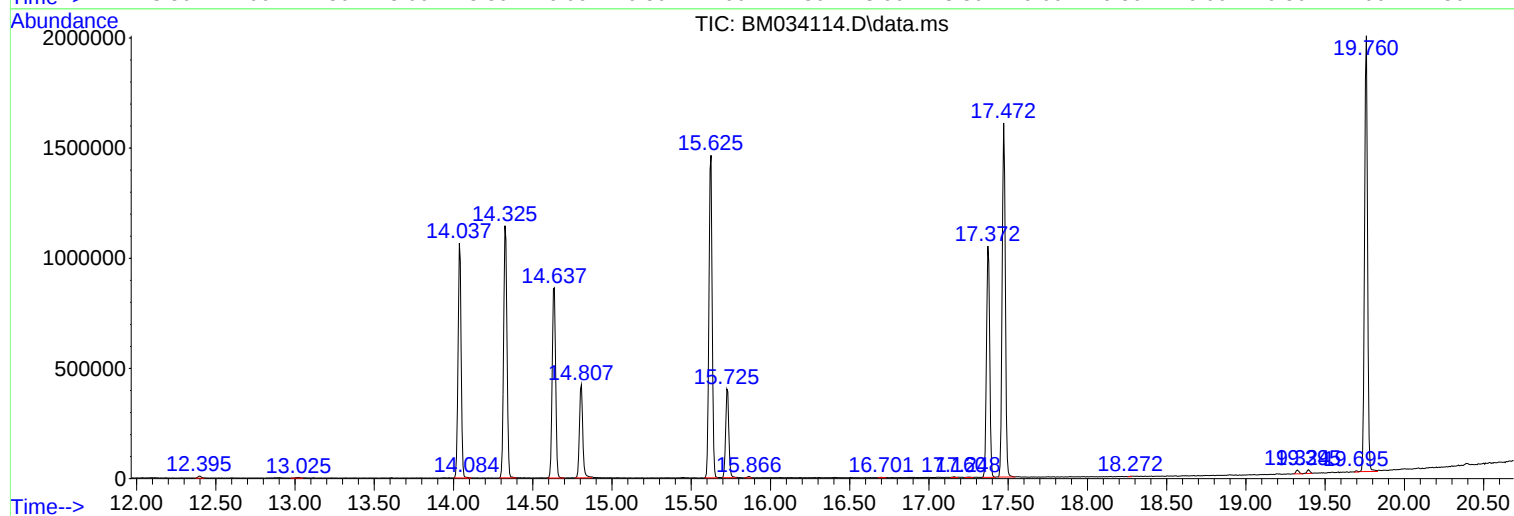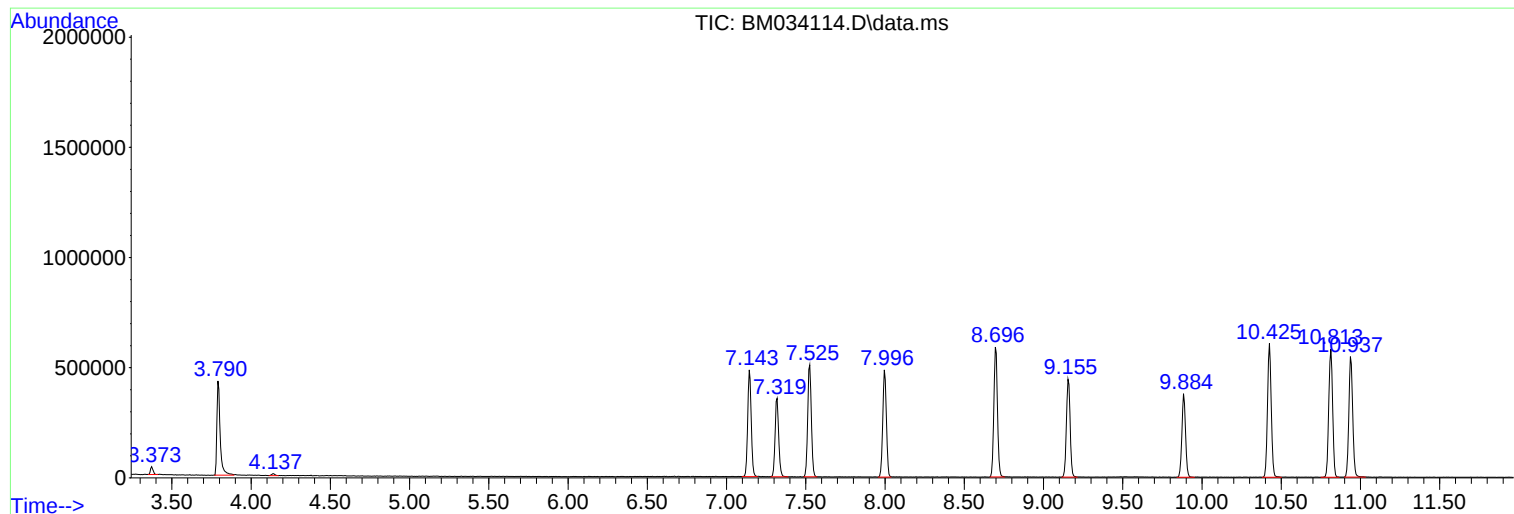

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030222\
Data File : BM034114.D
Acq On : 02 Mar 2022 12:50
Operator : CG/JU
Sample : PB142784BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK784

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030222\
Data File : BM034114.D
Acq On : 02 Mar 2022 12:50
Operator : CG/JU
Sample : PB142784BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK784

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc