

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030222\
 Data File : BM034116.D
 Acq On : 02 Mar 2022 14:02
 Operator : CG/JU
 Sample : PB142852BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK852

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022822.M
 Title : SVOA CALIBRATION

Signal : TIC: BM034116.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.372	20	23	32	rVB	36599	43433	1.58%	0.145%
2	3.790	90	94	114	rBV	416437	627156	22.88%	2.093%
3	4.143	150	154	160	rBV2	9492	13034	0.48%	0.043%
4	7.143	658	664	675	rBV	498986	773035	28.20%	2.580%
5	7.319	687	694	701	rBV	370468	576842	21.04%	1.925%
6	7.525	722	729	740	rVB	530099	836836	30.52%	2.793%
7	7.995	802	809	817	rBV	503732	787118	28.71%	2.627%
8	8.695	921	928	940	rBV	607874	969490	35.36%	3.235%
9	9.154	1000	1006	1016	rBV	457534	758446	27.67%	2.531%
10	9.884	1122	1130	1140	rBV	391055	632812	23.08%	2.112%
11	10.425	1215	1222	1233	rBV	641803	1031729	37.63%	3.443%
12	10.813	1280	1288	1296	rBV	609425	1021140	37.25%	3.408%
13	10.936	1302	1309	1321	rBV	576340	977314	35.65%	3.261%
14	12.401	1552	1558	1567	rVB	9811	16224	0.59%	0.054%
15	14.036	1830	1836	1843	rBV	1080461	1514189	55.23%	5.053%
16	14.324	1879	1885	1893	rBV	1161660	1733894	63.25%	5.786%
17	14.636	1931	1938	1950	rVB	905914	1354959	49.42%	4.522%
18	14.807	1960	1967	1986	rBV	451101	658432	24.02%	2.197%
19	14.983	1992	1997	2002	rBV7	1350	3342	0.12%	0.011%
20	15.454	2072	2077	2082	rVB5	1759	3086	0.11%	0.010%
21	15.624	2099	2106	2113	rBV	1518688	2185186	79.71%	7.292%
22	15.724	2118	2123	2132	rVV	427278	588193	21.45%	1.963%
23	15.860	2143	2146	2152	rVB3	6167	9156	0.33%	0.031%
24	17.160	2363	2367	2371	rBV	3602	5099	0.19%	0.017%
25	17.371	2397	2403	2413	rVB	1109762	1538722	56.13%	5.135%
26	17.471	2414	2420	2430	rBV	1669455	2320917	84.66%	7.745%
27	19.324	2731	2735	2740	rBV5	17699	23336	0.85%	0.078%
28	19.395	2744	2747	2750	rBV	17674	21581	0.79%	0.072%
29	19.701	2795	2799	2802	rBV6	6889	10800	0.39%	0.036%
30	19.759	2803	2809	2820	rVV	2006485	2686582	98.00%	8.966%
31	21.542	3107	3112	3119	rBV	1322280	1716696	62.62%	5.729%
32	23.836	3495	3502	3510	rBV2	1415177	2741534	100.00%	9.149%
33	23.994	3522	3529	3536	rVB2	872273	1785443	65.13%	5.958%




Sum of corrected areas: 29965756

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030222\
Data File : BM034116.D
Acq On : 02 Mar 2022 14:02
Operator : CG/JU
Sample : PB142852BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK852

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

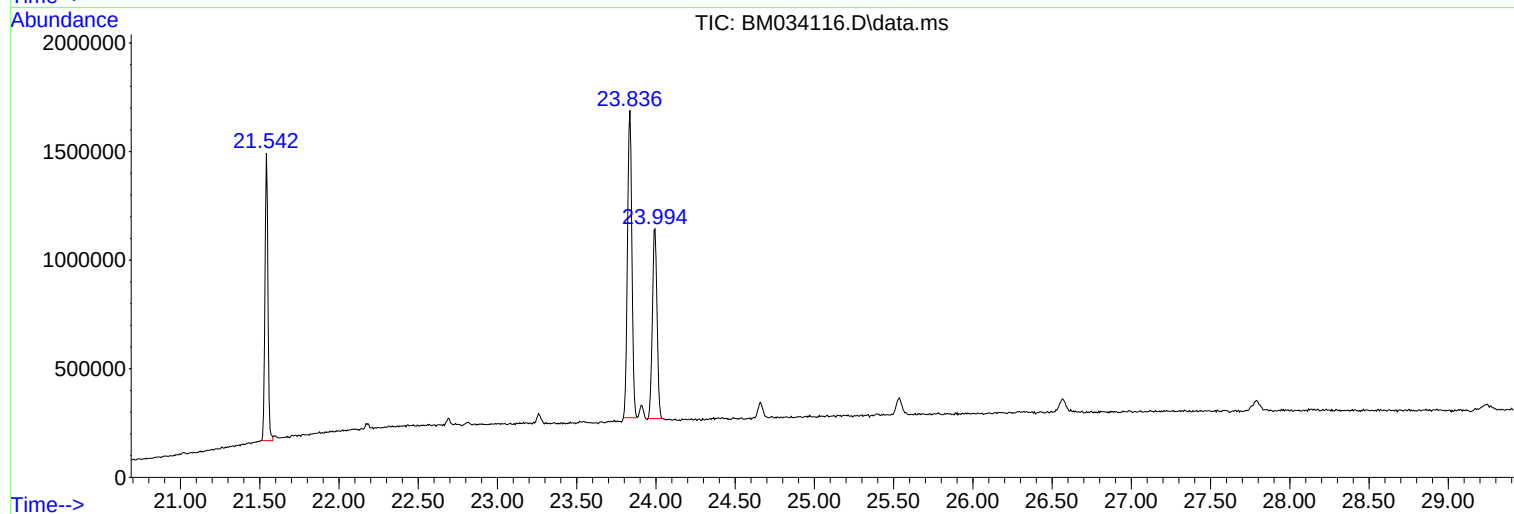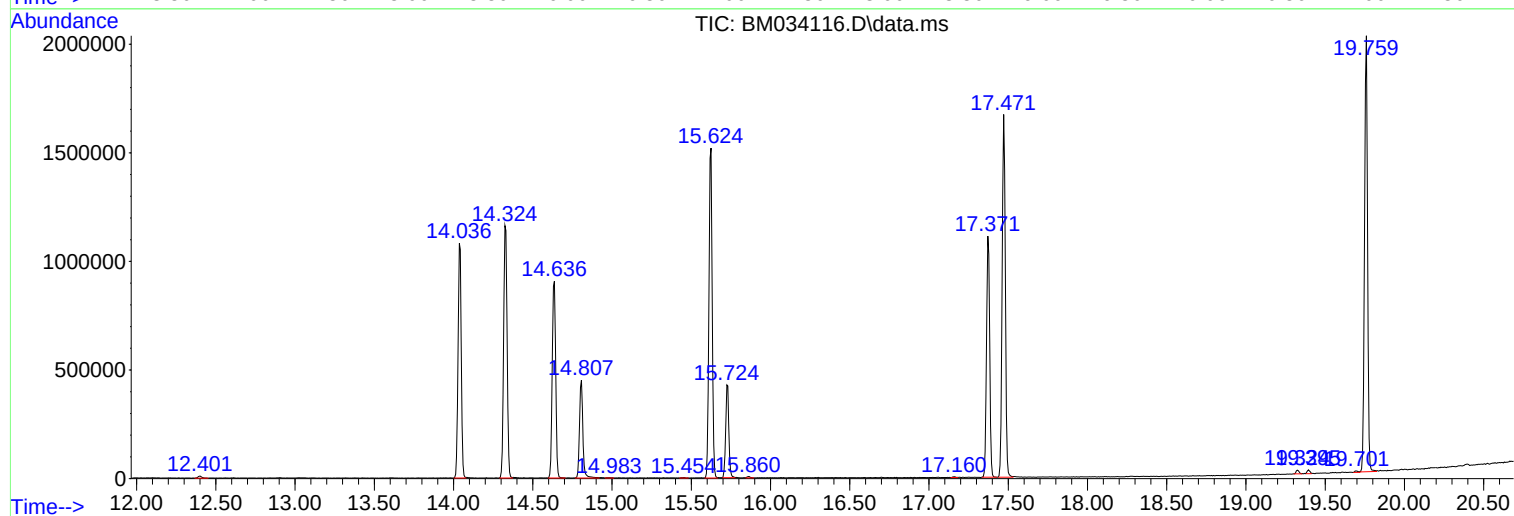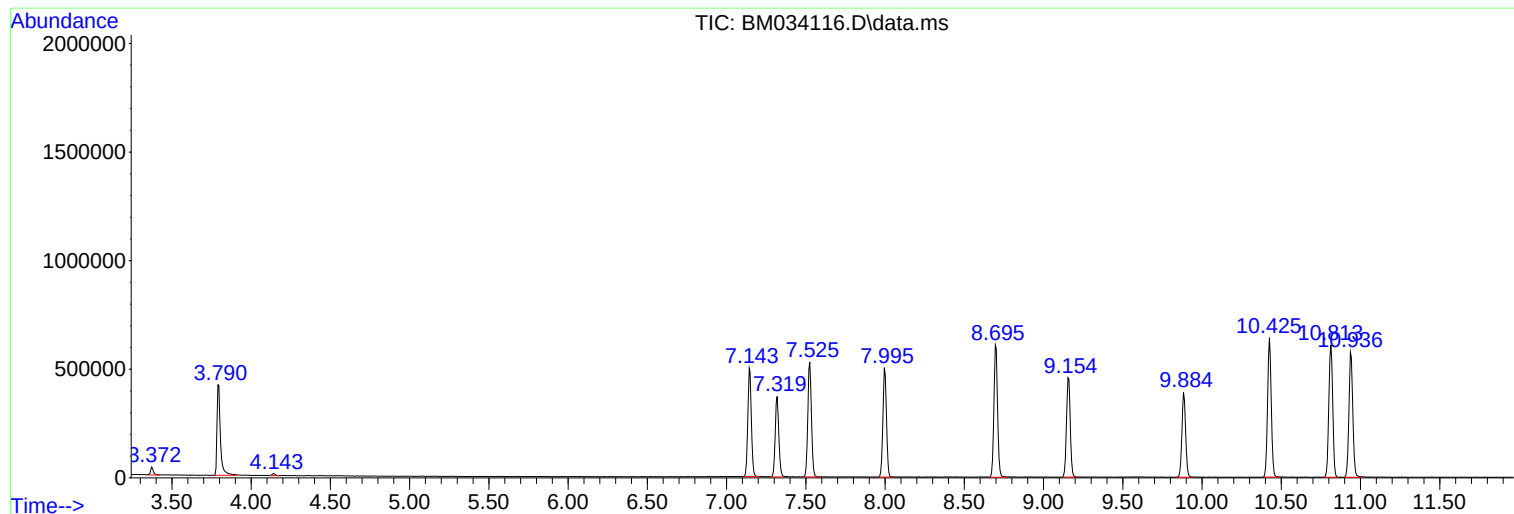

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030222\
Data File : BM034116.D
Acq On : 02 Mar 2022 14:02
Operator : CG/JU
Sample : PB142852BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK852

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030222\
Data File : BM034116.D
Acq On : 02 Mar 2022 14:02
Operator : CG/JU
Sample : PB142852BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK852

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------