


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030315\
 Data File : BM000616.D
 Acq On : 03 Mar 2015 15:03
 Operator : TP/IZ
 Sample : DFTPP29
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP29

Integration File: RTEINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-SIM-BM030315.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 04 02:50:23 2015

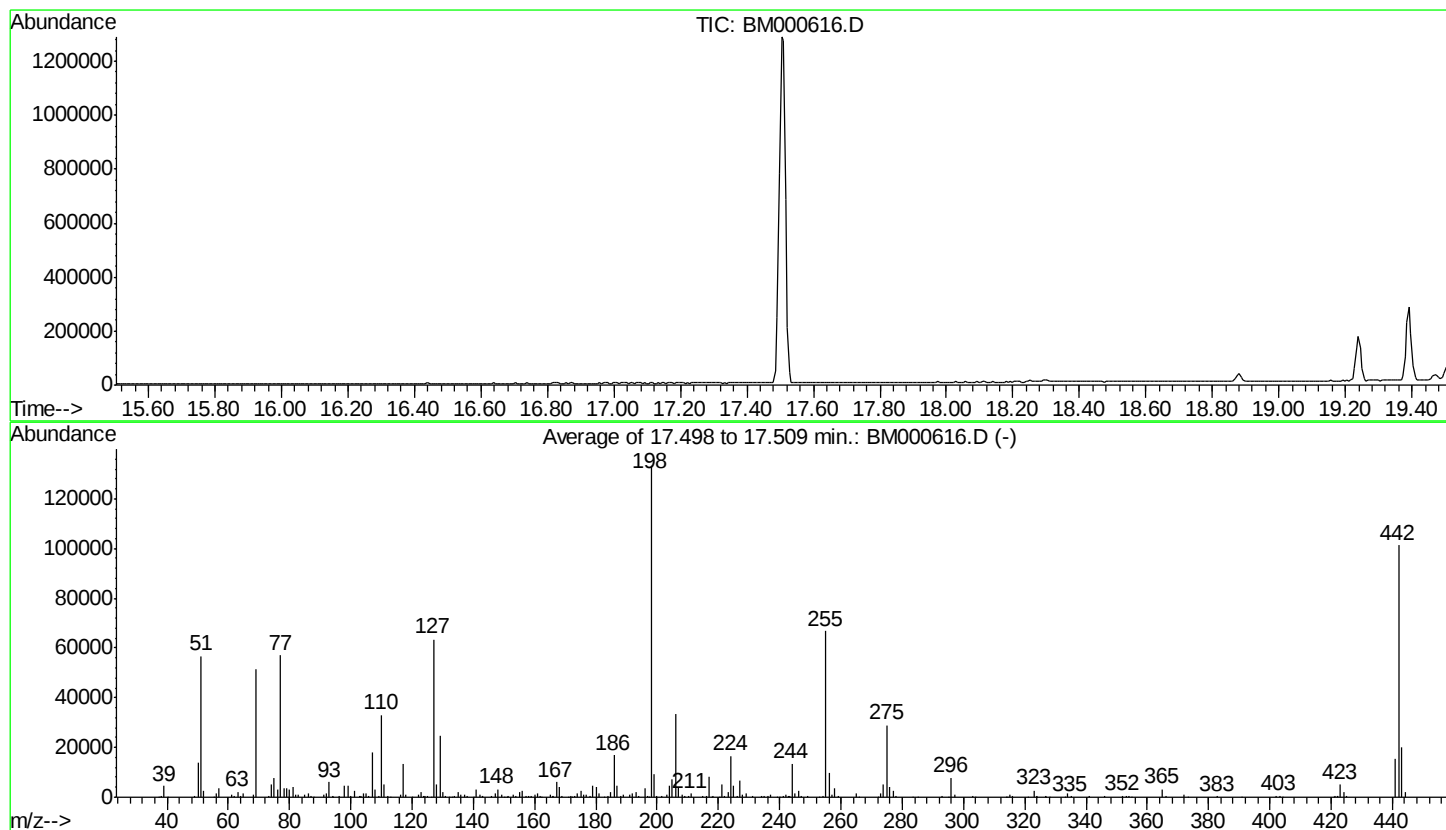

AutoFind: Scans 2518, 2519, 2520; Background Corrected with Scan 2512

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.5	56664	PASS
68	69	0.00	2	1.6	811	PASS
69	198	0.00	100	38.7	51632	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.6	63445	PASS
197	198	0.00	1	0.4	503	PASS
198	198	100	100	100.0	133301	PASS
199	198	5	9	6.9	9164	PASS
275	198	10	60	21.8	29056	PASS
365	198	1	100	2.5	3332	PASS
441	443	0.01	100	76.3	15430	PASS
442	198	50	100	75.9	101181	PASS
443	442	15	24	20.0	20212	PASS