


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030315\
 Data File : BM000616.D
 Acq On : 03 Mar 2015 15:03
 Operator : TP/IZ
 Sample : DFTPP29
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP29

Integration File: RTEINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-SIM-BM030315.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 04 02:50:23 2015

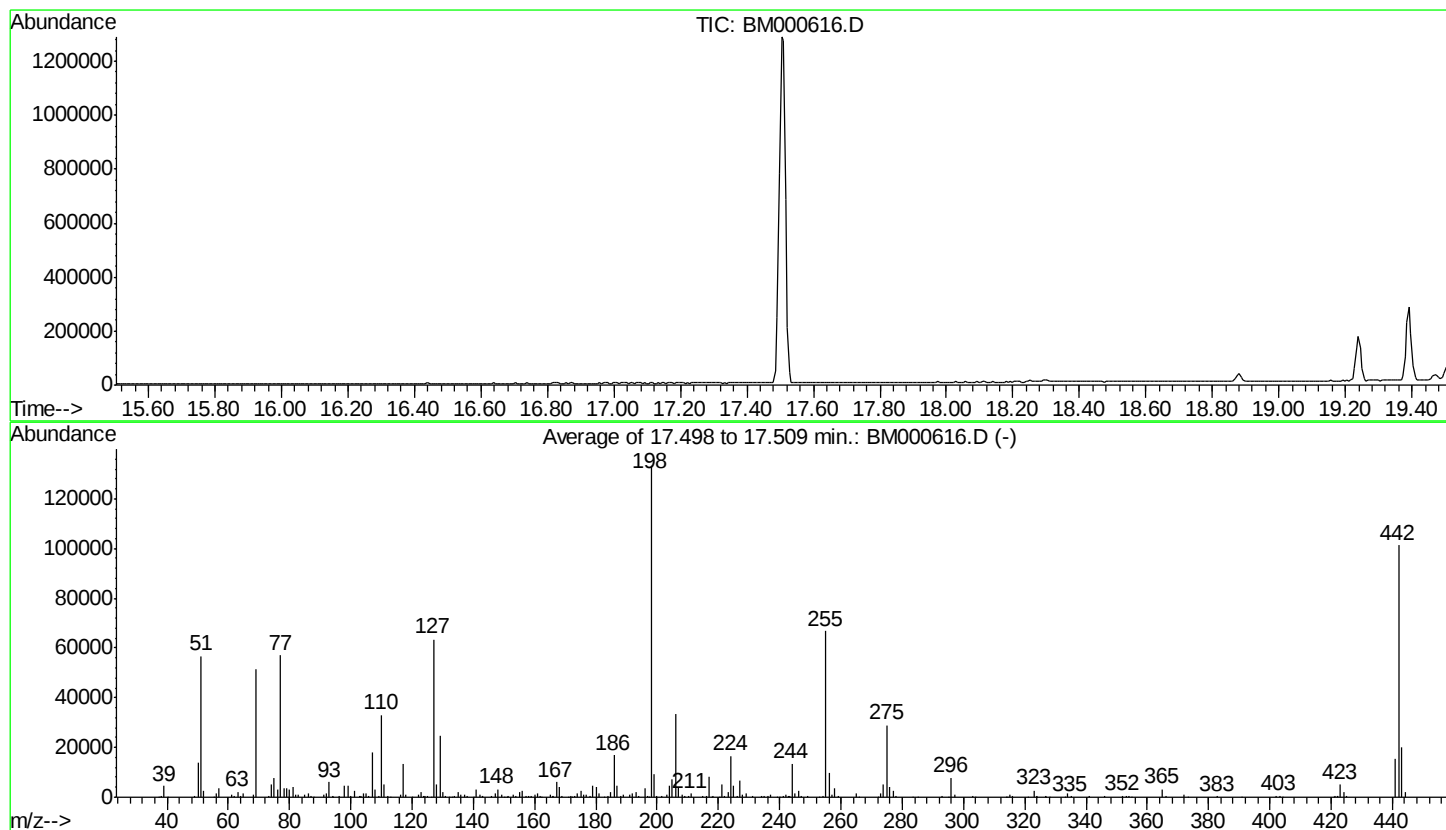

AutoFind: Scans 2518, 2519, 2520; Background Corrected with Scan 2512

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.5	56664	PASS
68	69	0.00	2	1.6	811	PASS
69	198	0.00	100	38.7	51632	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.6	63445	PASS
197	198	0.00	1	0.4	503	PASS
198	198	100	100	100.0	133301	PASS
199	198	5	9	6.9	9164	PASS
275	198	10	60	21.8	29056	PASS
365	198	1	100	2.5	3332	PASS
441	443	0.01	100	76.3	15430	PASS
442	198	50	100	75.9	101181	PASS
443	442	15	24	20.0	20212	PASS

m/z	Abundance
38.10	591.0
39.10	3828.0
40.00	1398.0
44.00	3288.0
49.20	374.0
50.10	11502.0
51.10	46616.0
52.00	2292.0
56.00	1277.0
57.00	2925.0
61.00	512.0
62.00	742.0
63.00	1768.0
64.00	513.0
65.10	1224.0
66.10	592.0
68.00	723.0
69.00	43176.0
73.10	818.0
74.00	4305.0
75.00	6225.0
76.10	2656.0
77.10	44008.0
78.10	3515.0
79.00	3013.0
80.00	2291.0
81.00	3545.0
82.00	1009.0
82.90	692.0
85.00	877.0
86.00	1136.0
87.00	365.0
91.00	758.0
92.00	1229.0
93.10	5082.0
93.90	505.0
96.10	464.0
98.00	4397.0
99.00	3765.0
101.00	2113.0
102.90	671.0
104.00	1131.0
105.00	1422.0
106.00	355.0
107.00	13664.0
108.00	2339.0
108.90	326.0
110.00	25600.0
111.00	4528.0
112.00	411.0
116.00	782.0
117.00	10676.0
118.00	829.0
122.00	854.0
123.00	1262.0
123.90	741.0
125.00	676.0
127.00	47984.0
128.00	3869.0
129.00	17552.0
130.00	1689.0
130.90	337.0
133.90	654.0
135.00	1482.0
136.00	624.0
137.10	1066.0
141.00	2070.0
142.00	898.0
142.80	462.0
146.00	358.0
147.10	1370.0
148.00	2519.0
149.10	746.0
150.90	301.0
152.90	689.0
154.00	502.0
154.90	1173.0
156.00	1825.0
157.20	507.0
157.90	334.0
159.10	324.0
160.00	841.0
161.00	1099.0
161.80	312.0
164.90	913.0
165.90	612.0
167.10	4252.0
168.00	3512.0
168.90	539.0
171.90	610.0
174.10	879.0

Instrument :
BNA_M
ClientSampleId :
DFTPP29

175.00	1892.0
176.10	720.0
176.90	716.0
177.90	328.0
179.00	3256.0
180.00	3224.0
181.00	891.0
185.00	1506.0
186.00	12190.0
187.10	3444.0
188.10	605.0
189.00	789.0
191.00	797.0
192.00	1165.0
193.00	1668.0
193.90	301.0
196.10	2538.0
198.00	92832.0
199.00	7085.0
199.90	626.0
201.50	508.0
202.90	668.0
204.10	3933.0
205.00	5430.0
206.10	22512.0
207.10	4645.0
208.00	794.0
209.00	550.0
210.10	604.0
211.10	941.0
215.00	320.0
216.00	525.0
217.00	5943.0
217.90	547.0
221.10	3500.0
223.10	1244.0
224.10	10406.0
225.00	3220.0
225.90	604.0
227.00	4290.0
228.10	648.0
229.00	1182.0
231.00	552.0
235.10	366.0
236.90	547.0
240.00	341.0
241.90	527.0
243.00	587.0
244.10	9367.0
245.10	1044.0
246.10	1746.0
249.00	428.0
255.00	44424.0
256.00	6496.0
257.00	569.0
258.00	2077.0
259.00	422.0
264.90	1103.0
273.00	1143.0
273.90	3028.0
275.10	18200.0
276.10	2523.0
277.00	1285.0
293.00	381.0
296.00	4474.0
297.10	675.0
302.90	496.0
314.00	326.0
315.00	636.0
316.00	349.0
323.10	1522.0
323.80	351.0
326.80	315.0
334.10	915.0
352.00	532.0
353.00	343.0
354.00	664.0
365.00	2021.0
366.00	365.0
372.00	647.0
402.00	331.0
403.10	518.0
420.90	405.0
421.90	662.0
423.10	2542.0
424.10	1731.0
425.00	426.0
441.00	7516.0
442.10	48544.0
443.00	9901.0
444.10	1125.0

Instrument :
BNA_M
ClientSampleId :
DFTPP29

m/z	Abundance
37.10	305.0
38.10	786.0
39.10	4696.0
40.00	1254.0
44.00	3404.0
49.00	647.0
50.10	15360.0
51.10	66800.0
52.10	3385.0
55.00	364.0
56.00	1730.0
57.00	3806.0
61.10	971.0
62.00	727.0
63.10	2769.0
63.90	716.0
65.10	1592.0
65.90	412.0
68.00	974.0
69.00	60752.0
73.00	841.0
74.10	6125.0
75.00	9577.0
76.10	3335.0
77.10	67920.0
78.10	4584.0
79.00	3908.0
80.00	3477.0
81.00	4550.0
82.00	975.0
83.00	1603.0
85.10	925.0
86.00	1615.0
86.90	731.0
91.00	1137.0
92.00	1481.0
93.00	7176.0
93.90	518.0
96.10	745.0
98.00	5091.0
99.10	5328.0
99.90	407.0
101.00	2853.0
103.10	1207.0
104.00	1704.0
105.00	1268.0
105.90	536.0
107.00	21360.0
108.00	3853.0
108.90	465.0
110.00	36824.0
111.00	6138.0
112.00	788.0
113.10	372.0
116.10	1227.0
117.00	15348.0
118.00	1051.0
120.00	349.0
122.00	1240.0
123.00	2338.0
124.10	785.0
125.00	870.0
126.10	347.0
127.00	73136.0
128.10	5731.0
129.00	30008.0
130.00	2216.0
131.00	339.0
132.00	319.0
132.90	356.0
134.00	673.0
135.10	2576.0
135.90	899.0
137.00	1288.0
137.80	509.0
140.00	332.0
141.00	3481.0
142.00	1584.0
143.00	772.0
146.00	691.0
147.00	1945.0
148.10	3729.0
149.10	1123.0
150.00	451.0
151.20	457.0
153.00	1431.0
154.00	698.0
155.00	2199.0
156.10	2643.0
157.00	597.0
157.90	574.0

Instrument :
BNA_M
ClientSampleId :
DFTPP29

158.90	678.0
160.00	1129.0
161.00	1700.0
161.90	599.0
165.00	1601.0
166.10	994.0
167.10	7123.0
168.10	4716.0
169.00	451.0
171.90	723.0
173.00	967.0
174.00	1650.0
175.10	2843.0
176.00	825.0
177.00	1177.0
177.90	554.0
179.00	6178.0
180.00	4161.0
181.00	1704.0
183.90	425.0
185.00	2432.0
186.00	19712.0
187.10	5436.0
188.00	938.0
189.00	1623.0
190.90	922.0
192.00	1757.0
193.00	2031.0
193.90	472.0
196.00	4335.0
196.80	696.0
197.10	714.0
198.00	154496.0
199.00	10433.0
200.00	850.0
201.40	891.0
203.00	924.0
204.00	5211.0
205.00	8250.0
206.10	39288.0
207.10	6983.0
208.00	1477.0
209.00	761.0
210.00	611.0
211.10	1739.0
215.10	700.0
216.10	1004.0
217.00	9923.0
218.10	1146.0
220.20	337.0
221.10	6021.0
223.00	2081.0
224.10	19288.0
225.10	5268.0
226.00	767.0
227.00	7147.0
227.90	982.0
229.00	1481.0
231.00	833.0
234.00	554.0
234.90	627.0
236.10	462.0
237.00	1424.0
239.10	305.0
241.00	542.0
241.90	784.0
243.20	979.0
244.10	15143.0
245.10	2176.0
246.00	3453.0
247.00	802.0
248.80	593.0
252.90	492.0
254.00	624.0
255.00	78160.0
256.00	11494.0
257.10	1265.0
258.10	4253.0
258.90	658.0
265.00	1505.0
272.00	300.0
273.10	2334.0
274.00	6146.0
275.00	33432.0
276.00	4706.0
277.00	2942.0
277.90	610.0
283.20	370.0
285.10	359.0
293.00	526.0
295.00	330.0
296.00	9103.0
297.00	1358.0
302.80	620.0
315.00	1012.0

Instrument :
BNA_M
ClientSampleId :
DFTPP29

315.90	429.0
323.10	3334.0
324.10	732.0
327.00	504.0
334.00	1905.0
335.00	688.0
341.00	527.0
345.90	512.0
352.00	791.0
353.00	517.0
354.10	805.0
365.00	3531.0
366.00	653.0
372.00	1501.0
383.00	439.0
402.00	692.0
403.10	815.0
421.10	1045.0
421.90	717.0
423.00	5955.0
424.10	2466.0
425.00	686.0
441.00	17704.0
442.00	112664.0
443.00	22368.0
444.00	2060.0

Instrument :
BNA_M
ClientSampleId :
DFTPP29

m/z	Abundance
38.10	715.0
39.10	4813.0
40.00	1260.0
44.00	3450.0
49.10	651.0
50.10	14543.0
51.10	56576.0
52.00	2783.0
55.10	347.0
56.00	1770.0
57.00	3715.0
61.10	990.0
61.90	786.0
63.00	2409.0
64.00	616.0
65.00	1369.0
66.00	385.0
68.00	736.0
69.00	50968.0
73.00	1074.0
74.10	5274.0
75.00	8112.0
76.10	2862.0
77.10	58944.0
78.10	3172.0
79.00	3923.0
80.00	3240.0
81.00	4590.0
82.00	1083.0
83.00	1146.0
84.90	800.0
86.00	1442.0
87.00	759.0
87.90	348.0
91.00	782.0
92.00	1291.0
93.00	6117.0
94.10	360.0
96.00	300.0
98.00	4922.0
99.00	4414.0
99.90	435.0
101.00	2748.0
102.90	825.0
104.00	1586.0
105.00	1656.0
105.90	411.0
107.00	19544.0
108.00	3018.0
109.00	496.0
110.00	36432.0
111.00	5190.0
111.90	696.0
116.00	1505.0
117.10	14703.0
118.10	747.0
122.00	1345.0
123.00	2259.0
123.80	527.0
124.10	538.0
124.90	733.0
126.20	322.0
127.00	69216.0
128.00	5371.0
129.00	27176.0
130.00	2008.0
131.00	448.0
134.00	725.0
135.00	1996.0
135.90	1159.0
137.10	1368.0
137.80	332.0
139.90	338.0
141.00	3575.0
141.90	902.0
142.80	489.0
143.10	613.0
146.10	685.0
147.10	1555.0
147.90	3324.0
149.00	814.0
151.30	559.0
152.90	1038.0
154.00	798.0
155.00	2132.0
156.00	2545.0
157.00	449.0
158.00	584.0
158.80	457.0
160.00	1330.0
161.00	1716.0

Instrument :
BNA_M
ClientSampleId :
DFTPP29

162.10	565.0
165.00	1332.0
165.90	1349.0
167.10	6518.0
168.00	4295.0
169.00	680.0
170.80	383.0
172.10	785.0
173.00	846.0
174.10	1470.0
175.10	2677.0
176.10	989.0
177.00	1462.0
177.90	535.0
179.00	4921.0
180.00	4503.0
181.00	1926.0
182.80	401.0
184.00	557.0
184.90	2130.0
186.00	18376.0
187.00	5466.0
188.00	585.0
188.90	1154.0
190.80	695.0
192.00	1853.0
193.10	2245.0
193.90	305.0
196.10	3814.0
196.90	815.0
198.00	152576.0
199.00	9975.0
200.00	779.0
201.60	682.0
203.00	1104.0
204.00	5267.0
205.00	8402.0
206.10	38552.0
207.00	6334.0
207.90	1304.0
208.90	660.0
210.20	681.0
210.90	1481.0
214.90	402.0
215.90	694.0
217.00	9454.0
218.00	1126.0
221.00	6037.0
221.90	1273.0
223.00	2302.0
224.10	20232.0
225.00	5016.0
226.00	661.0
227.00	8416.0
228.00	1065.0
229.00	1675.0
231.00	982.0
234.00	729.0
234.90	773.0
236.00	386.0
237.10	934.0
239.90	345.0
241.00	549.0
242.00	1149.0
243.00	926.0
244.10	15799.0
245.10	1997.0
246.00	2934.0
247.00	324.0
249.00	558.0
253.00	322.0
253.90	629.0
255.00	77544.0
256.00	12173.0
256.90	833.0
258.00	4284.0
259.10	881.0
265.00	1862.0
265.80	513.0
273.00	1885.0
274.00	5731.0
275.00	35536.0
276.10	4638.0
277.00	3154.0
277.90	600.0
284.90	385.0
292.90	770.0
294.90	302.0
296.00	10025.0
297.00	1629.0
303.00	1095.0
303.90	371.0
313.80	429.0
314.20	330.0
314.90	877.0

Instrument :
BNA_M
ClientSampleId :
DFTPP29

316.00	595.0
321.00	336.0
323.10	3344.0
324.00	441.0
326.80	968.0
328.10	412.0
333.00	386.0
333.90	2172.0
335.10	617.0
341.00	542.0
345.90	668.0
352.00	849.0
353.10	835.0
354.10	816.0
355.00	335.0
365.00	4446.0
366.00	599.0
372.00	1655.0
373.10	365.0
382.80	485.0
390.80	301.0
401.90	842.0
403.10	952.0
404.00	520.0
421.00	1052.0
422.10	1087.0
423.10	6259.0
424.10	2801.0
425.10	370.0
441.00	21072.0
442.00	142336.0
443.10	28368.0
444.10	2610.0

Instrument :
BNA_M
ClientSampleId :
DFTPP29

m/z	Abundance
40.00	1191.0
44.00	3433.0
66.00	611.0
73.10	471.0
207.10	2088.0

Instrument :
BNA_M
ClientSampleId :
DFTPP29