

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030317\
 Data File : BM009076.D
 Acq On : 03 Mar 2017 20:01
 Operator : SJ/MA
 Sample : I2051-05
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AE1

Quant Time: Mar 03 23:59:48 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 03 23:57:02 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.90	152	162	0.40	ng/ul	0.00
2) Naphthalene-d8	10.69	136	486	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.52	164	301	0.40	ng/ul	-0.02
10) Phenanthrene-d10	17.36	188	60850	0.40	ng/ul	0.09
16) Chrysene-d12	21.45	240	760	0.40	ng/ul	0.00
20) Perylene-d12	23.64	264	59329	0.40	ng/ul	-0.15
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.28	152	250	0.31	ng/ul	0.00
14) Fluoranthene-d10	19.30	212	703	0.00	ng/ul	0.00
Target Compounds						
9) Fluorene	15.53	166	131	0.09	ng/ul#	41
17) Pyrene	19.67	202	150	0.06	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030317\
Data File : BM009076.D
Acq On : 03 Mar 2017 20:01
Operator : SJ/MA
Sample : I2051-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AE1

Quant Time: Mar 03 23:59:48 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 03 23:57:02 2017
Response via : Initial Calibration

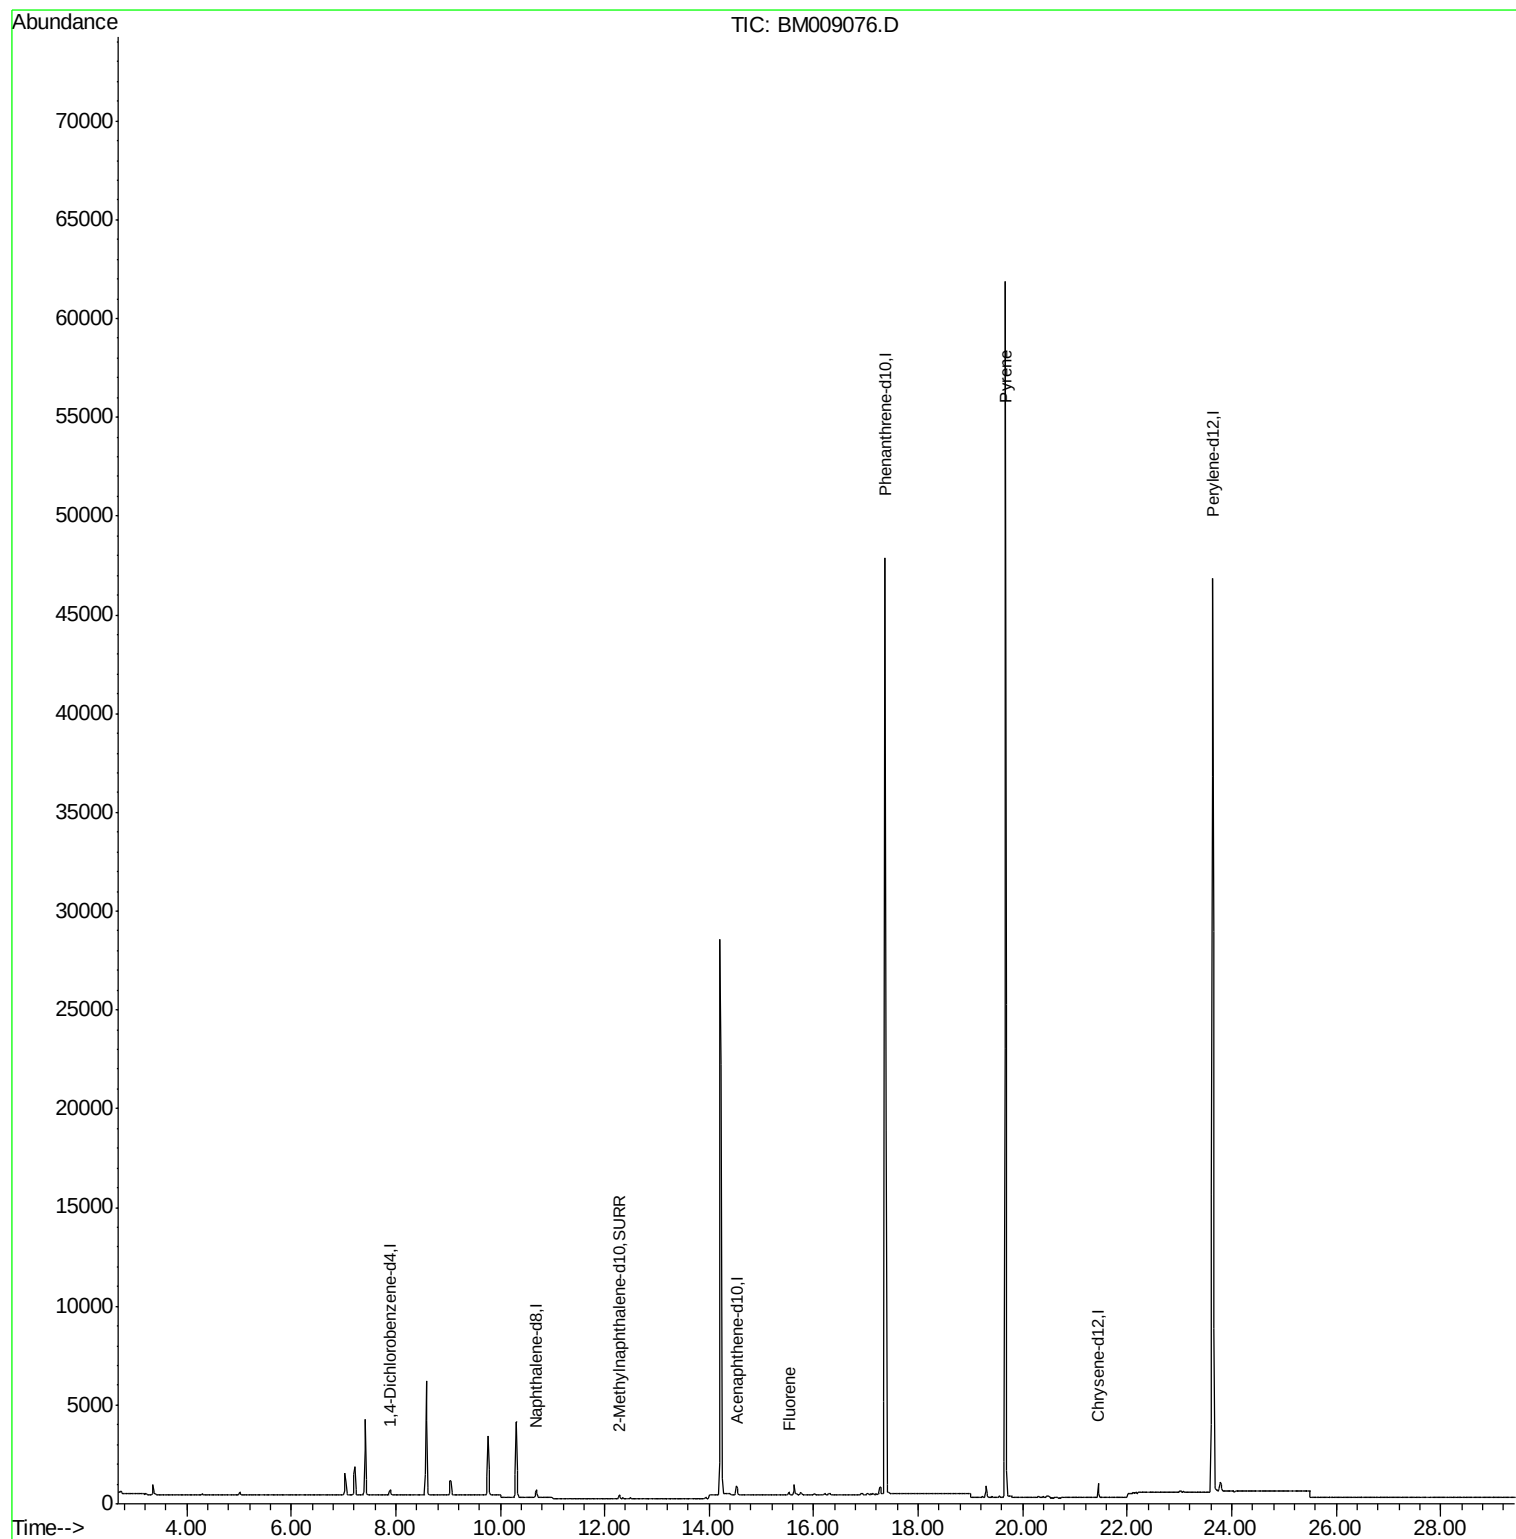

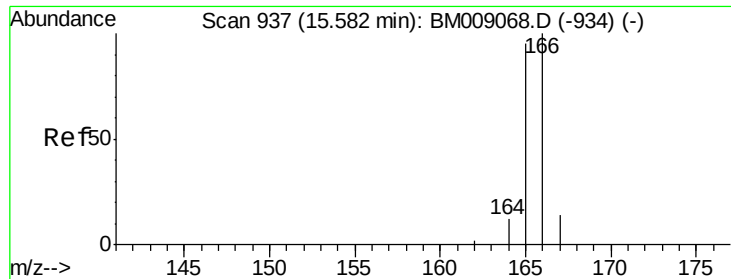

#9

Fluorene

Concen: 0.09 ng/ul

RT: 15.53 min Scan# 934

Delta R.T. -0.05 min

Lab File: BM009076.D

Acq: 03 Mar 2017 20:01

Instrument :

BNA_M

ClientSampleId :

C0AE1





Tgt Ion:166 Resp: 131

Ion Ratio Lower Upper

166 100

165 44.8 73.4 110.2#

167 65.5 14.6 22.0#

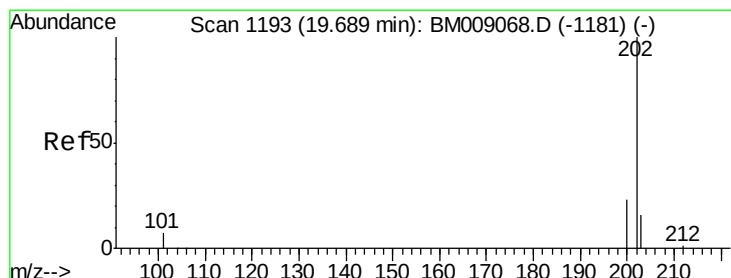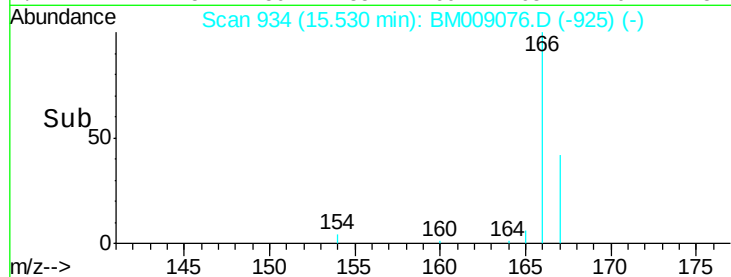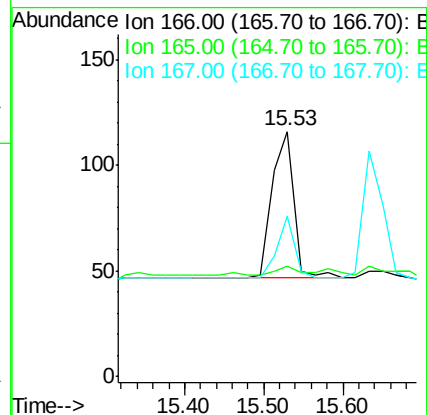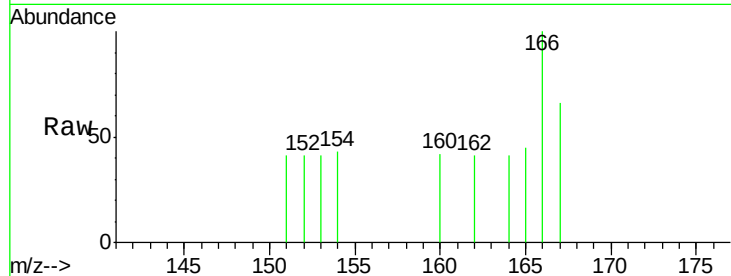

#17

Pyrene

Concen: 0.06 ng/ul

RT: 19.67 min Scan# 1191

Delta R.T. -0.02 min

Lab File: BM009076.D

Acq: 03 Mar 2017 20:01

Tgt Ion:202 Resp: 150

Ion Ratio Lower Upper

202 100

200 34.2 18.2 27.4#

203 150.7 15.6 23.4#

