

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030317\
 Data File : BM009077.D
 Acq On : 03 Mar 2017 20:38
 Operator : SJ/MA
 Sample : I2051-06
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AE2

Quant Time: Mar 03 23:59:52 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 03 23:57:02 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.90	152	160	0.40	ng/ul	0.00
2) Naphthalene-d8	10.69	136	483	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.52	164	284	0.40	ng/ul	-0.02
10) Phenanthrene-d10	17.36	188	54873	0.40	ng/ul	0.09
16) Chrysene-d12	21.45	240	747	0.40	ng/ul	0.00
20) Perylene-d12	23.64	264	55652	0.40	ng/ul	-0.15
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.28	152	245	0.31	ng/ul	0.00
14) Fluoranthene-d10	19.30	212	637	0.00	ng/ul	0.00
Target Compounds						
9) Fluorene	15.53	166	117	0.09	ng/ul#	44
17) Pyrene	19.67	202	168	0.07	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030317\
Data File : BM009077.D
Acq On : 03 Mar 2017 20:38
Operator : SJ/MA
Sample : I2051-06
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AE2

Quant Time: Mar 03 23:59:52 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 03 23:57:02 2017
Response via : Initial Calibration

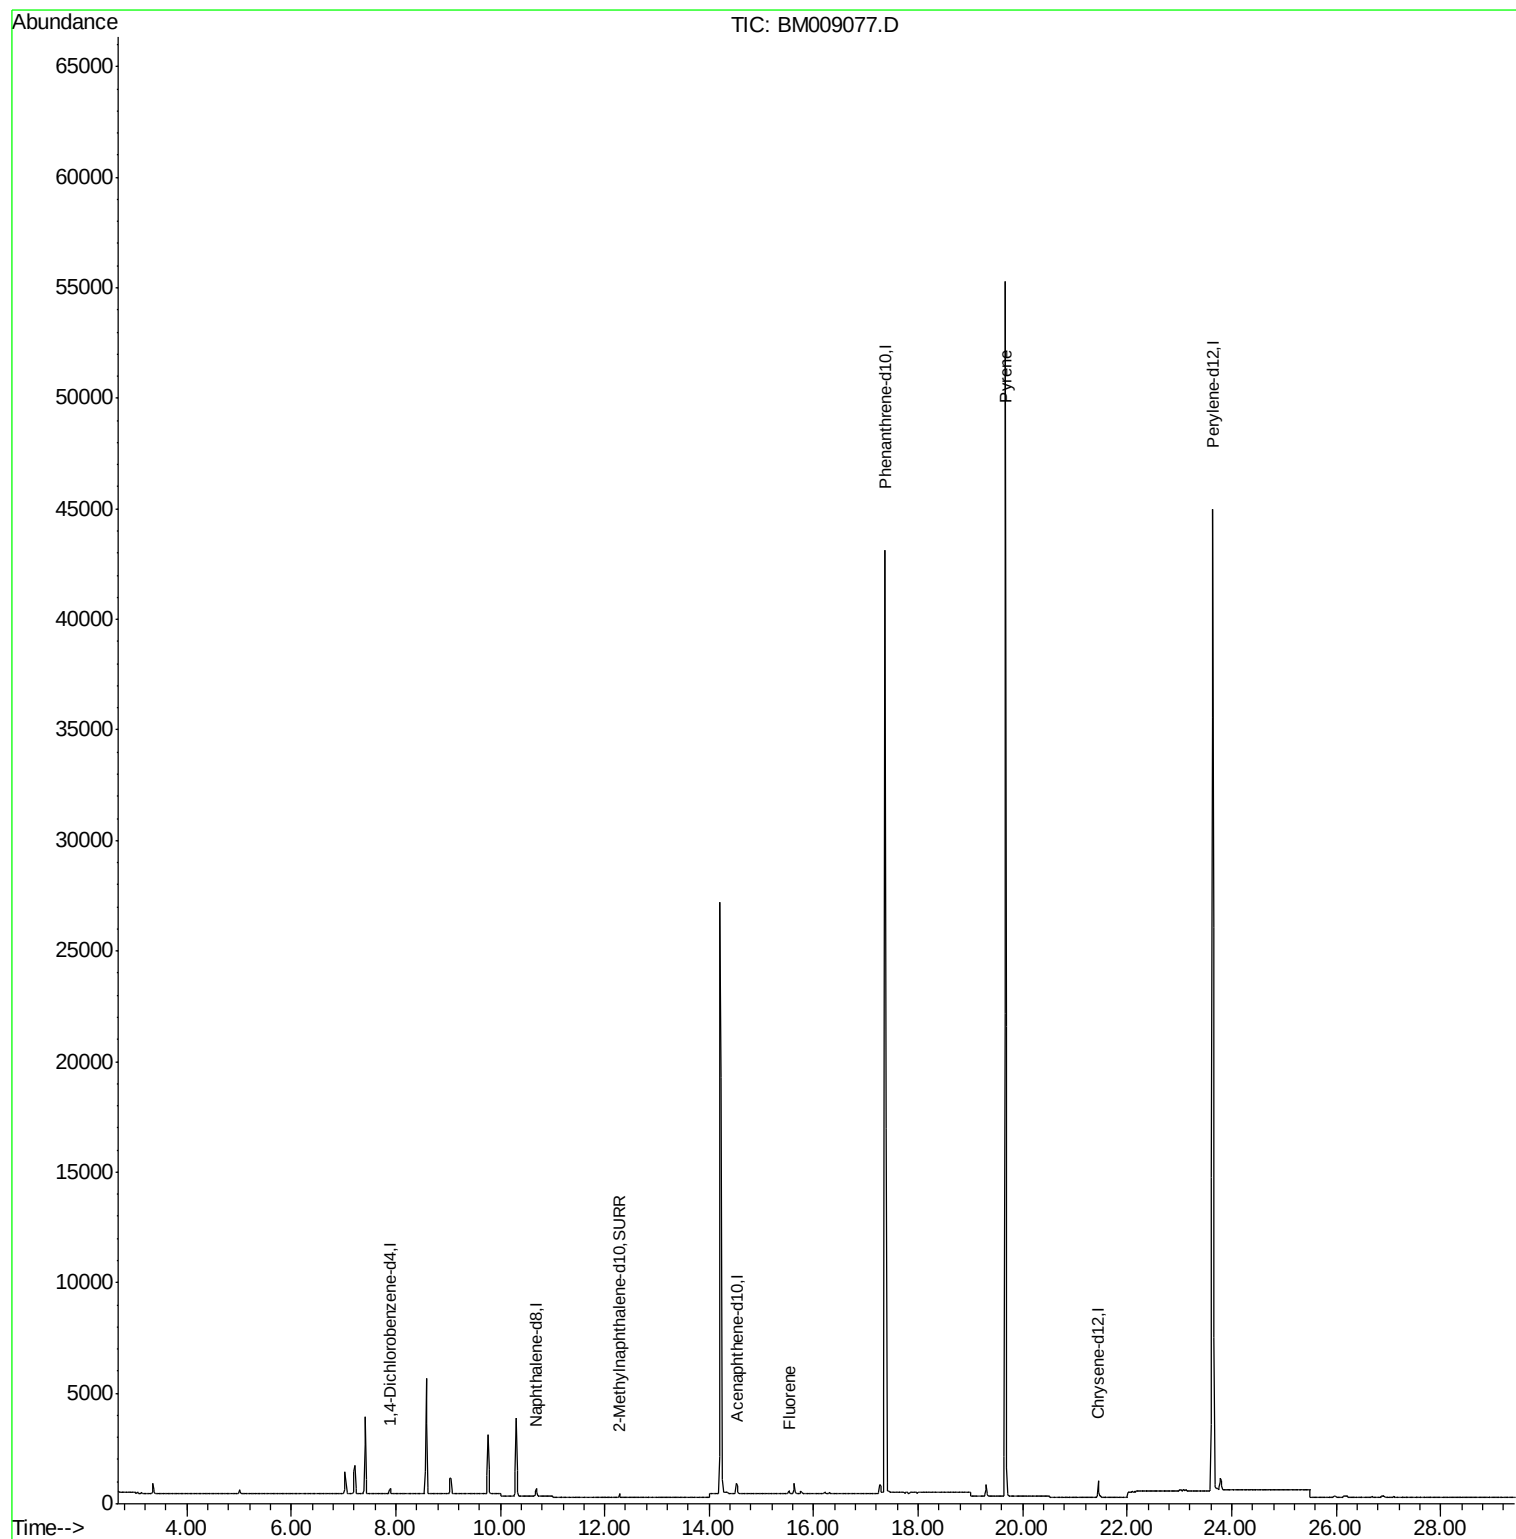

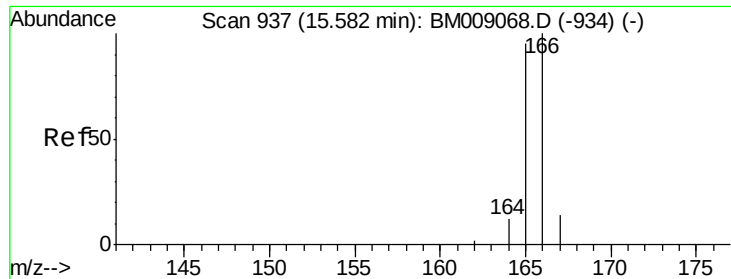

#9

Fluorene

Concen: 0.09 ng/ul

RT: 15.53 min Scan# 934

Delta R.T. -0.05 min

Lab File: BM009077.D

Acq: 03 Mar 2017 20:38

Instrument :

BNA_M

ClientSampleId :

C0AE2


Tgt Ion:166 Resp: 117

Ion Ratio Lower Upper

166 100

165 48.6 73.4 110.2#




167 67.3 14.6 22.0#

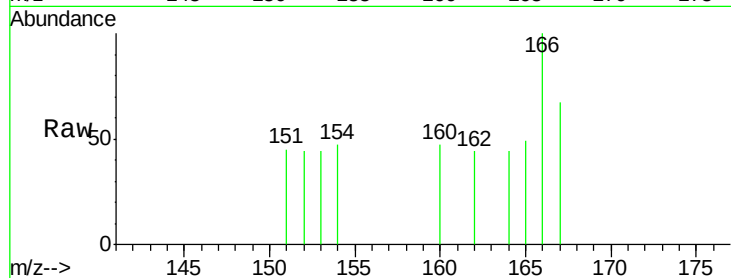

Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

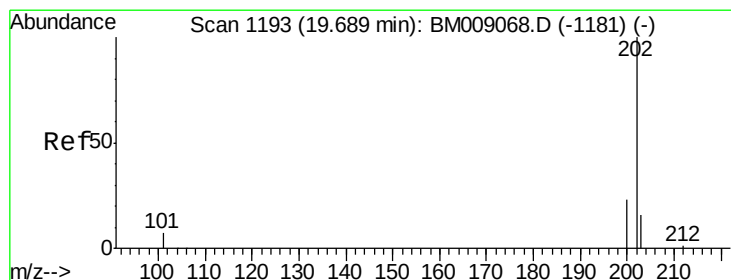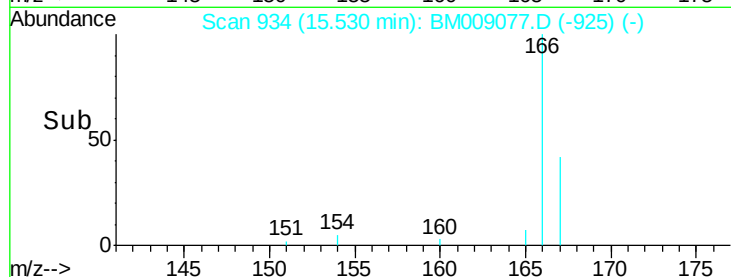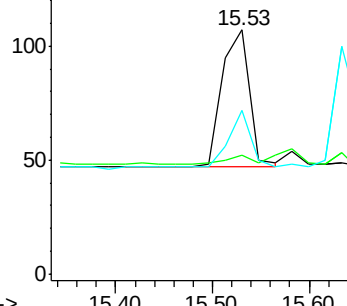

#17

Pyrene

Concen: 0.07 ng/ul

RT: 19.67 min Scan# 1191

Delta R.T. -0.02 min

Lab File: BM009077.D

Acq: 03 Mar 2017 20:38


Tgt Ion:202 Resp: 168

Ion Ratio Lower Upper

202 100

200 36.3 18.2 27.4#

203 153.3 15.6 23.4#

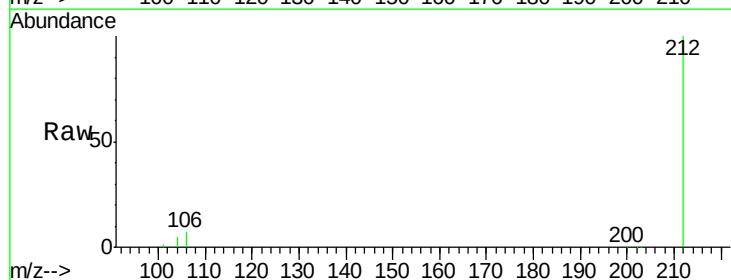

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 200.00 (199.70 to 200.70): E

Ion 203.00 (202.70 to 203.70): E

