

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030317\
 Data File : BM009079.D
 Acq On : 03 Mar 2017 21:50
 Operator : SJ/MA
 Sample : I2051-08
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AF1

Quant Time: Mar 04 00:00:01 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 03 23:57:02 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.90	152	158	0.40	ng/ul	0.00
2) Naphthalene-d8	10.69	136	478	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.52	164	296	0.40	ng/ul	-0.02
10) Phenanthrene-d10	17.36	188	49793	0.40	ng/ul	0.09
16) Chrysene-d12	21.45	240	704	0.40	ng/ul	0.00
20) Perylene-d12	23.64	264	48880	0.40	ng/ul	-0.15
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.28	152	217	0.27	ng/ul	0.00
14) Fluoranthene-d10	19.30	212	564	0.00	ng/ul	0.00
Target Compounds						
9) Fluorene	15.53	166	104	0.08	ng/ul#	44
17) Pyrene	19.66	202	129	0.05	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030317\
Data File : BM009079.D
Acq On : 03 Mar 2017 21:50
Operator : SJ/MA
Sample : I2051-08
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF1

Quant Time: Mar 04 00:00:01 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 03 23:57:02 2017
Response via : Initial Calibration

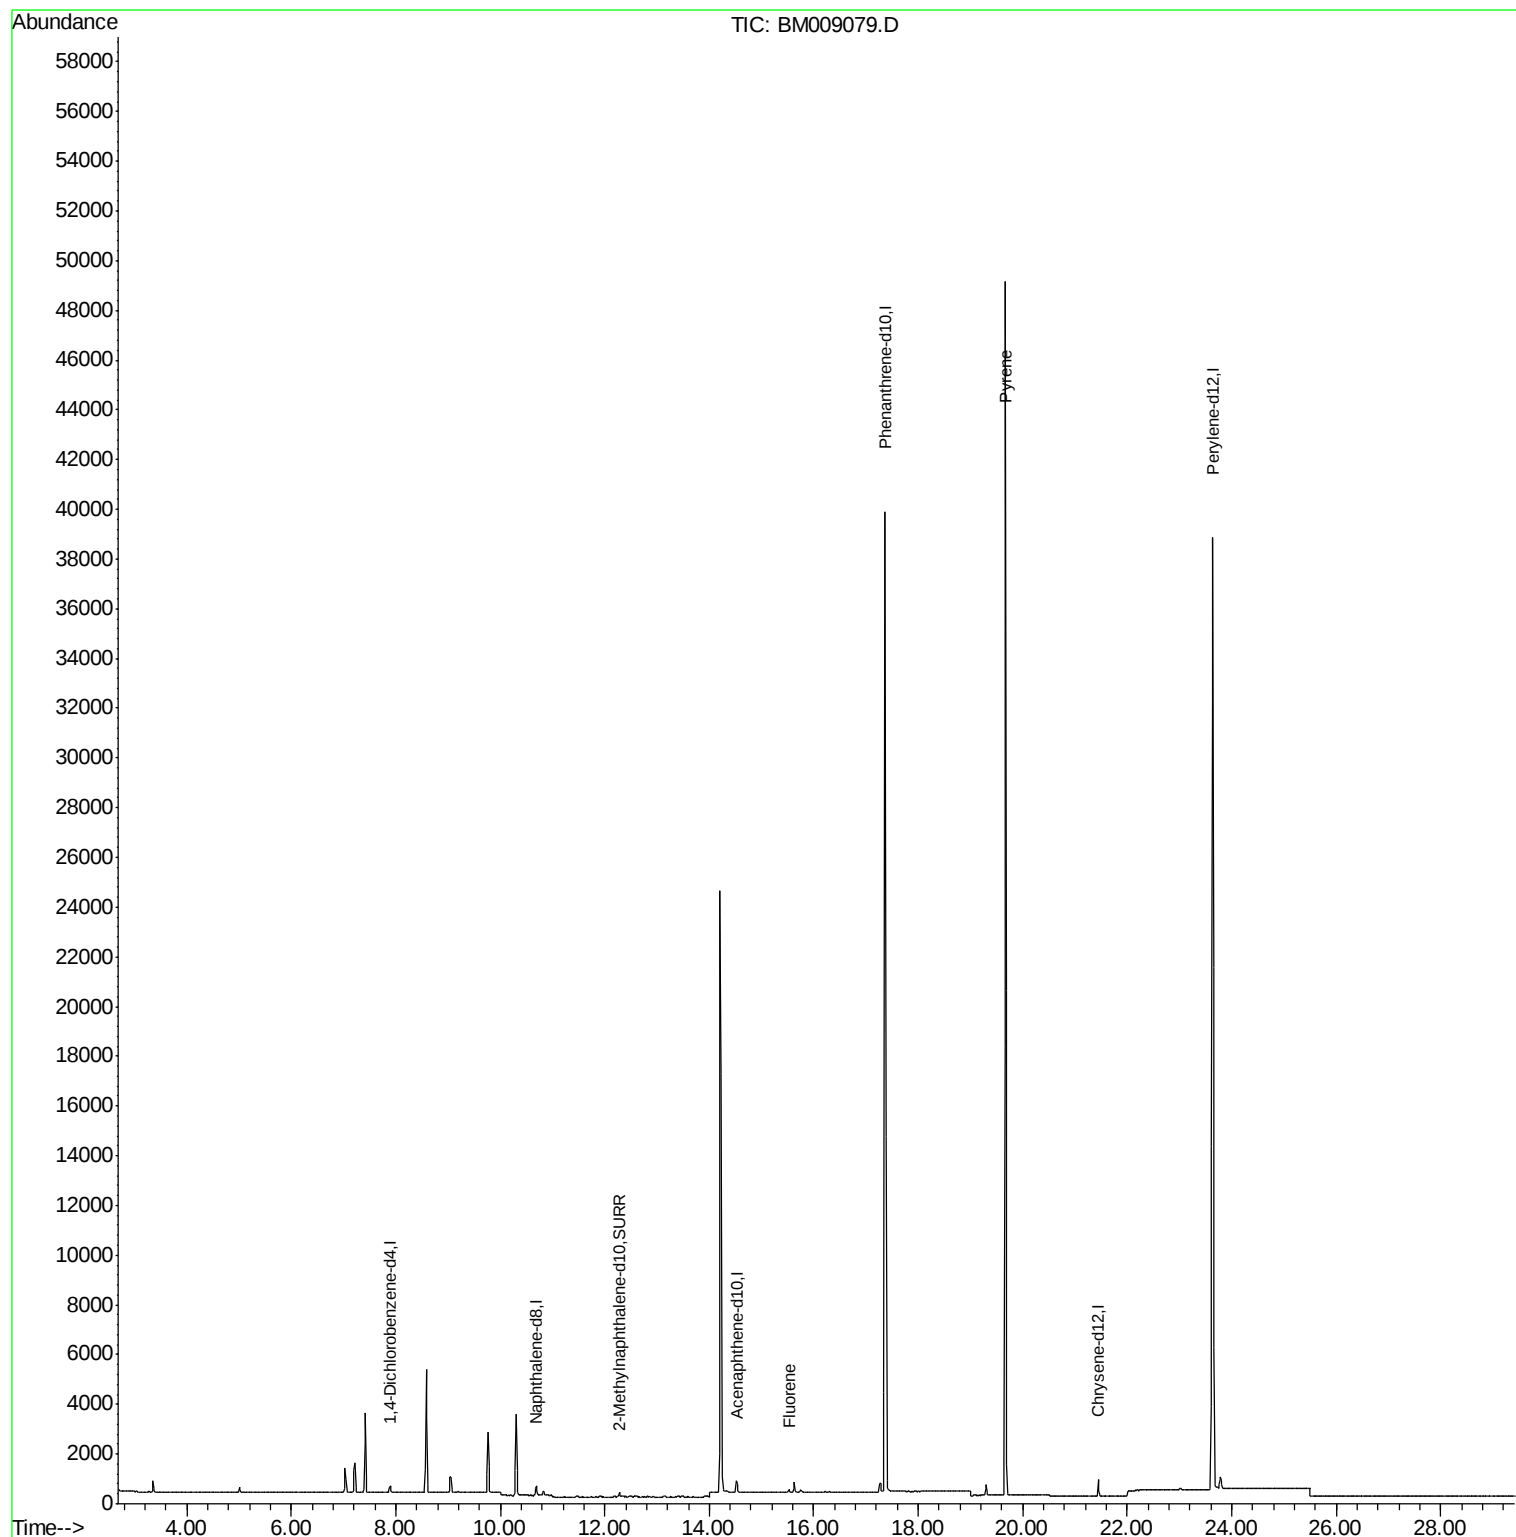

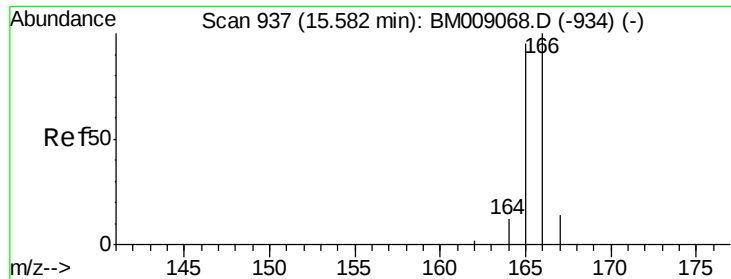

#9

Fluorene

Concen: 0.08 ng/ul

RT: 15.53 min Scan# 934

Delta R.T. -0.05 min

Lab File: BM009079.D

Acq: 03 Mar 2017 21:50

Instrument :

BNA_M

ClientSampleId :

C0AF1





Tgt Ion:166 Resp: 104

Ion Ratio Lower Upper

166 100

165 49.5 73.4 110.2#

167 69.9 14.6 22.0#

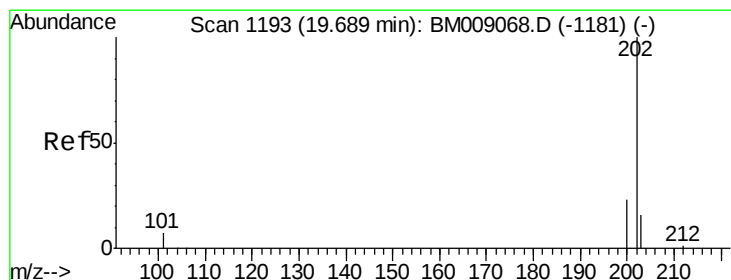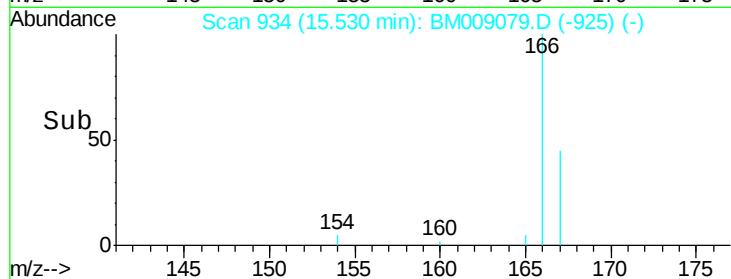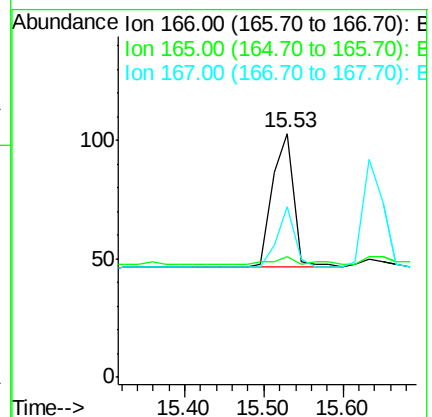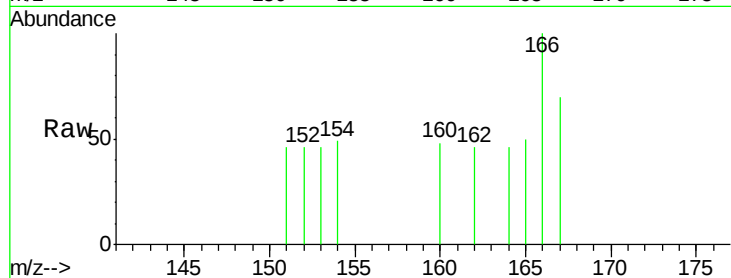

#17

Pyrene

Concen: 0.05 ng/ul

RT: 19.66 min Scan# 1191

Delta R.T. -0.02 min

Lab File: BM009079.D

Acq: 03 Mar 2017 21:50

Tgt Ion:202 Resp: 129

Ion Ratio Lower Upper

202 100

200 38.6 18.2 27.4#

203 144.9 15.6 23.4#

