


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030317\
Data File : BM009079.D
Acq On : 03 Mar 2017 21:50
Operator : SJ/MA
Sample : I2051-08
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF1

Manual Integrations
APPROVED

mohammad
3/6/2017 3:17:00 PM

Quant Time: Mar 04 00:12:30 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 03 23:57:02 2017
Response via : Initial Calibration

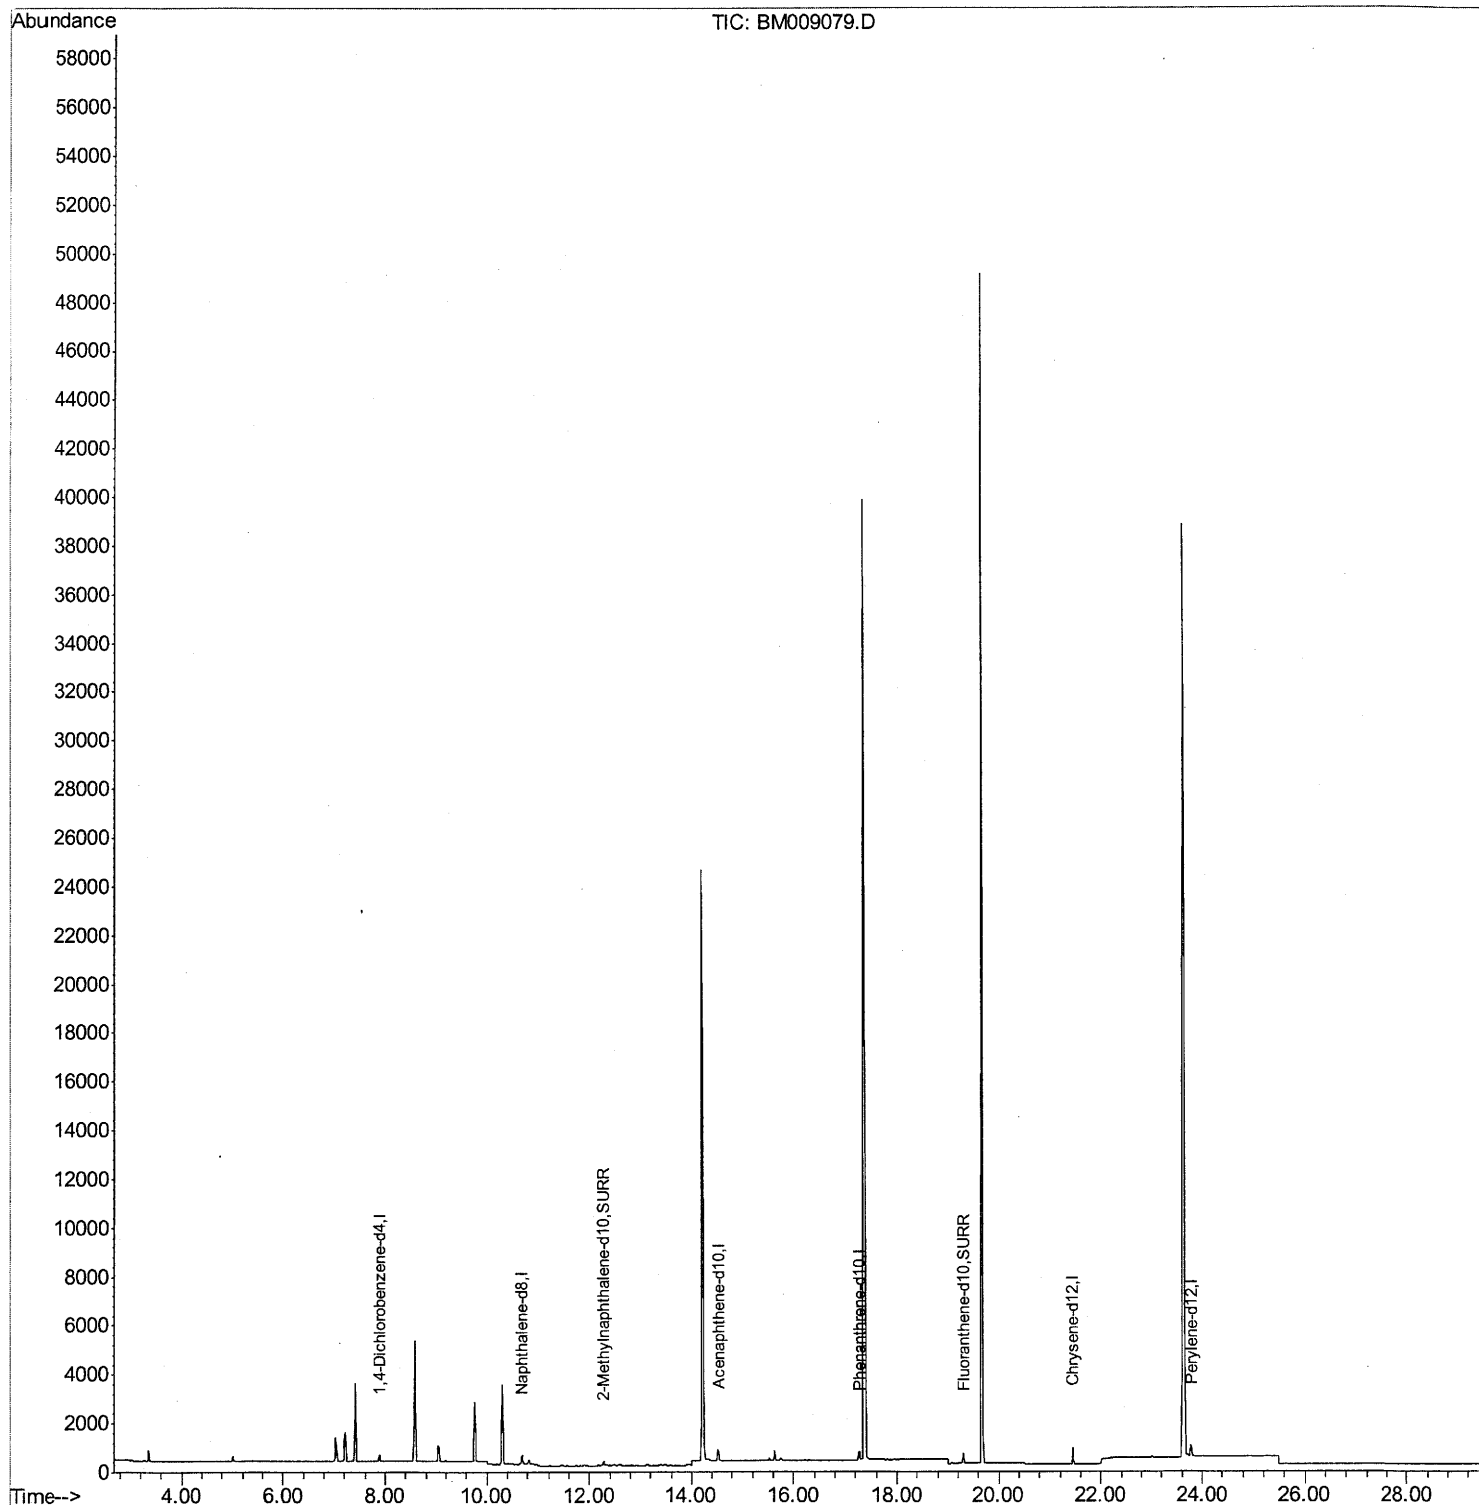




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030317\
Data File : BM009079.D
Acq On : 03 Mar 2017 21:50
Operator : SJ/MA
Sample : I2051-08
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF1

Manual Integrations
APPROVED

mohammad
3/6/2017 3:17:00 PM

Quant Time: Mar 04 00:00:01 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 03 23:57:02 2017
Response via : Initial Calibration

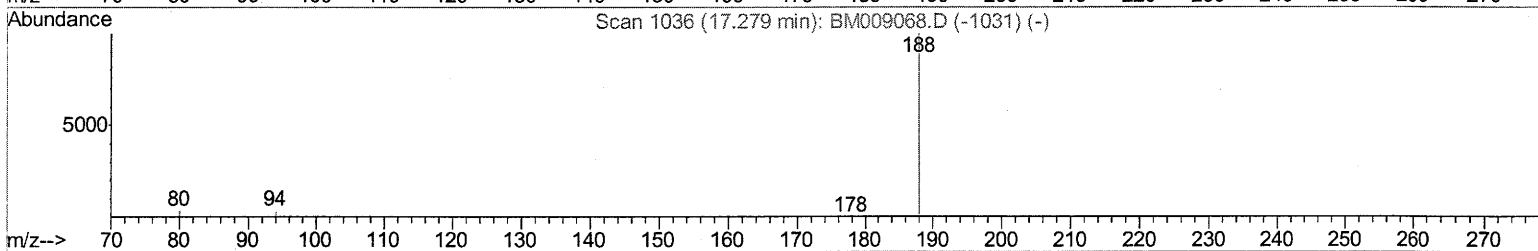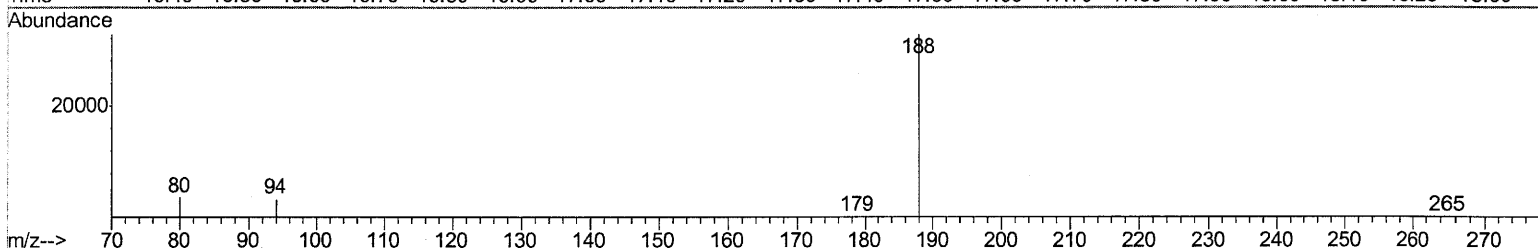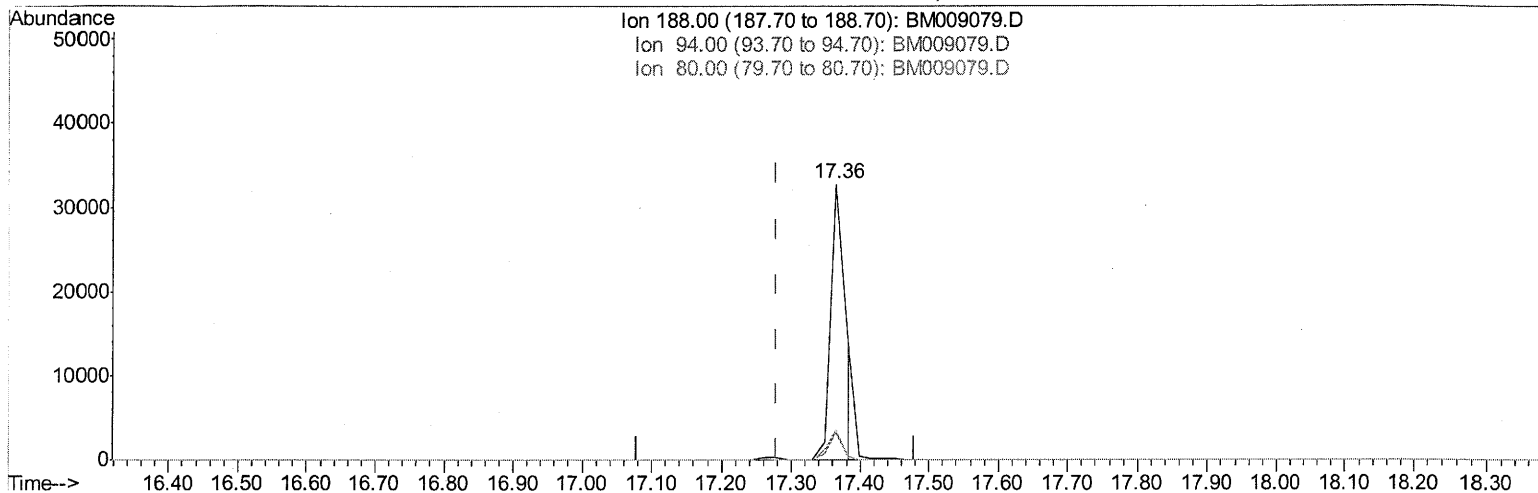

TIC: BM009079.D

(10) Phenanthrene-d10 (I)

17.365min (+0.086) 0.40ng/ul

response 49793

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	9.80
80.00	11.80	10.78
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030317\
Data File : BM009079.D
Acq On : 03 Mar 2017 21:50
Operator : SJ/MA
Sample : I2051-08
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF1

Manual Integrations
APPROVED

mohammad
3/6/2017 3:17:00 PM

Quant Time: Mar 04 00:00:01 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 03 23:57:02 2017
Response via : Initial Calibration

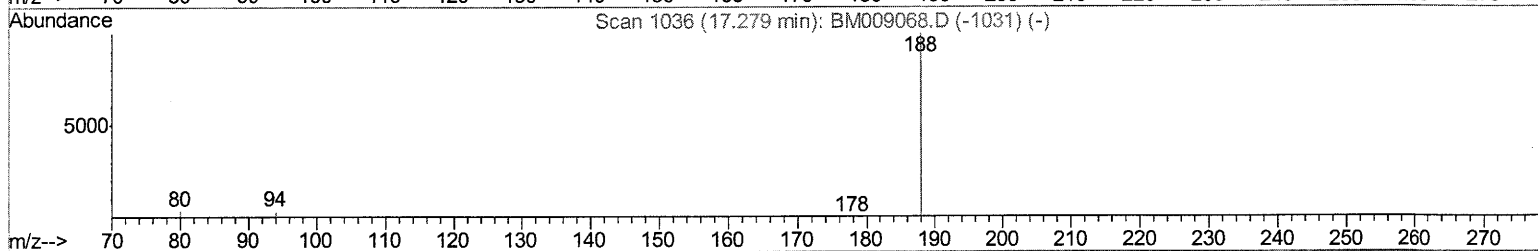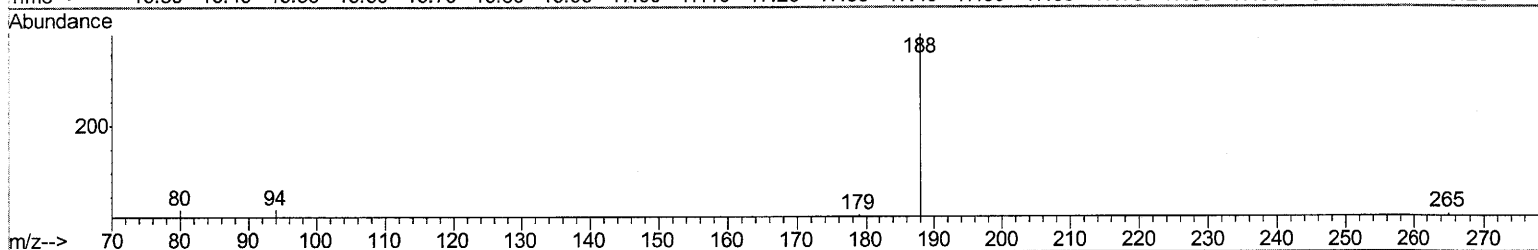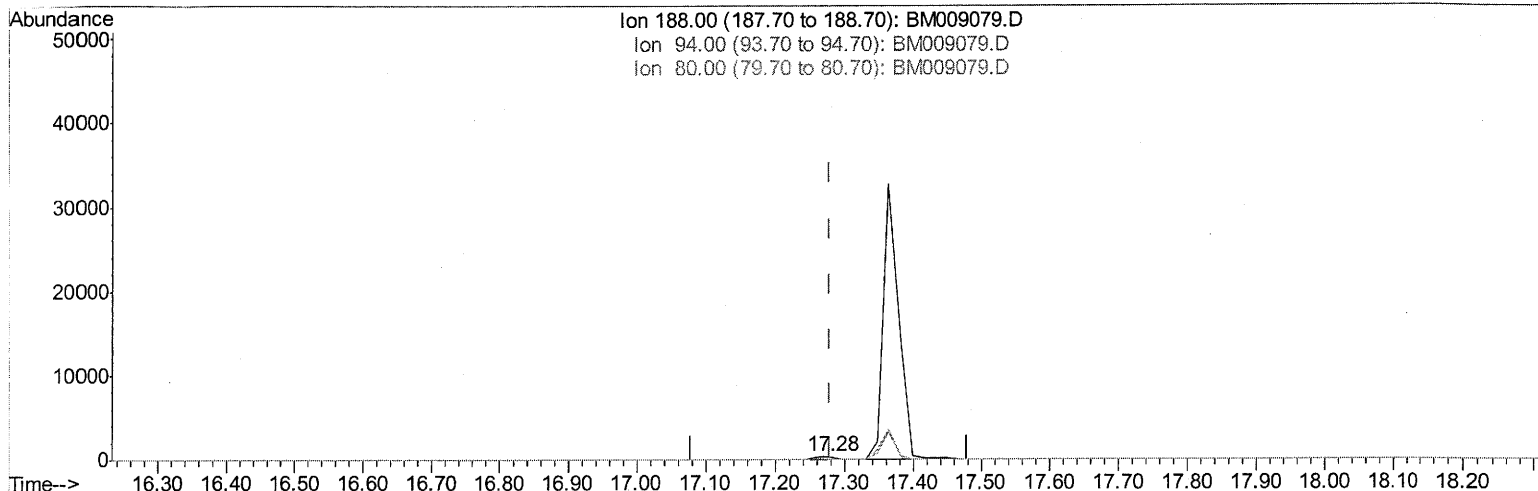

TIC: BM009079.D

(10) Phenanthrene-d10 (I)

17.279min (-0.000) 0.40ng/ul m SJ 3/8/17

response 676

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	16.43#
80.00	11.80	16.43#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030317\
Data File : BM009079.D
Acq On : 03 Mar 2017 21:50
Operator : SJ/MA
Sample : I2051-08
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF1

Manual Integrations
APPROVED

mohammad
3/6/2017 3:17:00 PM

Quant Time: Mar 04 00:00:01 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 03 23:57:02 2017
Response via : Initial Calibration

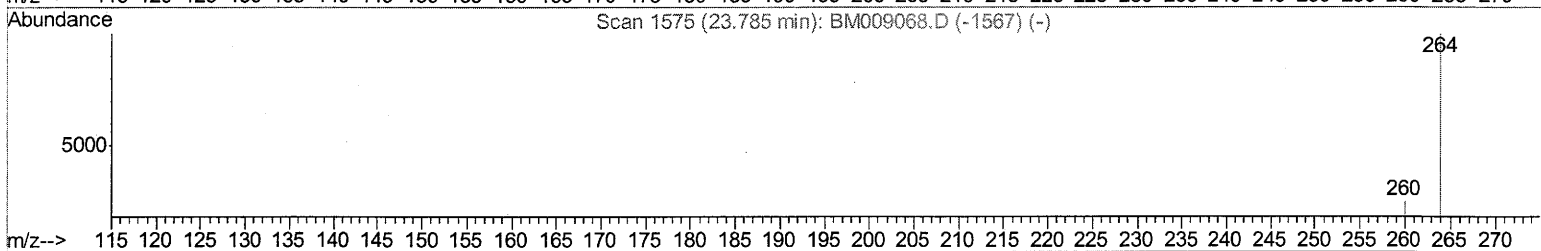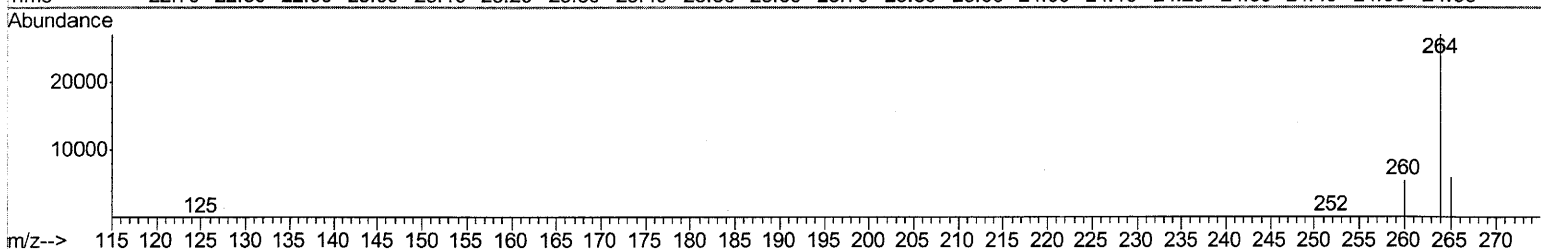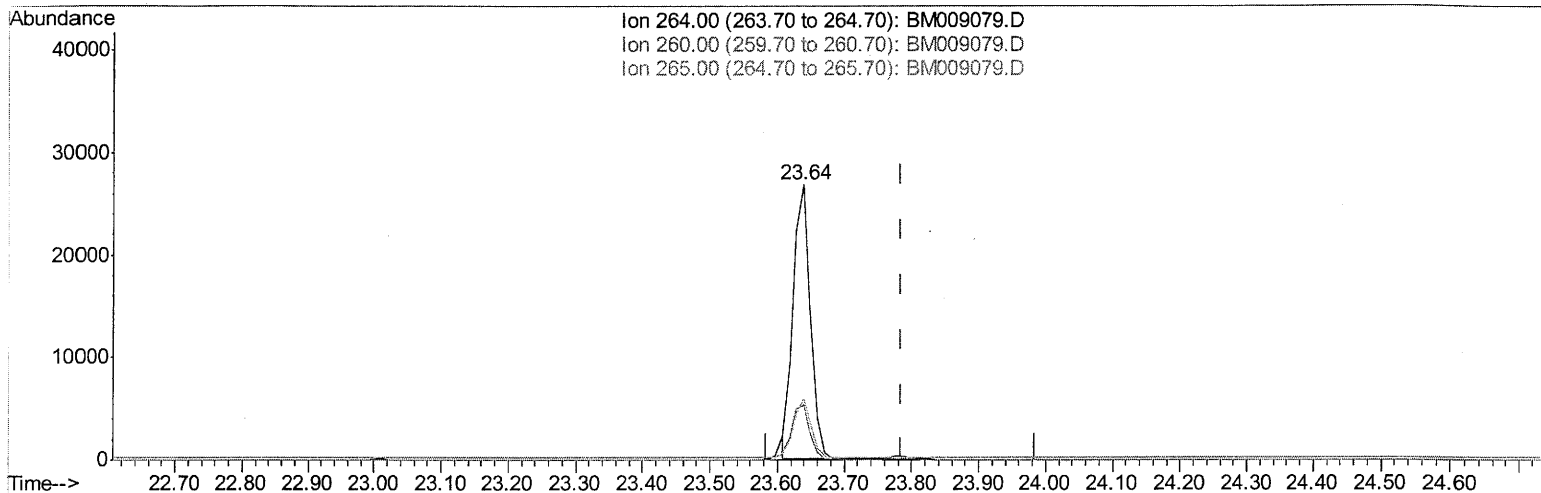

TIC: BM009079.D

(20) Perylene-d12 (I)

23.639min (-0.146) 0.40ng/ul

response 48880

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	20.22#
265.00	103.50	22.50#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030317\
Data File : BM009079.D
Acq On : 03 Mar 2017 21:50
Operator : SJ/MA
Sample : I2051-08
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF1

Manual Integrations
APPROVED

mohammad
3/6/2017 3:17:00 PM

Quant Time: Mar 04 00:00:01 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 03 23:57:02 2017
Response via : Initial Calibration

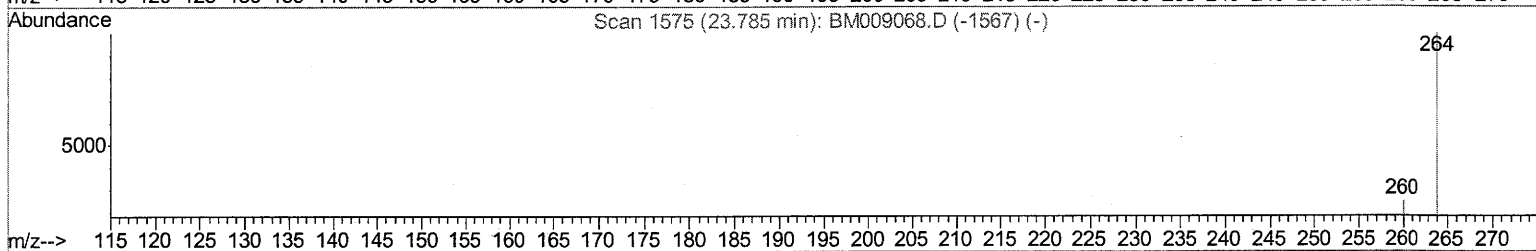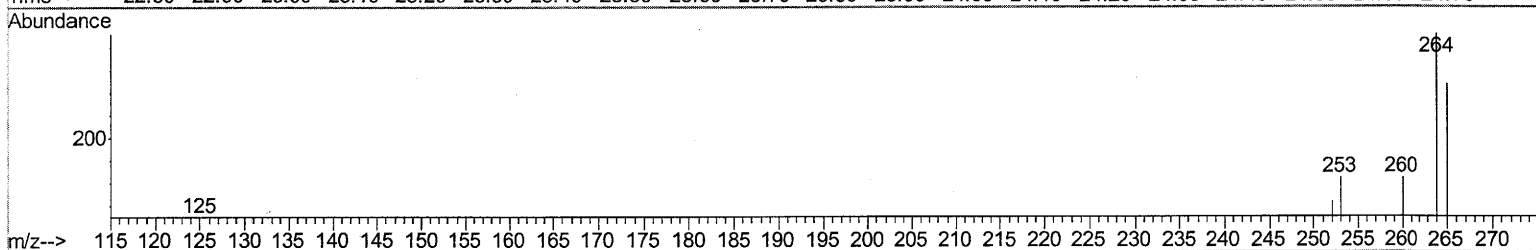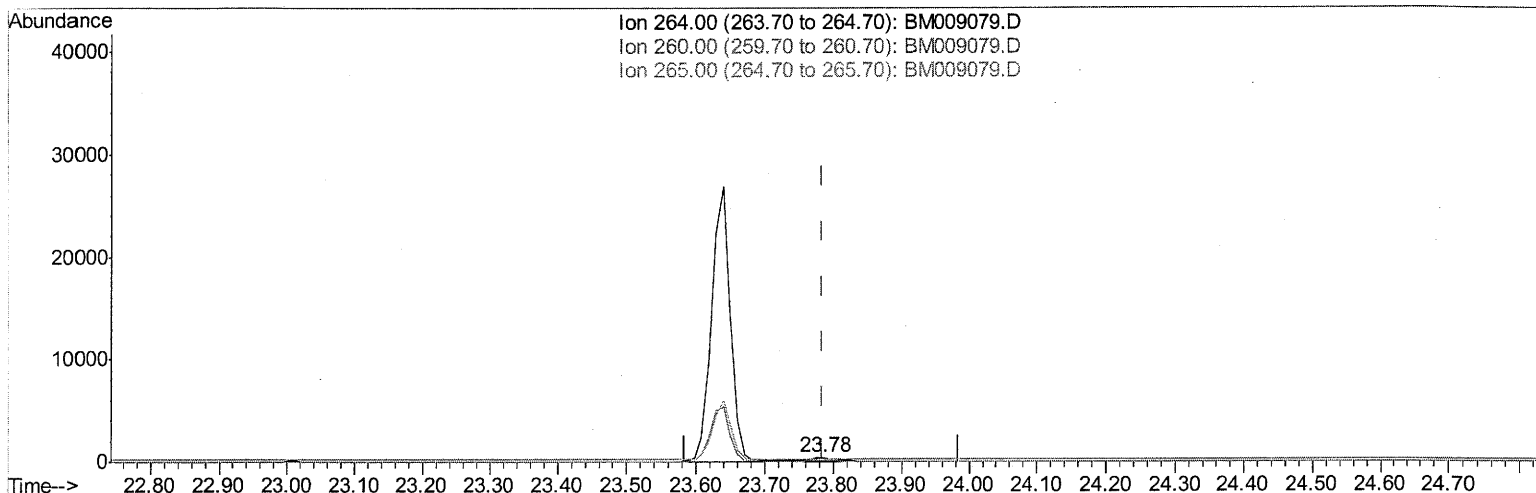

TIC: BM009079.D

(20) Perylene-d12 (I)

23.785min (-0.000) 0.40ng/ul m

SJ 3/8/17

response 652

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	33.59
265.00	103.50	77.08#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030317\
Data File : BM009079.D
Acq On : 03 Mar 2017 21:50
Operator : SJ/MA
Sample : I2051-08
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF1

Manual Integrations
APPROVED

mohammad
3/6/2017 3:17:00 PM

Quant Time: Mar 04 00:12:30 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 03 23:57:02 2017
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.90	152	158	0.40	ng/ul	0.00
2) Naphthalene-d8	10.69	136	478	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.52	164	296	0.40	ng/ul	-0.02
10) Phenanthrene-d10	17.28	188	676m>	0.40	ng/ul	0.00
16) Chrysene-d12	21.45	240	704	0.40	ng/ul	0.00
20) Perylene-d12	23.78	264	652m>	0.40	ng/ul	0.00

} SJ 3/8/17

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	12.28	152	217	0.27	ng/ul	0.00
14) Fluoranthene-d10	19.30	212	564	0.27	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed