
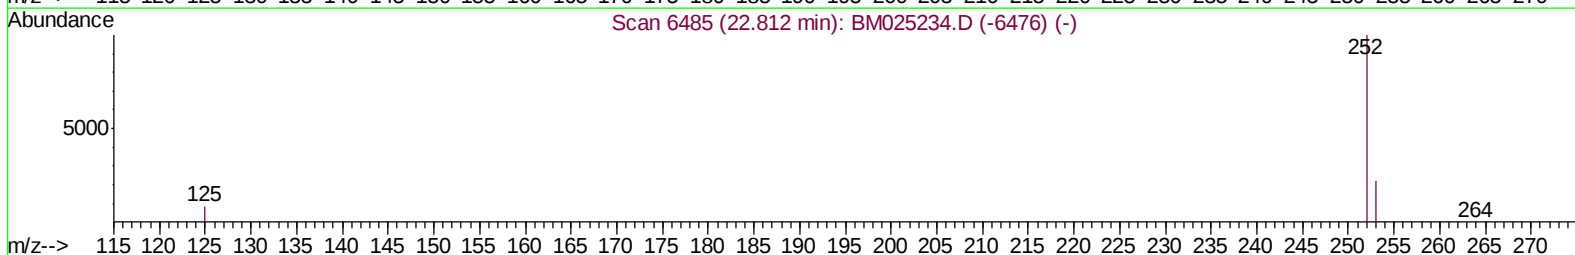
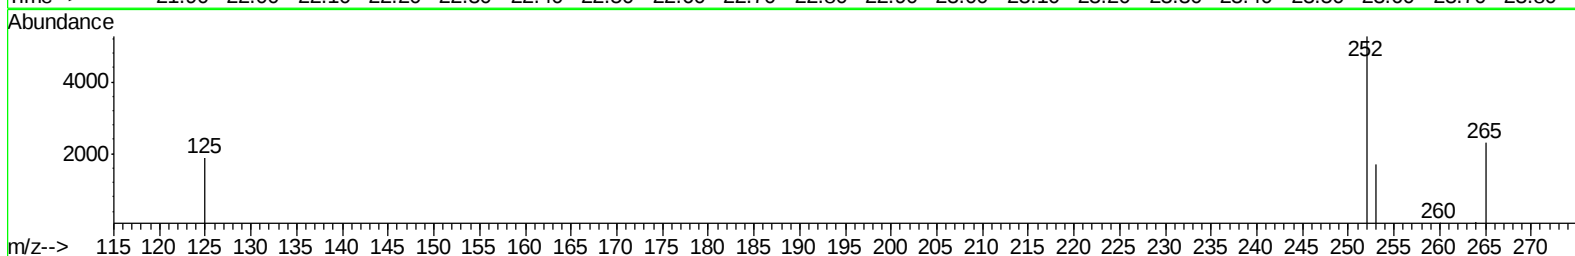


Data File : BM025235.D
Acq On : 04 Mar 2020 05:40
Operator : CG/JU
Sample : L1516-01
Misc :
ALS Vial : 31 Sample Multiplier: 1

Quant Time: Mar 04 08:03:52 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 04 08:02:03 2020
Response via : Initial Calibration

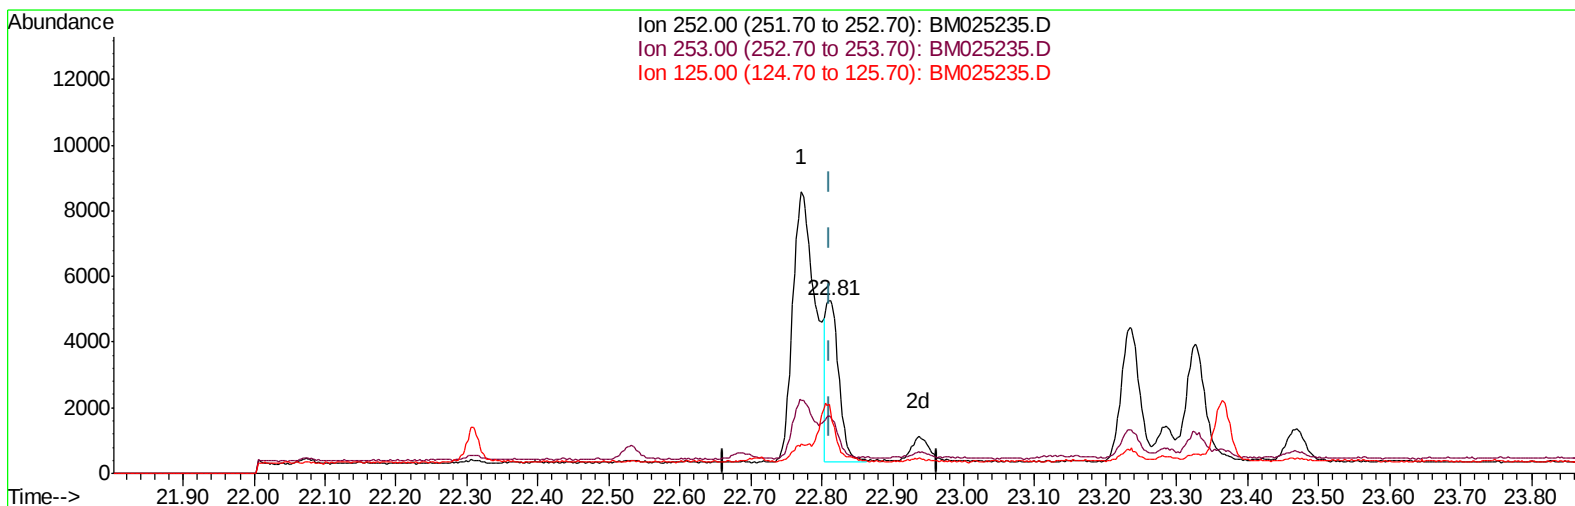

TIC: BM025235.D

(22) Benzo(k)fluoranthene

22.812min (+0.000) 0.06ng/ul m

response 6507

Ion	Exp%	Act%
252.00	100	100
253.00	24.20	32.64#
125.00	13.40	35.51#
0.00	0.00	0.00