
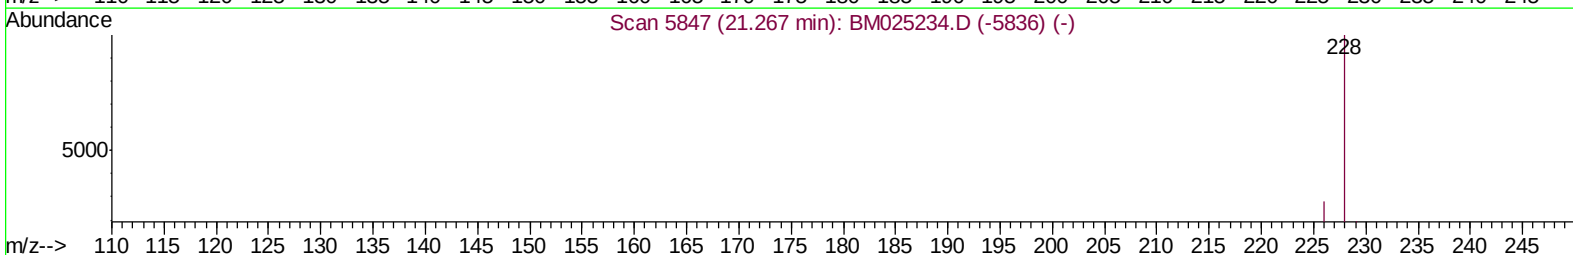
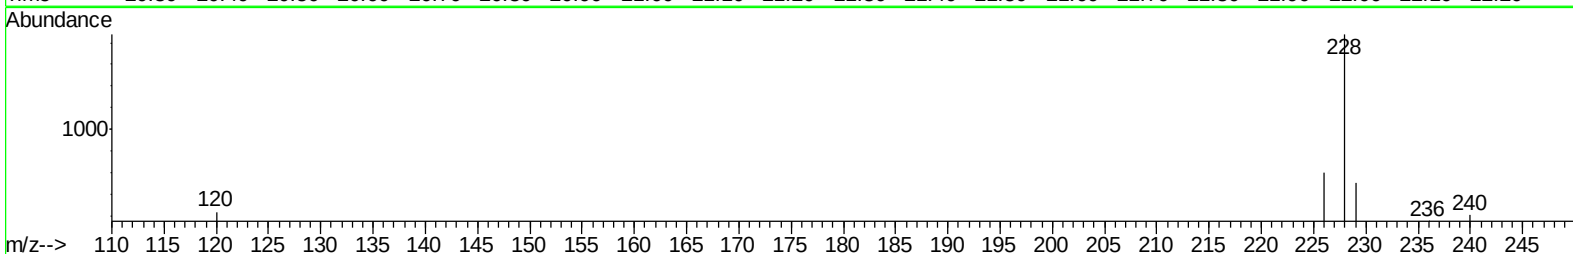


Data File : BM025236.D
Acq On : 04 Mar 2020 06:16
Operator : CG/JU
Sample : L1516-21
Misc :
ALS Vial : 32 Sample Multiplier: 1

Quant Time: Mar 04 08:10:25 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 04 08:02:03 2020
Response via : Initial Calibration

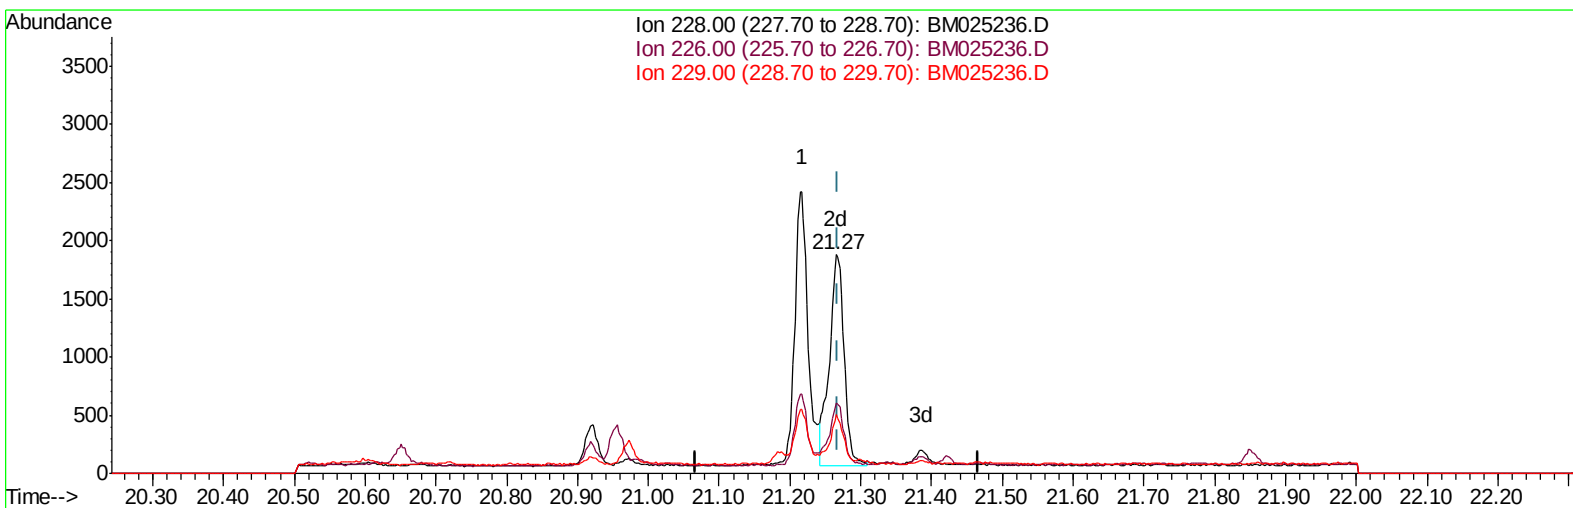

TIC: BM025236.D

(19) Chrysene

21.265min (-0.002) 0.02ng/ul m

response 2641

Ion	Exp%	Act%
228.00	100	100
226.00	29.80	31.95
229.00	21.10	27.05#
0.00	0.00	0.00