

Data File : BM025219.D
Acq On : 03 Mar 2020 19:23
Operator : CG/JU
Sample : PB126929BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK29

Quant Time: Mar 04 00:54:45 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 04 00:52:51 2020
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.68	152	2657	0.40	ng/ul	0.00
2) Naphthalene-d8	10.45	136	10960	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.31	164	8503	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.05
16) Chrysene-d12	21.23	240	19822	0.40	ng/ul	0.00
20) Perylene-d12	23.43	264	19964	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.04	152	6500	0.32	ng/ul	0.00
14) Fluoranthene-d10	19.08	212	19524	0.00	ng/ul	0.00
Target Compounds						
17) Pyrene	19.44	202	3001	0.040	ng/ul#	1
23) Benzo(a)pyrene	23.29	252	7116	0.106	ng/ul#	70


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BM025219.D
Acq On : 03 Mar 2020 19:23
Operator : CG/JU
Sample : PB126929BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK29

Quant Time: Mar 04 00:54:45 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 04 00:52:51 2020
Response via : Initial Calibration

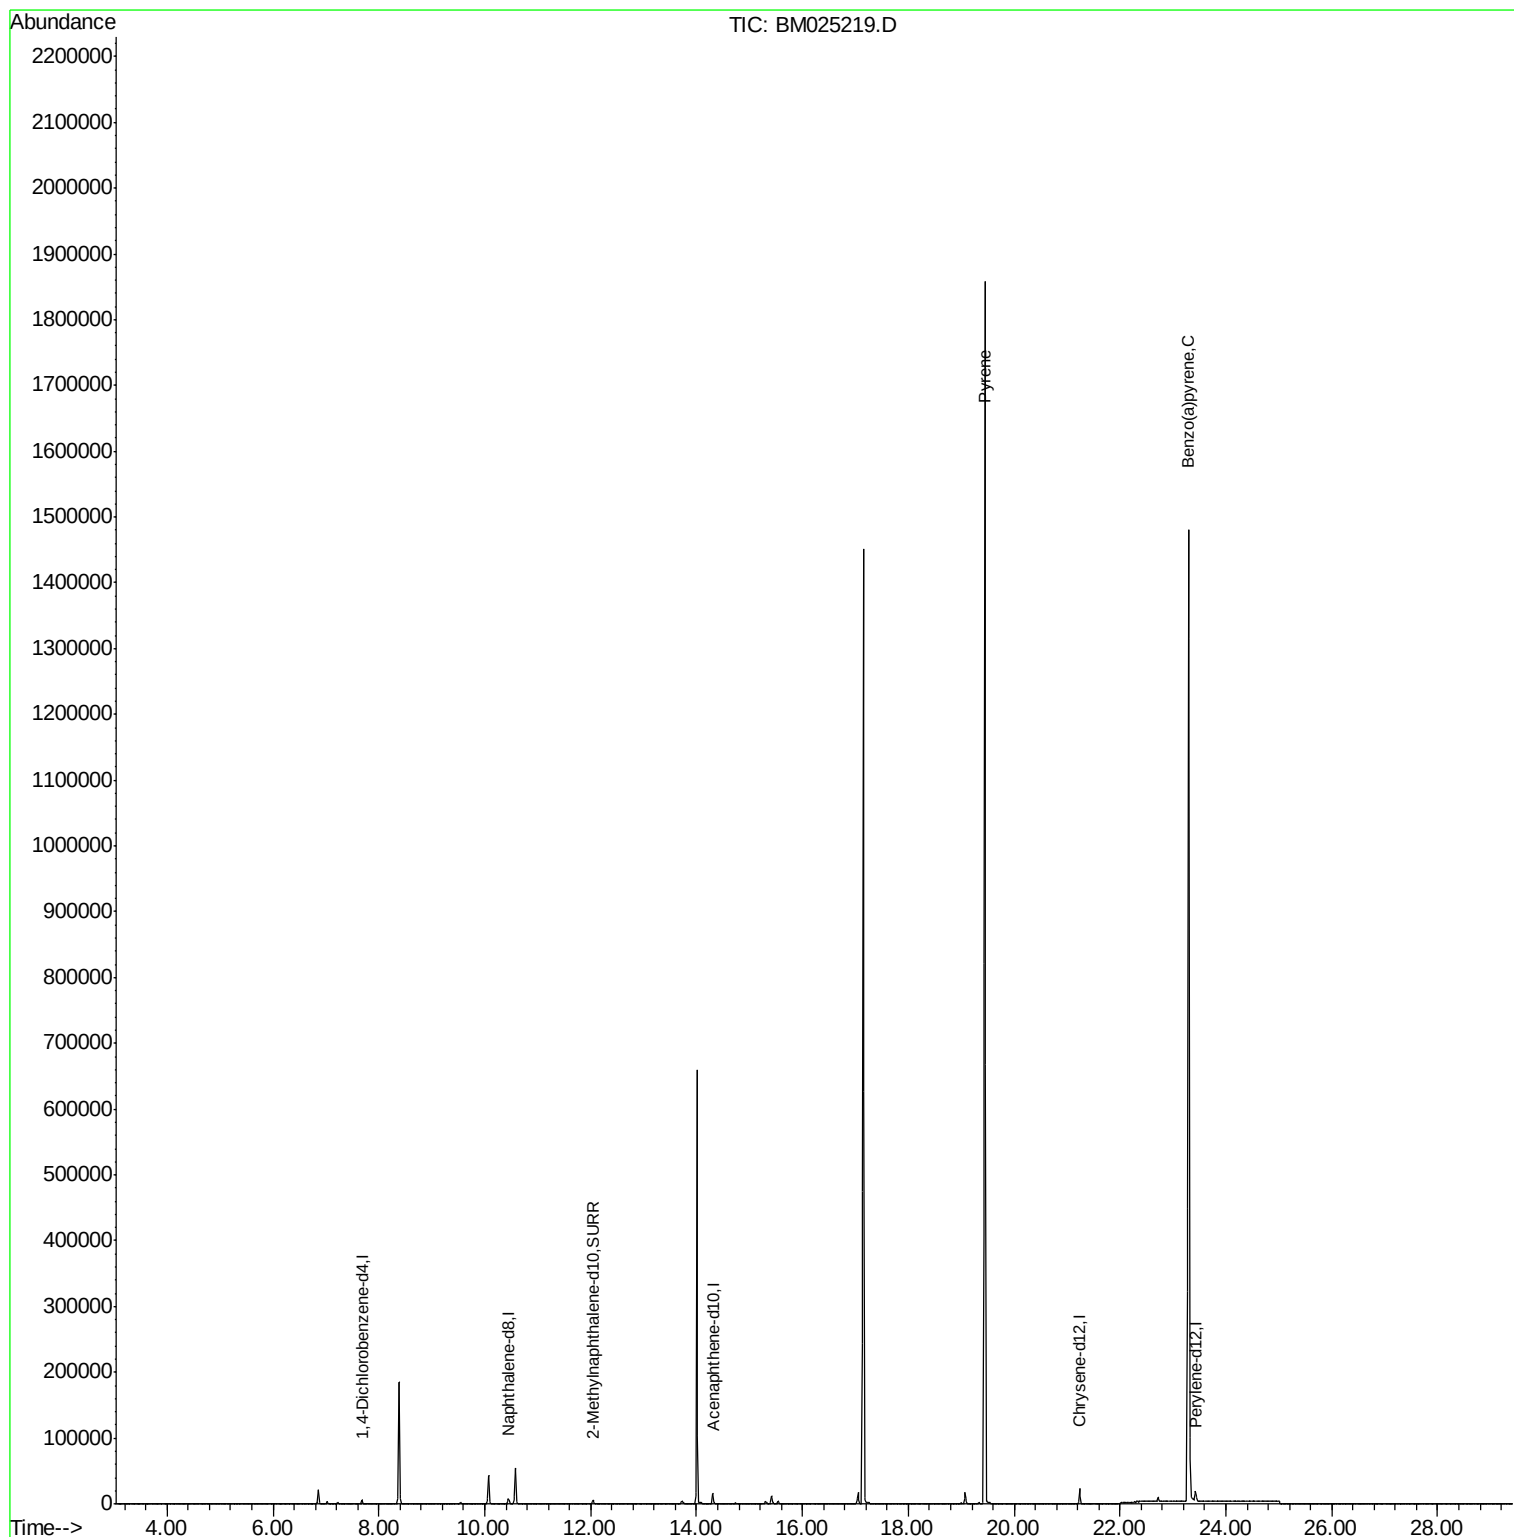

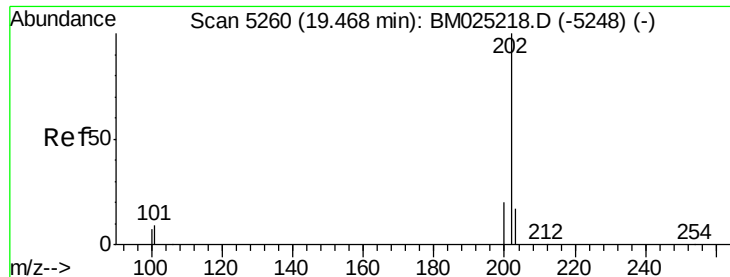

#17

Pyrene

Concen: 0.040 ng/ul

RT: 19.44 min Scan# 5254

Delta R.T. -0.02 min

Lab File: BM025219.D

Acq: 03 Mar 2020 19:23

Instrument :

BNA_M

ClientSampleId :

SBLK29


Tgt Ion:202 Resp: 3001

Ion Ratio Lower Upper

202 100

101 146.4 8.7 13.1#




100 1096.1 7.3 10.9#

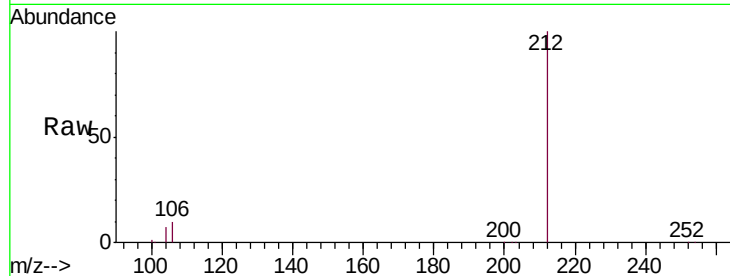

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

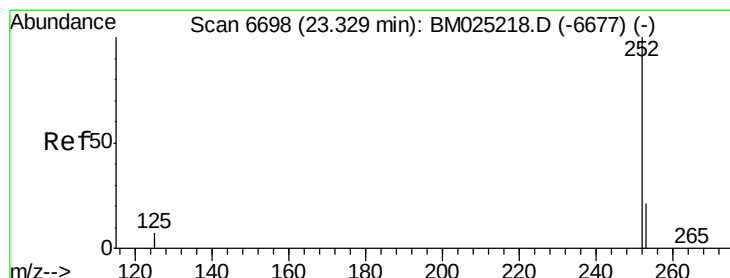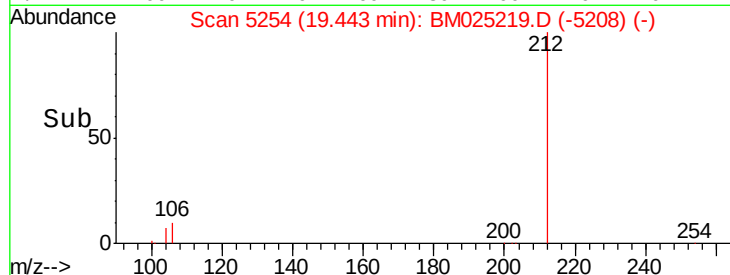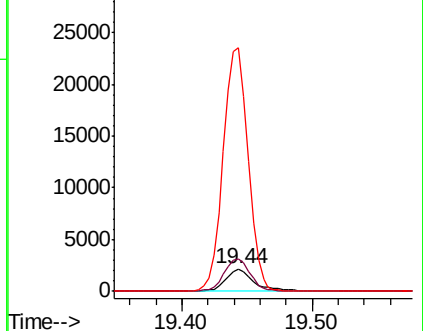

#23

Benzo(a)pyrene

Concen: 0.106 ng/ul

RT: 23.29 min Scan# 6684

Delta R.T. -0.04 min

Lab File: BM025219.D

Acq: 03 Mar 2020 19:23


Tgt Ion:252 Resp: 7116

Ion Ratio Lower Upper

252 100

253 42.2 20.3 30.5#

125 27.1 13.0 19.4#

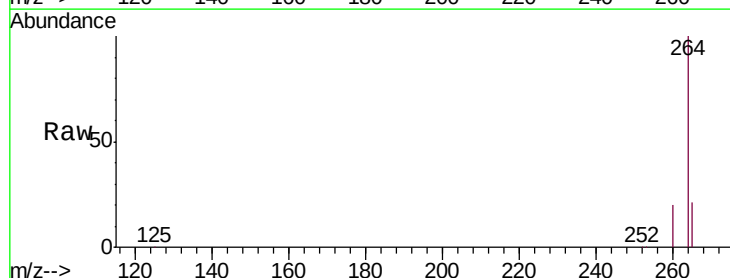

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

