

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM030320\
Quantitation Report (Not Reviewed)

Data File : BM025222.D
Acq On : 03 Mar 2020 21:13
Operator : CG/JU
Sample : L1542-09
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBD45

Quant Time: Mar 04 00:55:02 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 04 00:52:51 2020
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.68	152	3750	0.40	ng/ul	0.00
2) Naphthalene-d8	10.45	136	15879	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.31	164	11691	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.05
16) Chrysene-d12	21.23	240	24326	0.40	ng/ul	0.00
20) Perylene-d12	23.43	264	22240	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.04	152	7395	0.25	ng/ul	0.00
14) Fluoranthene-d10	19.08	212	20364	0.00	ng/ul	0.00
Target Compounds						
23) Benzo(a)pyrene	23.29	252	4834	0.065	ng/ul#	Qvalue 76


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BM025222.D
Acq On : 03 Mar 2020 21:13
Operator : CG/JU
Sample : L1542-09
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBD45

Quant Time: Mar 04 00:55:02 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 04 00:52:51 2020
Response via : Initial Calibration

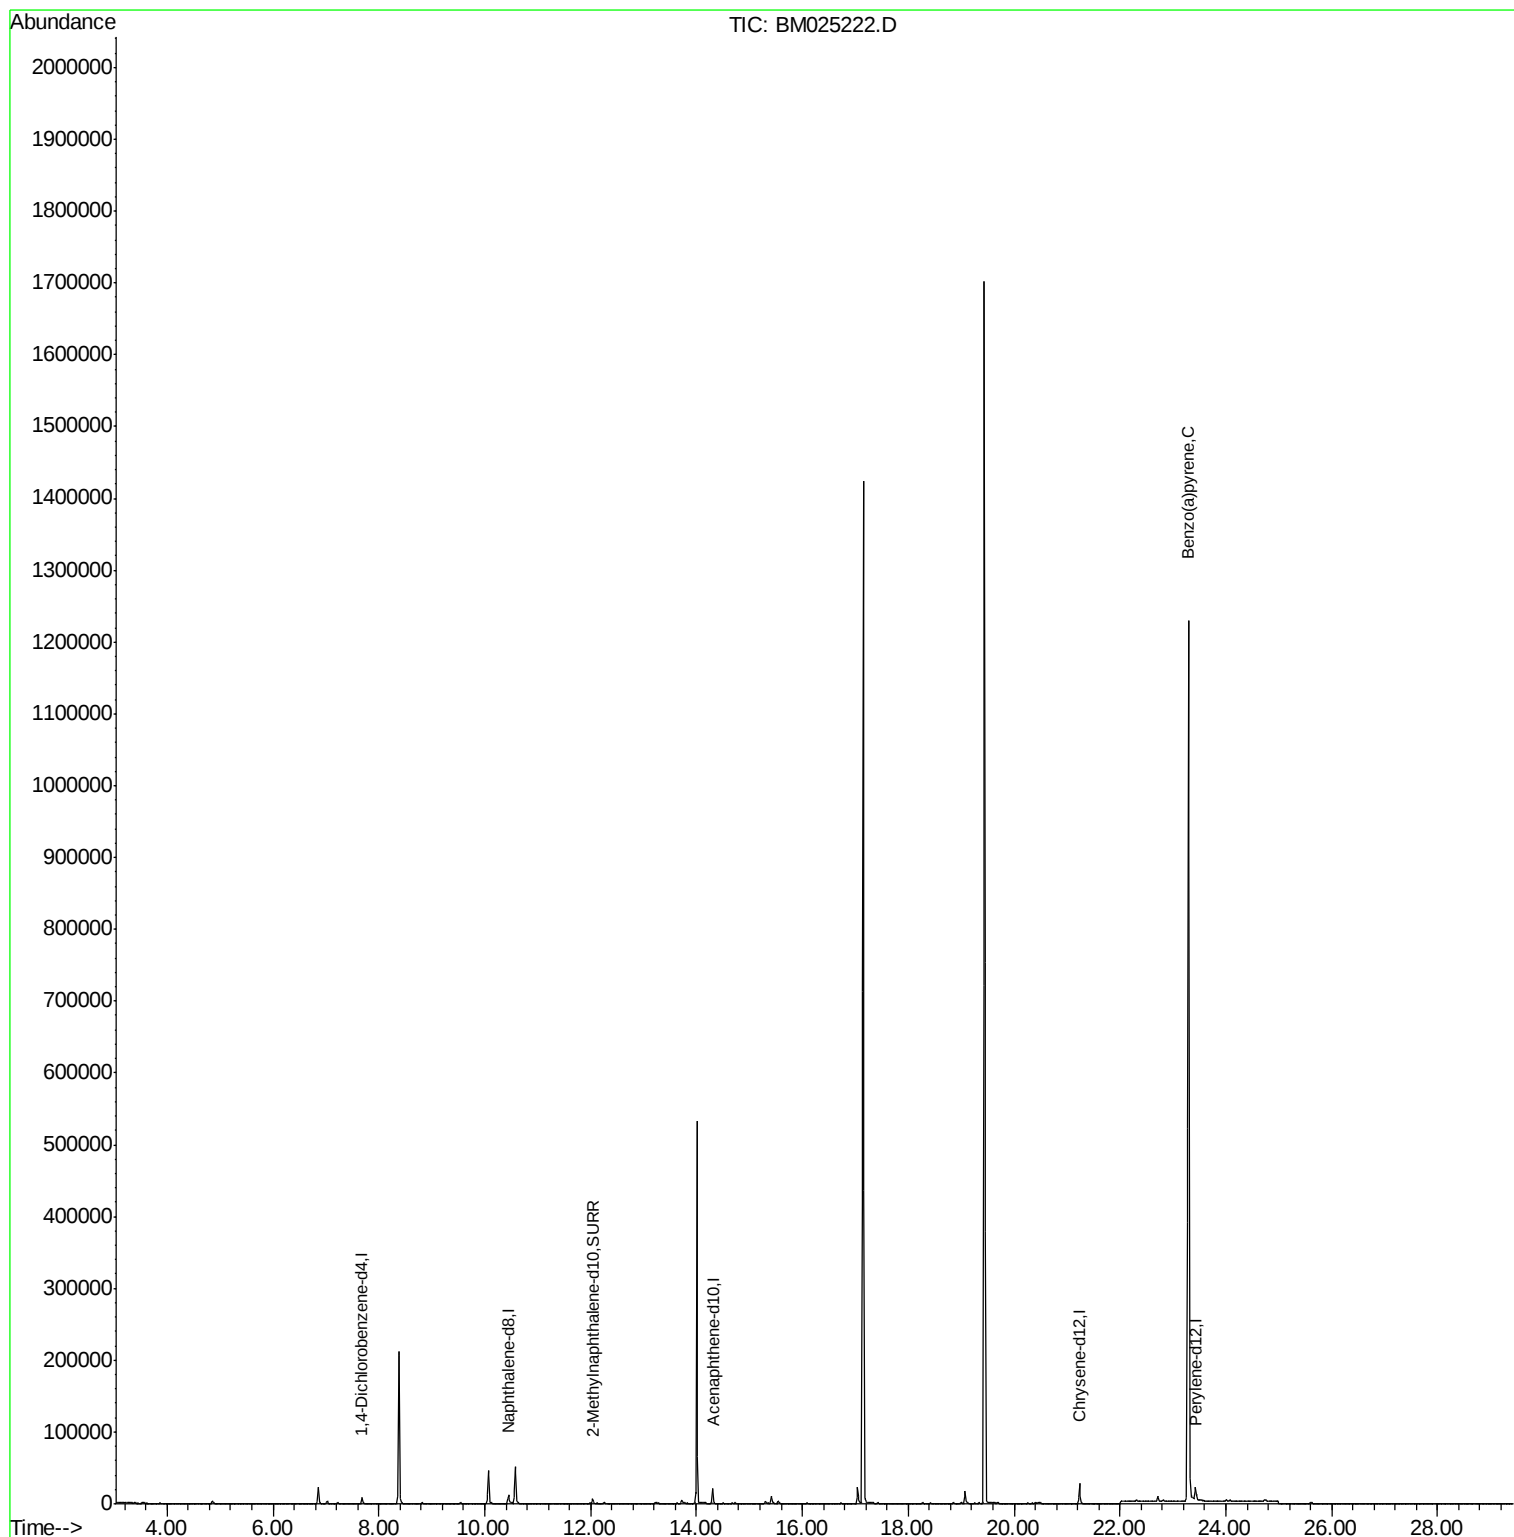

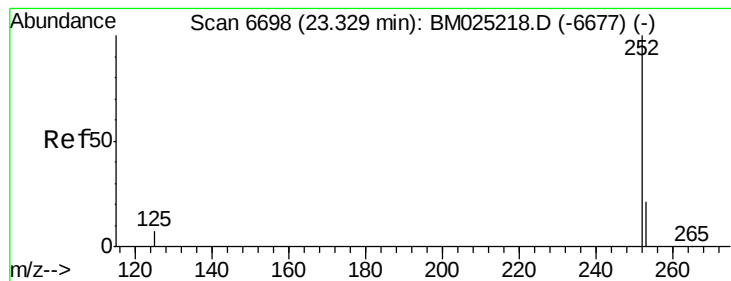

#23

Benzo(a)pyrene

Concen: 0.065 ng/ul

RT: 23.29 min Scan# 6683

Delta R.T. -0.04 min

Lab File: BM025222.D


Acq: 03 Mar 2020 21:13

Instrument :

BNA_M

ClientSampleId :

DBD45

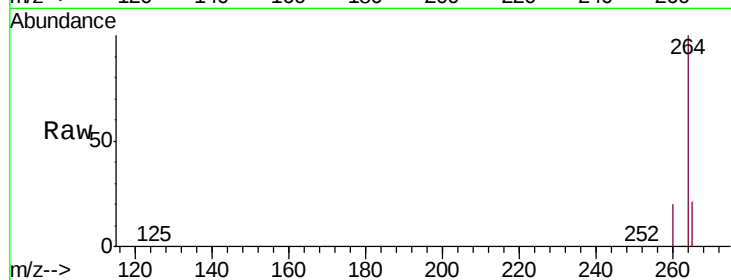

Tgt Ion:	252	Resp:	4834
Ion	Ratio	Lower	Upper
252	100		
253	37.5	20.3	30.5#
125	26.6	13.0	19.4#

