

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM030320\
Quantitation Report (Not Reviewed)

Data File : BM025225.D
Acq On : 03 Mar 2020 23:02
Operator : CG/JU
Sample : L1542-21
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBD55

Quant Time: Mar 04 00:55:19 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 04 00:52:51 2020
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.68	152	5778	0.40	ng/ul	0.00
2) Naphthalene-d8	10.45	136	25648	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.31	164	18905	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.05
16) Chrysene-d12	21.23	240	45685	0.40	ng/ul	0.00
20) Perylene-d12	23.43	264	44668	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.04	152	13375	0.28	ng/ul	0.00
14) Fluoranthene-d10	19.08	212	40227	0.00	ng/ul	0.00
Target Compounds						
17) Pyrene	19.44	202	6637	0.038	ng/ul#	Qvalue 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BM025225.D
Acq On : 03 Mar 2020 23:02
Operator : CG/JU
Sample : L1542-21
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBD55

Quant Time: Mar 04 00:55:19 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 04 00:52:51 2020
Response via : Initial Calibration

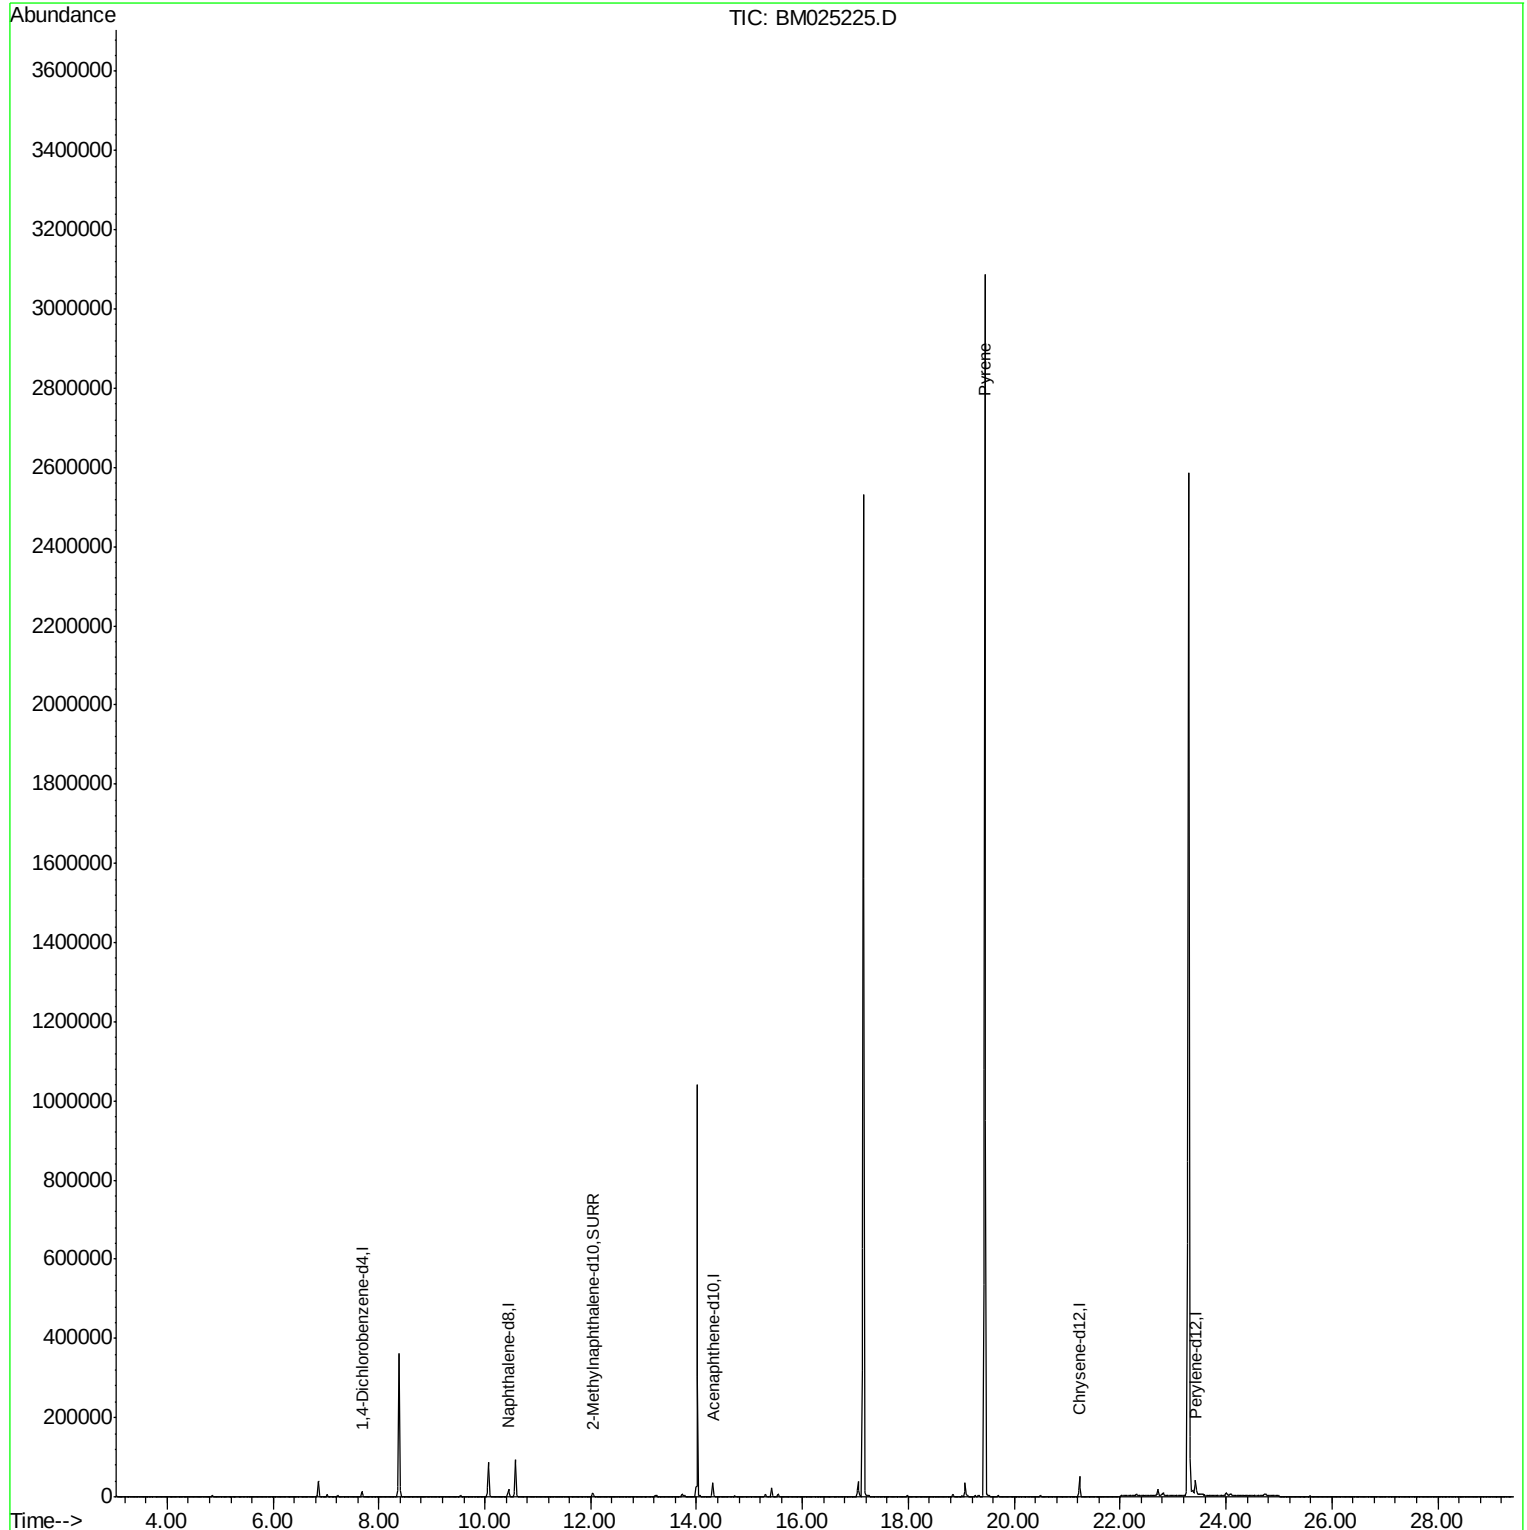

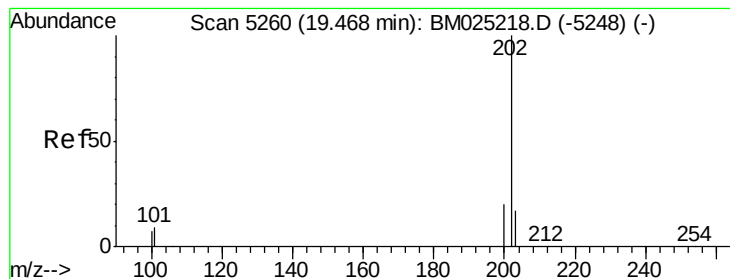

#17

Pyrene

Concen: 0.038 ng/ul

RT: 19.44 min Scan# 5254

Delta R.T. -0.02 min

Lab File: BM025225.D

Acq: 03 Mar 2020 23:02

Instrument :

BNA_M

ClientSampleId :

DBD55



Tgt Ion: 202 Resp: 6637

Ion Ratio Lower Upper

202 100

101 143.0 8.7 13.1#

100 966.7 7.3 10.9#

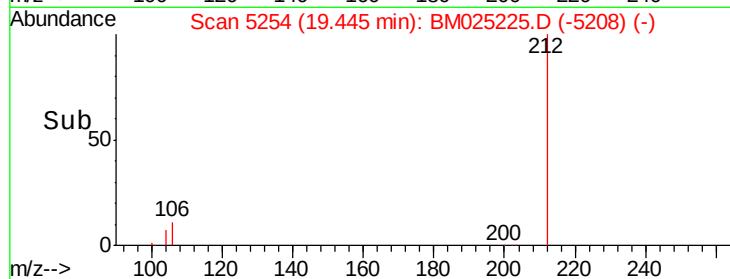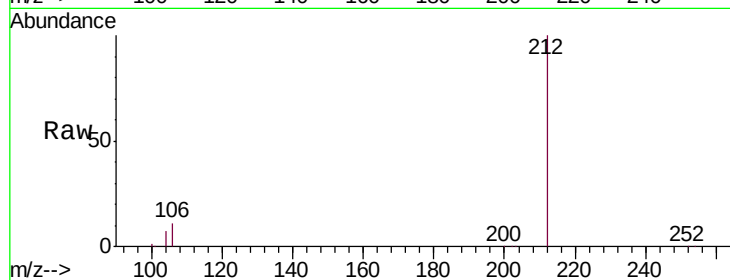

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

