

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030320\
 Data File : BM025255.D
 Acq On : 04 Mar 2020 18:08
 Operator : CG/JU
 Sample : L1516-12
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Mar 05 00:36:42 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 04 08:02:03 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.68	152	5483	0.40	ng/ul	0.00
2) Naphthalene-d8	10.45	136	23770	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.30	164	17417	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.05
16) Chrysene-d12	21.23	240	40571	0.40	ng/ul	0.00
20) Perylene-d12	23.42	264	37557	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.04	152	12919	0.29	ng/ul	0.00
14) Fluoranthene-d10	19.07	212	38597	0.00	ng/ul	0.00
Target Compounds						
17) Pyrene	19.44	202	5777	0.038	ng/ul#	1
23) Benzo(a)pyrene	23.29	252	9388	0.074	ng/ul#	82


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030320\
Data File : BM025255.D
Acq On : 04 Mar 2020 18:08
Operator : CG/JU
Sample : L1516-12
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Mar 05 00:36:42 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 04 08:02:03 2020
Response via : Initial Calibration

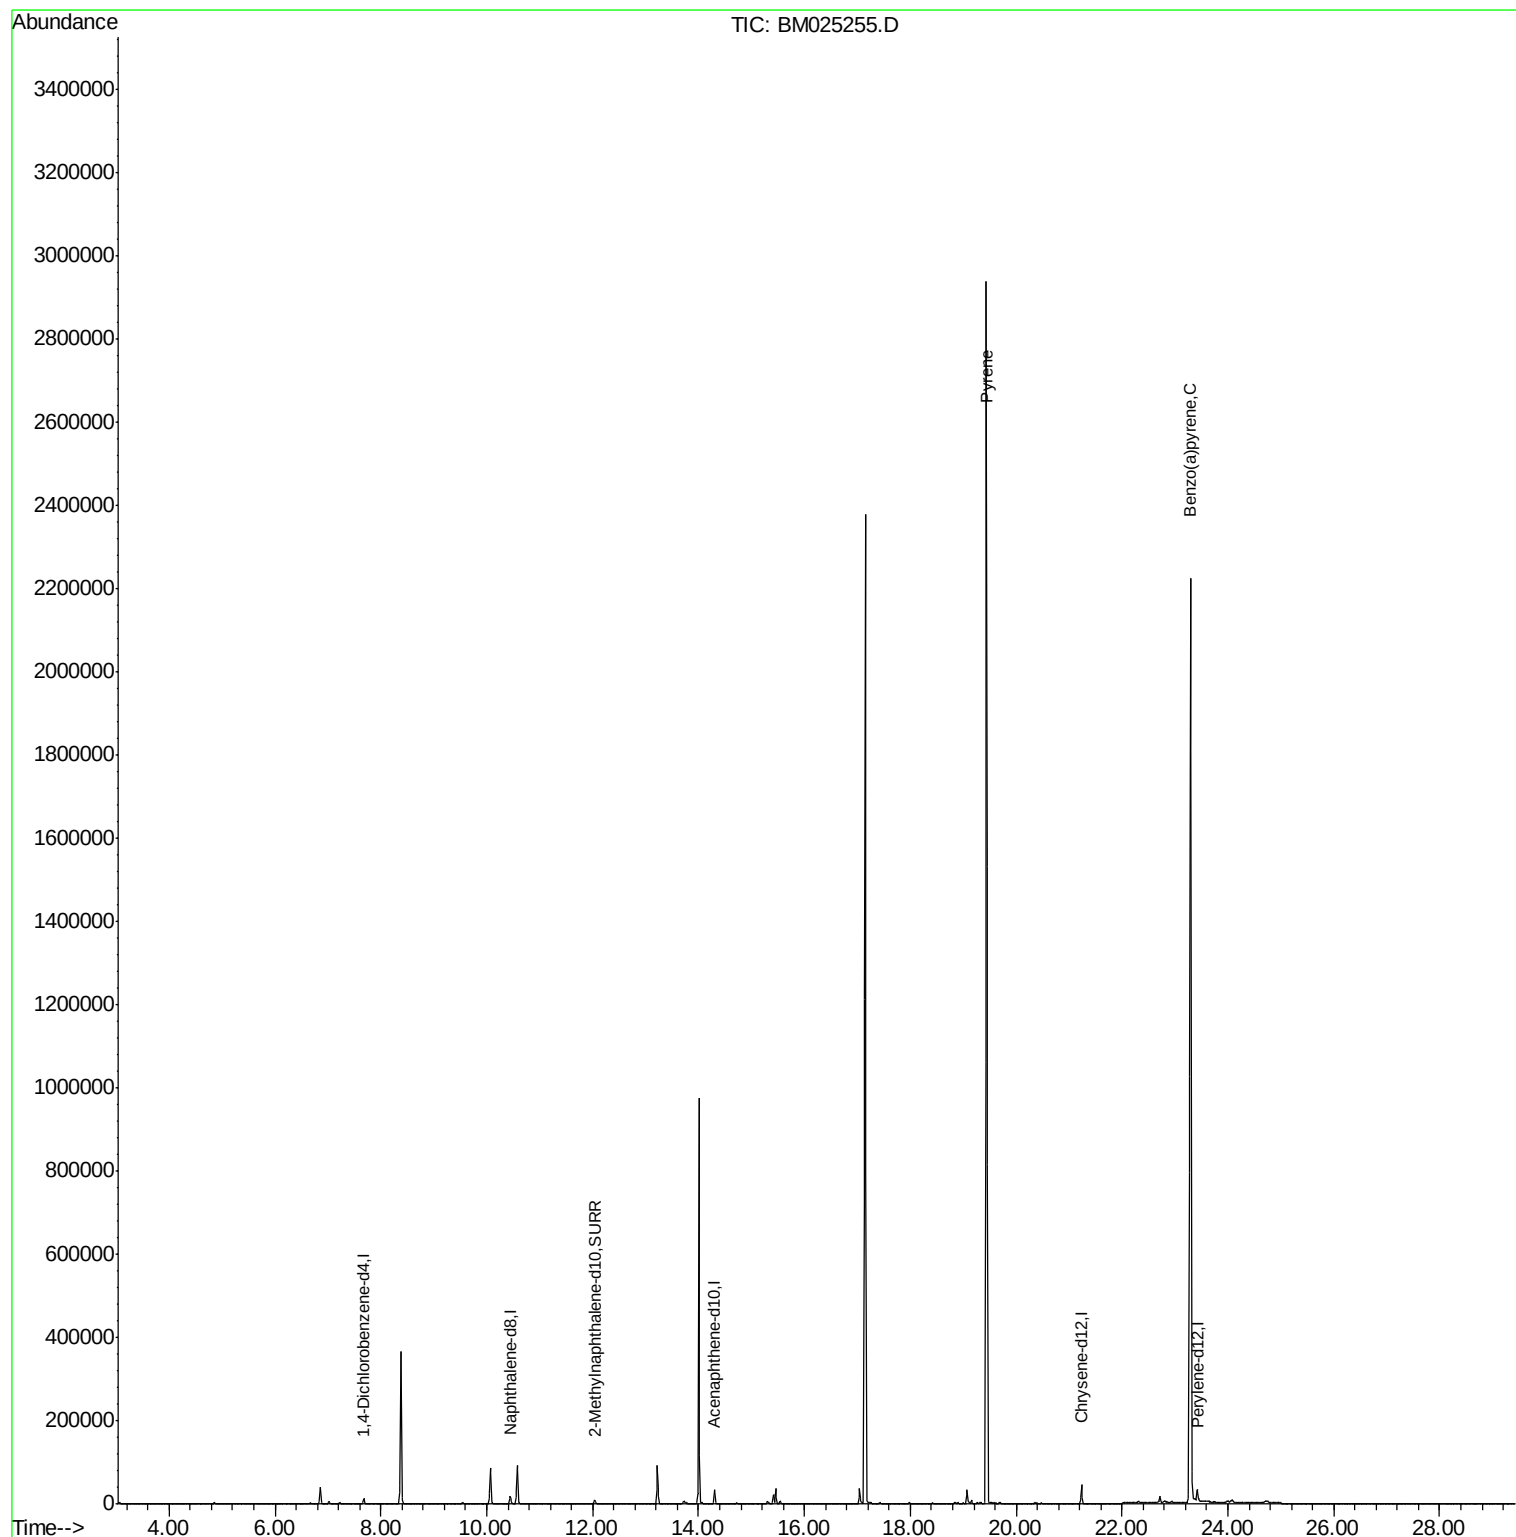

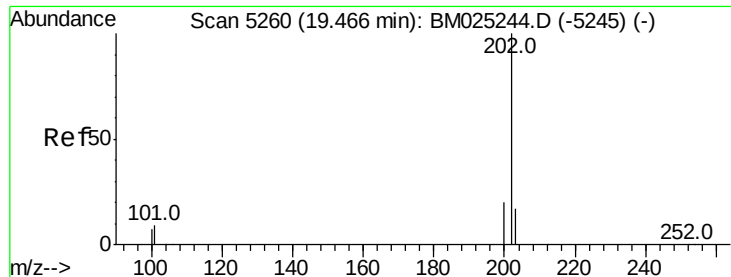

#17

Pvrene

Concen: 0.038 ng/ul

RT: 19.44 min Scan# 5253

Delta R.T. -0.03 min

Lab File: BM025255.D

Acq: 04 Mar 2020 18:08

Instrument :

BNA_M

ClientSampleId :


Tot Ion:202 Resp: 5777

Ion Ratio Lower Upper

202 100

101 149.3 8.7 13.1#




100 1037.1 7.3 10.9#

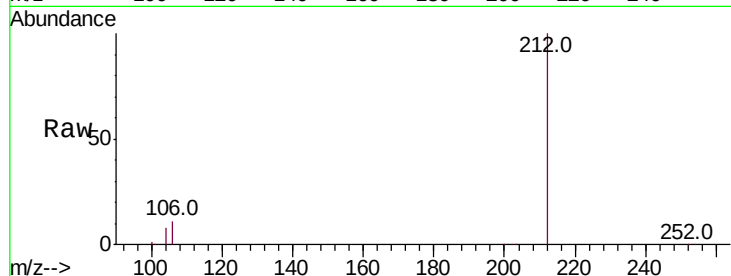

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

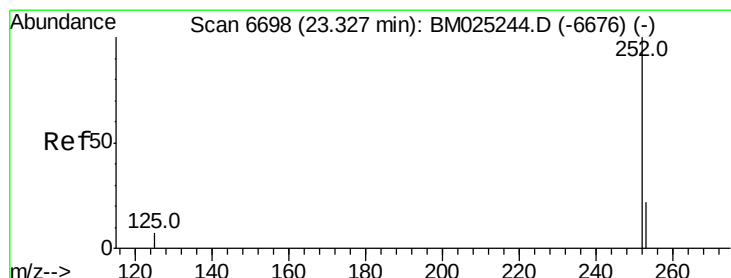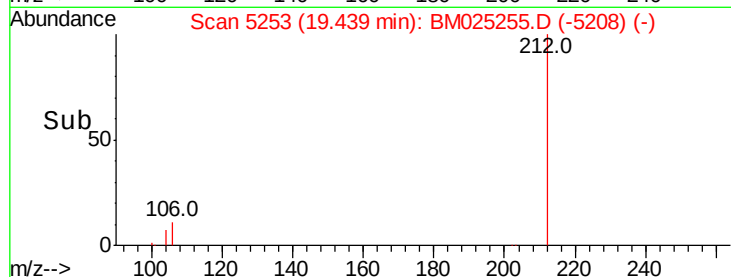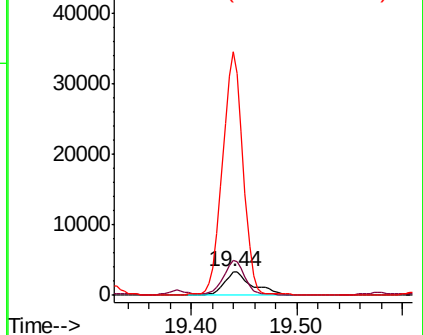

#23

Benzo(a)pyrene

Concen: 0.074 ng/ul

RT: 23.29 min Scan# 6684

Delta R.T. -0.03 min

Lab File: BM025255.D

Acq: 04 Mar 2020 18:08


Tgt Ion:252 Resp: 9388

Ion Ratio Lower Upper

252 100

253 34.2 20.3 30.5#

125 23.7 13.0 19.4#

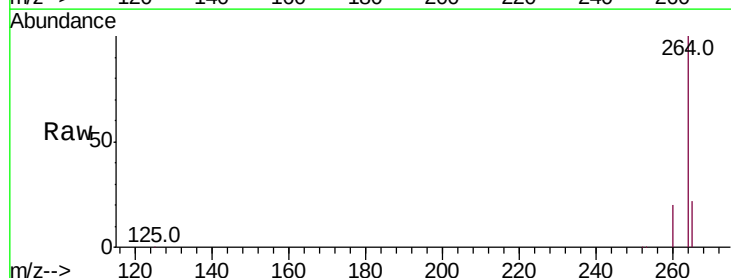

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

