

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030320\
 Data File : BM025259.D
 Acq On : 04 Mar 2020 20:34
 Operator : CG/JU
 Sample : L1516-08
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Mar 05 00:36:59 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 04 08:02:03 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.68	152	5939	0.40	ng/ul	0.00
2) Naphthalene-d8	10.44	136	26049	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.30	164	18927	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.05
16) Chrysene-d12	21.23	240	44648	0.40	ng/ul	0.00
20) Perylene-d12	23.43	264	43277	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.04	152	14695	0.30	ng/ul	0.00
14) Fluoranthene-d10	19.07	212	42942	0.00	ng/ul	0.00
Target Compounds						
17) Pyrene	19.44	202	6447	0.038	ng/ul#	1
23) Benzo(a)pyrene	23.29	252	10866	0.075	ng/ul#	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030320\
Data File : BM025259.D
Acq On : 04 Mar 2020 20:34
Operator : CG/JU
Sample : L1516-08
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Mar 05 00:36:59 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 04 08:02:03 2020
Response via : Initial Calibration




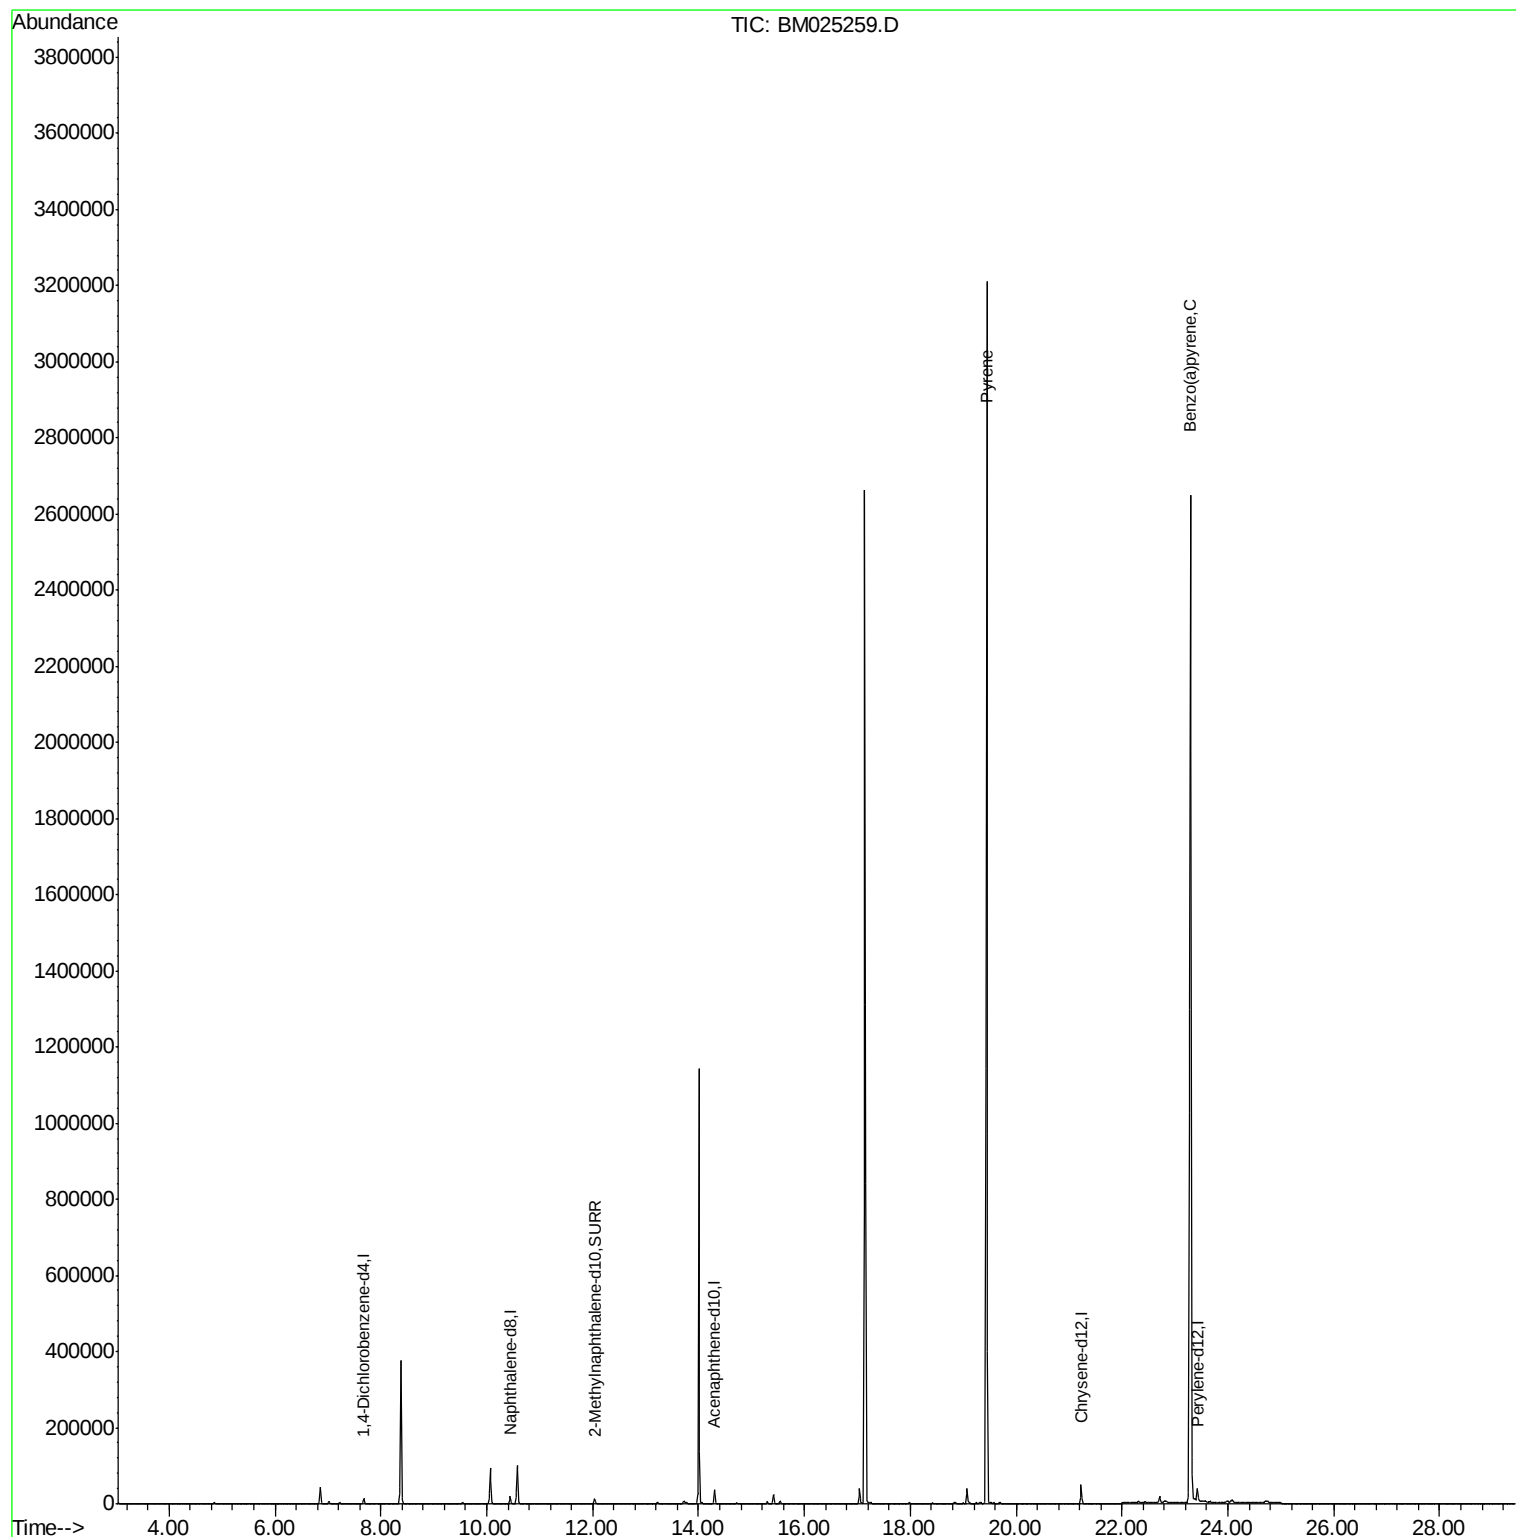


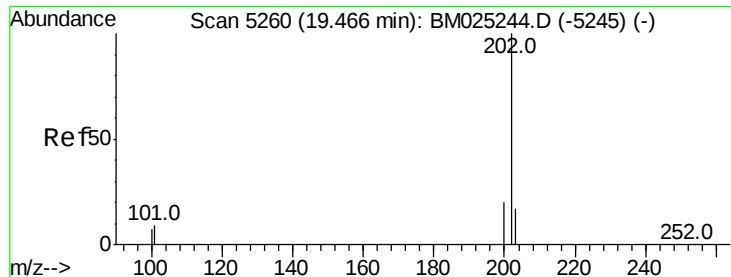

#17
Pvrene
Concen: 0.038 ng/ul
RT: 19.44 min Scan# 5254
Delta R.T. -0.02 min
Lab File: BM025259.D
Acq: 04 Mar 2020 20:34

Instrument :
BNA_M
ClientSampleId :

Tot Ion:202 Resp: 6447
Ion Ratio Lower Upper
202 100
101 137.4 8.7 13.1#
100 930.6 7.3 10.9#

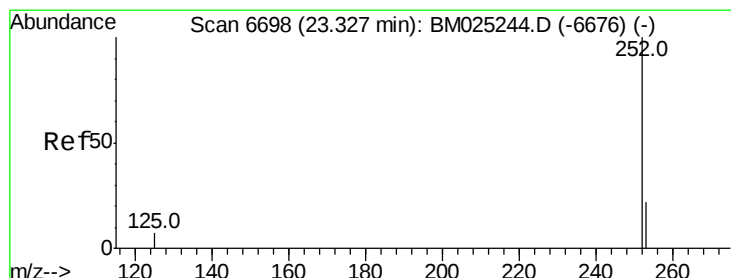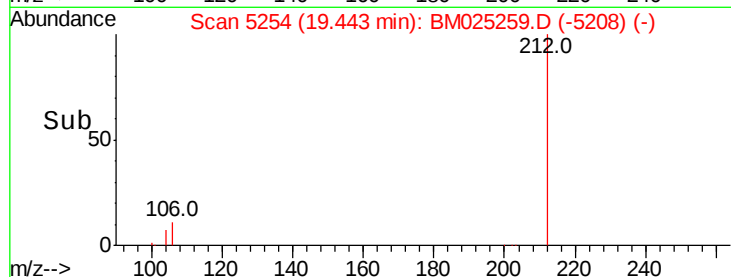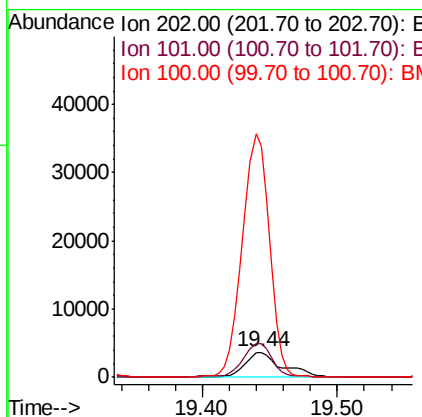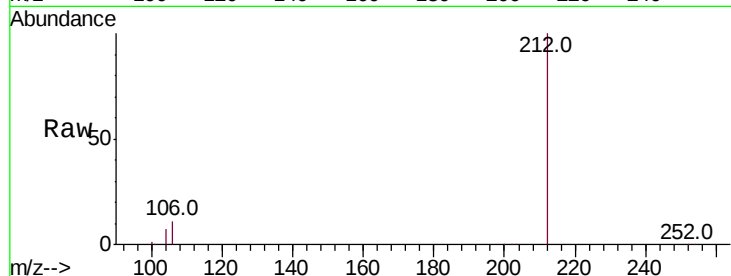

#23
Benzo(a)pyrene
Concen: 0.075 ng/ul
RT: 23.29 min Scan# 6684
Delta R.T. -0.03 min
Lab File: BM025259.D
Acq: 04 Mar 2020 20:34

Tgt Ion:252 Resp: 10866
Ion Ratio Lower Upper
252 100
253 33.5 20.3 30.5#
125 21.9 13.0 19.4#

