

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030320\
 Data File : BM025261.D
 Acq On : 04 Mar 2020 21:46
 Operator : CG/JU
 Sample : L1516-18
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Mar 05 00:37:06 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 04 08:02:03 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.68	152	5851	0.40	ng/ul	0.00
2) Naphthalene-d8	10.44	136	25549	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.30	164	18451	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.05
16) Chrysene-d12	21.23	240	34292	0.40	ng/ul	0.00
20) Perylene-d12	23.42	264	32633	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.04	152	15092	0.32	ng/ul	0.00
14) Fluoranthene-d10	19.07	212	39137	0.00	ng/ul	0.00
Target Compounds						
23) Benzo(a)pyrene	23.29	252	8577	0.078	ng/ul#	80


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030320\
Data File : BM025261.D
Acq On : 04 Mar 2020 21:46
Operator : CG/JU
Sample : L1516-18
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Mar 05 00:37:06 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 04 08:02:03 2020
Response via : Initial Calibration

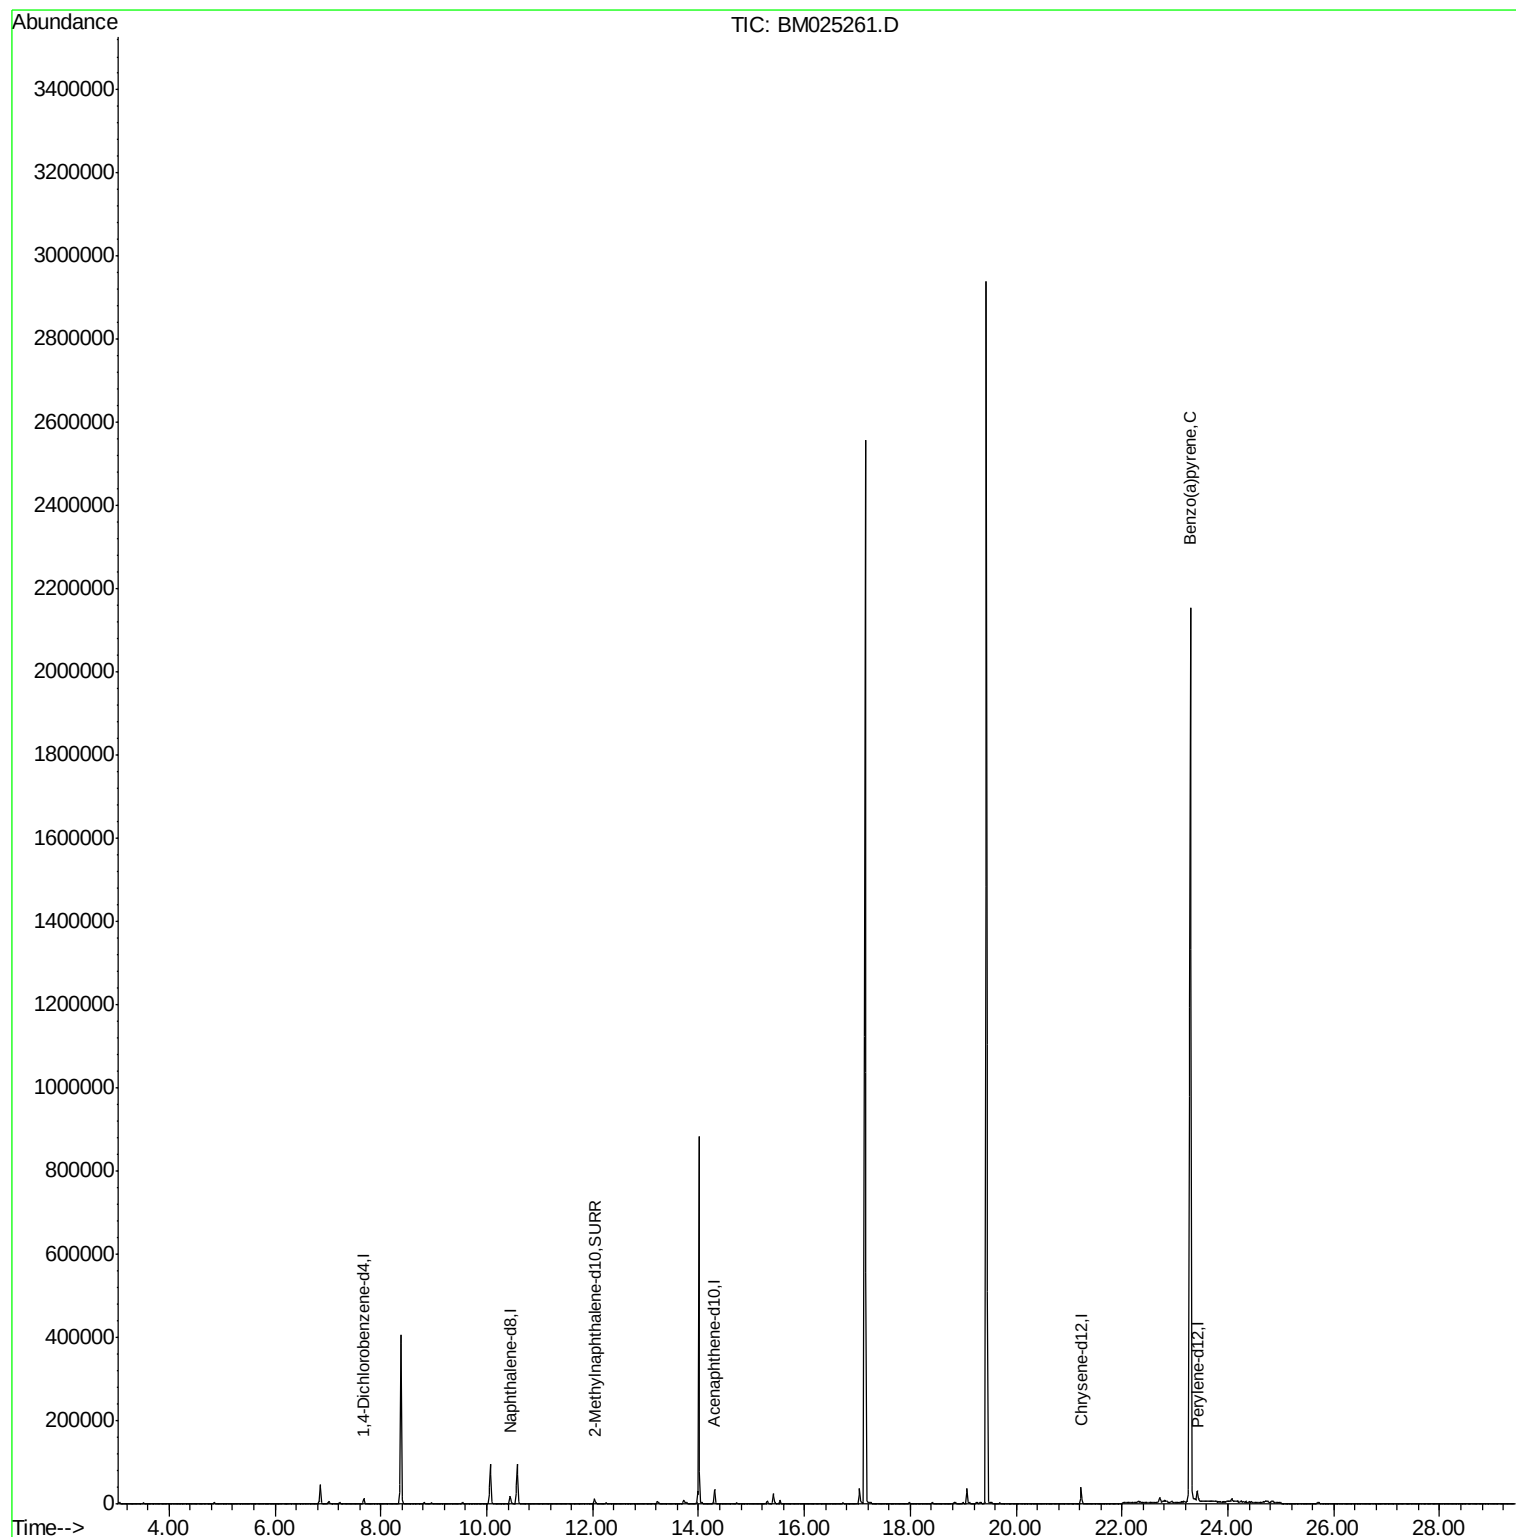

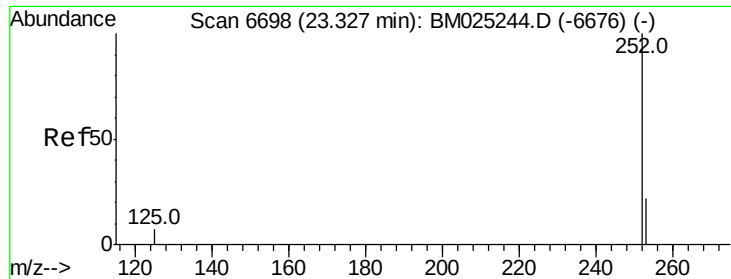

#23

Benzo(a)pyrene

Concen: 0.078 ng/ul

RT: 23.29 min Scan# 6682

Delta R.T. -0.03 min


Lab File: BM025261.D

Acq: 04 Mar 2020 21:46

Instrument :

BNA_M

ClientSampleId :

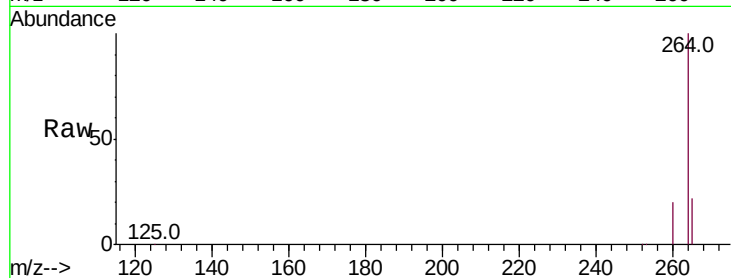

Tot Ion: 252 Resp: 8577

Ion Ratio Lower Upper

252 100

253 35.1 20.3 30.5#

125 24.7 13.0 19.4#

