

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030320\
 Data File : BM025294.D
 Acq On : 05 Mar 2020 18:56
 Operator : CG/JU
 Sample : L1543-14
 Misc :
 ALS Vial : 90 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Mar 06 02:45:46 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 04 08:02:03 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.67	152	3407	0.40	ng/ul	0.00
2) Naphthalene-d8	10.44	136	14787	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.30	164	10920	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.05
16) Chrysene-d12	21.23	240	25024	0.40	ng/ul	0.00
20) Perylene-d12	23.42	264	22861	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.04	152	7990	0.29	ng/ul	0.00
14) Fluoranthene-d10	19.07	212	23056	0.00	ng/ul	0.00
Target Compounds						
17) Pyrene	19.44	202	3064	0.032	ng/ul#	Ovalue 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030320\
Data File : BM025294.D
Acq On : 05 Mar 2020 18:56
Operator : CG/JU
Sample : L1543-14
Misc :
ALS Vial : 90 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Mar 06 02:45:46 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 04 08:02:03 2020
Response via : Initial Calibration

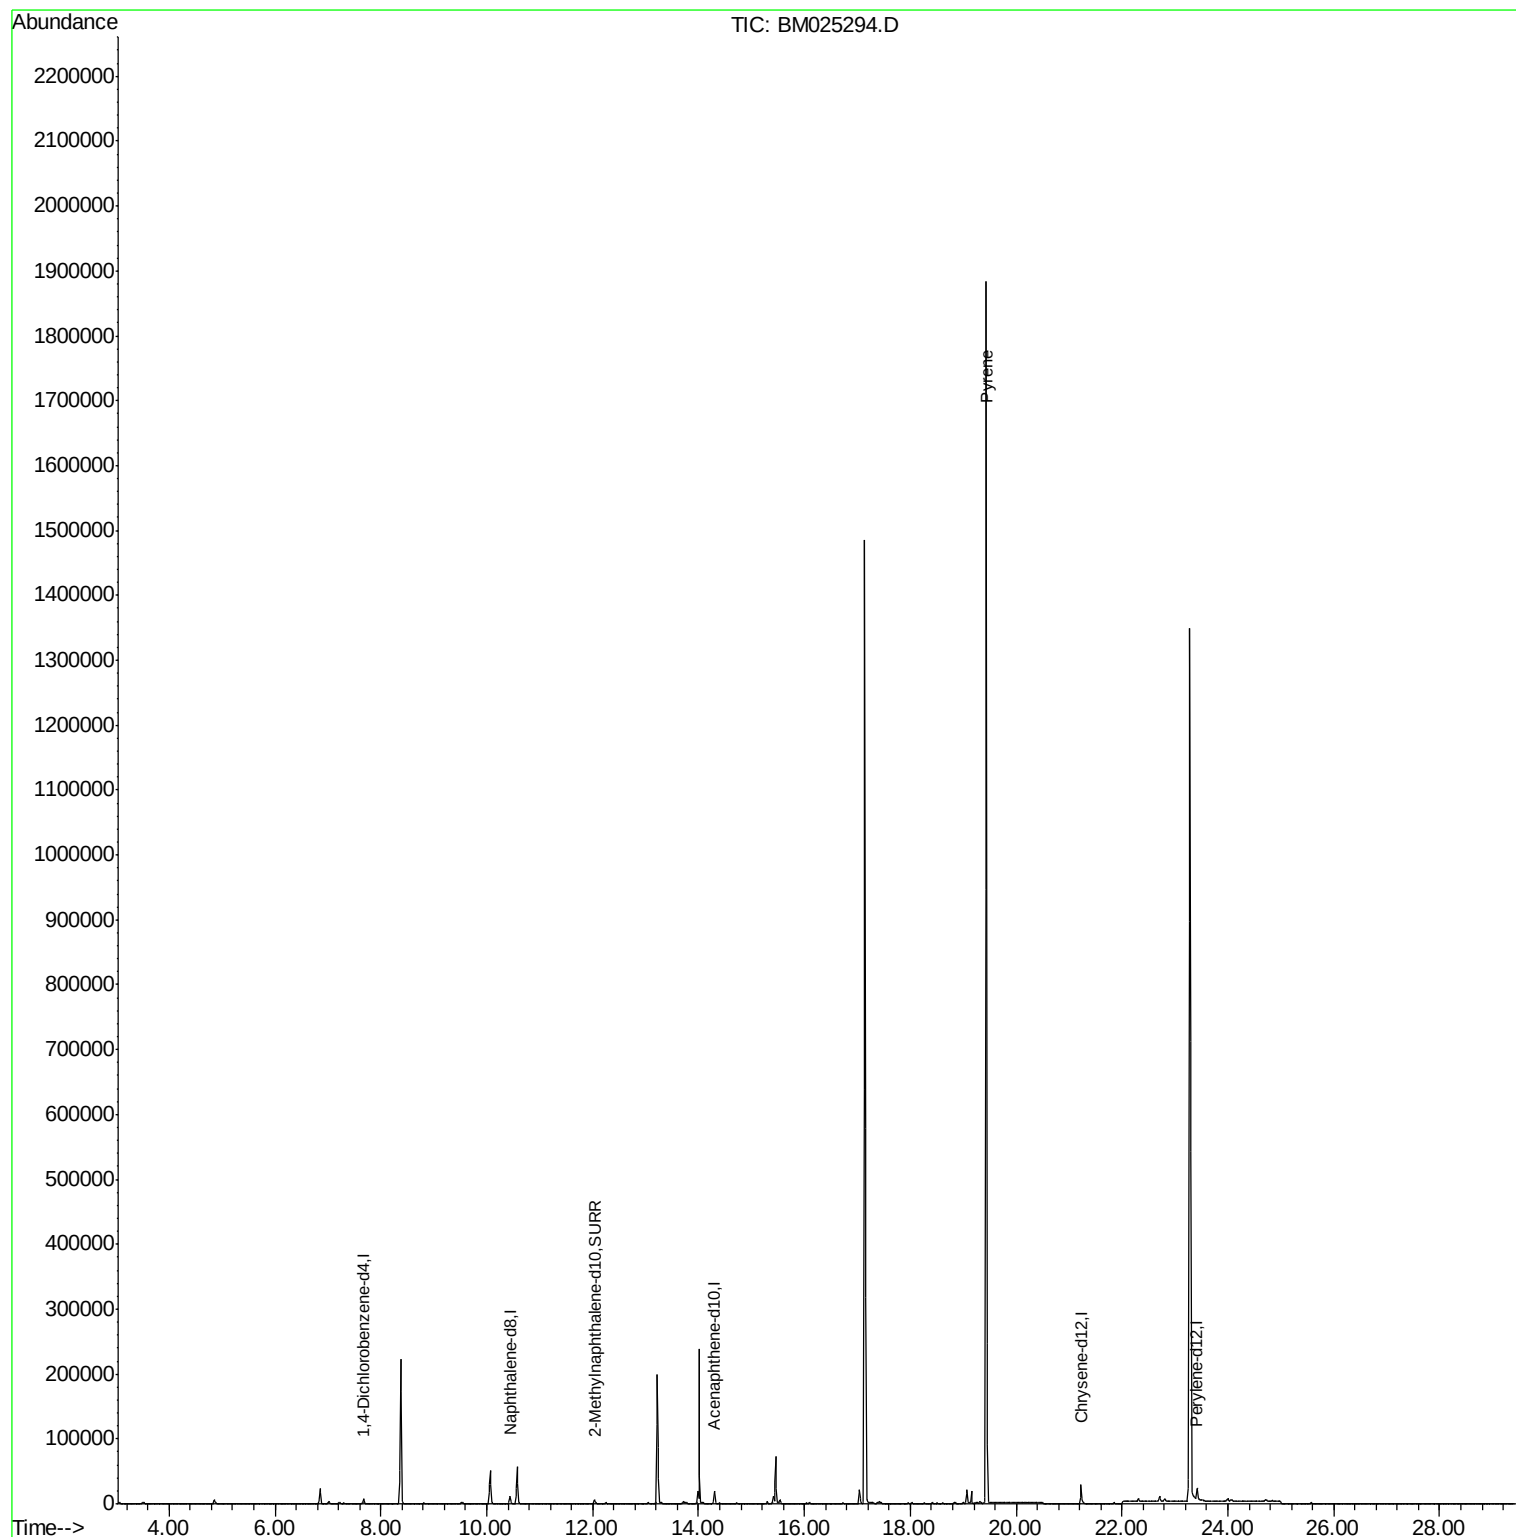

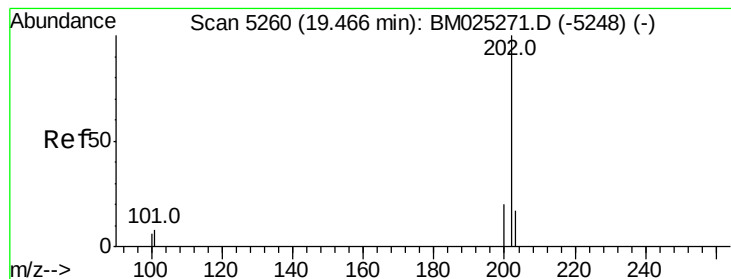

#17

Pvrene

Concen: 0.032 ng/ul

RT: 19.44 min Scan# 5252

Delta R.T. -0.03 min

Lab File: BM025294.D

Acq: 05 Mar 2020 18:56

Instrument :

BNA_M

ClientSampleId :


Tot Ion:202 Resp: 3064

Ion Ratio Lower Upper

202 100

101 151.7 8.7 13.1#

100 942.8 7.3 10.9#

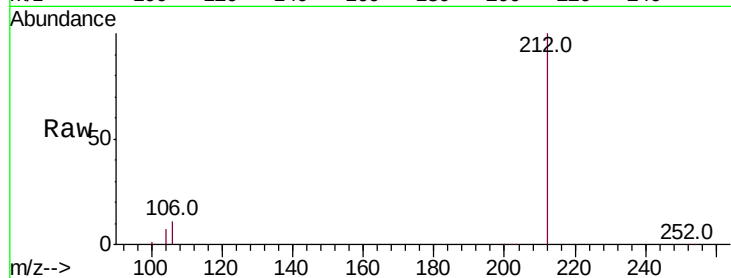

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

