

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030320\
 Data File : BM025304.D
 Acq On : 06 Mar 2020 02:10
 Operator : CG/JU
 Sample : L1568-04
 Misc :
 ALS Vial : 101 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Mar 06 02:46:32 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 04 08:02:03 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.67	152	3576	0.40	ng/ul	0.00
2) Naphthalene-d8	10.44	136	15743	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.30	164	11780	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.05
16) Chrysene-d12	21.23	240	27514	0.40	ng/ul	0.00
20) Perylene-d12	23.42	264	25861	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.04	152	7030	0.24	ng/ul	0.00
14) Fluoranthene-d10	19.07	212	22560	0.00	ng/ul	0.00
Target Compounds				Ovalue		
3) Naphthalene	10.49	128	1060	0.022	ng/ul	98
8) Acenaphthene	14.36	153	1241	0.029	ng/ul	97
9) Fluorene	15.35	166	1229	0.023	ng/ul	95
17) Pyrene	19.46	202	17413	0.167	ng/ul	98
18) Benzo(a)anthracene	21.21	228	7793	0.077	ng/ul	97
19) Chrysene	21.26	228	9584	0.086	ng/ul	99
21) Benzo(b)fluoranthene	22.76	252	22577	0.218	ng/ul	95
22) Benzo(k)fluoranthene	22.76	252	22577	0.208	ng/ul	94
23) Benzo(a)pyrene	23.32	252	6460	0.074	ng/ul#	84
24) Indeno(1,2,3-cd)pyrene	25.59	276	3872	0.036	ng/ul#	100
26) Benzo(g,h,i)perylene	26.26	276	3515	0.038	ng/ul#	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030320\
Data File : BM025304.D
Acq On : 06 Mar 2020 02:10
Operator : CG/JU
Sample : L1568-04
Misc :
ALS Vial : 101 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Mar 06 02:46:32 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 04 08:02:03 2020
Response via : Initial Calibration

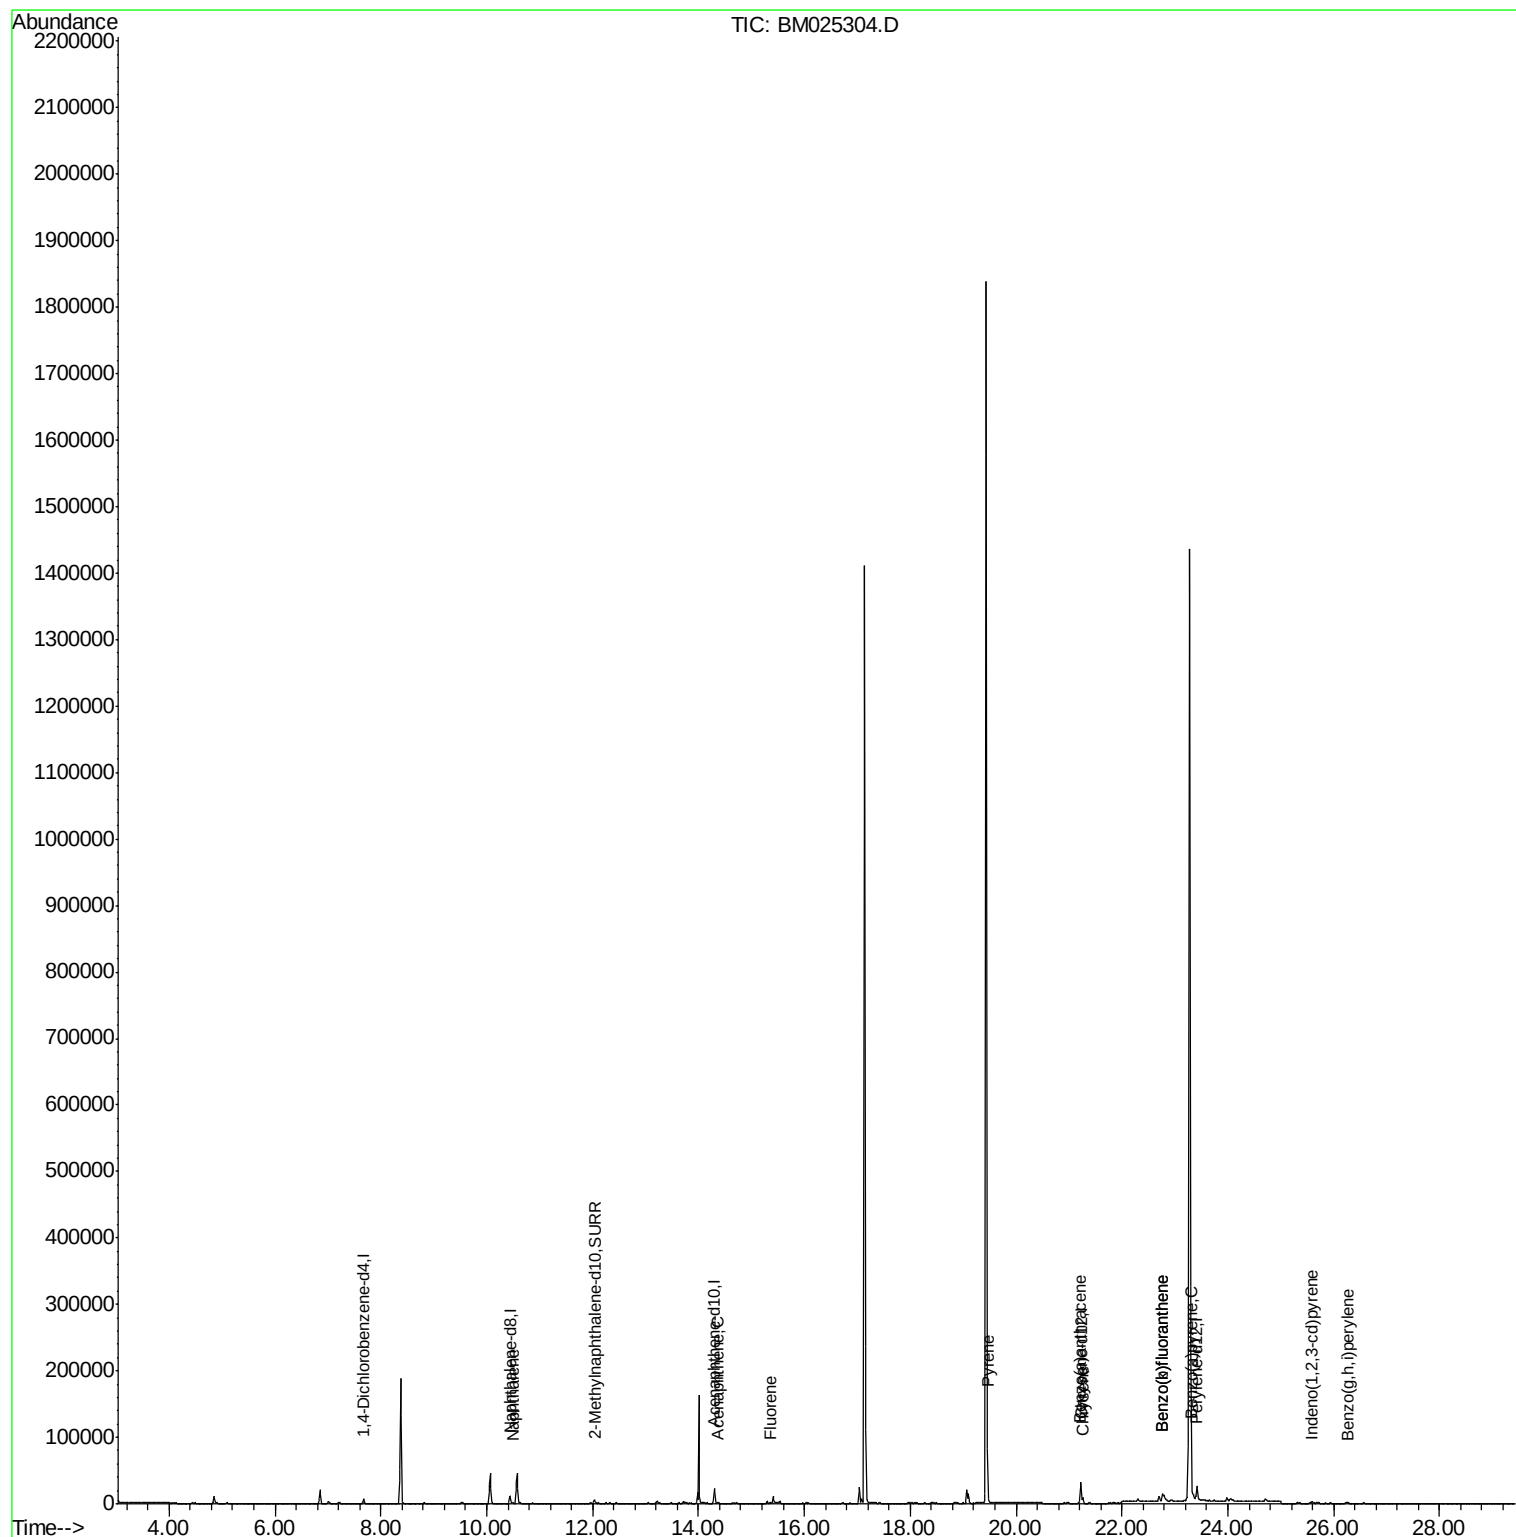

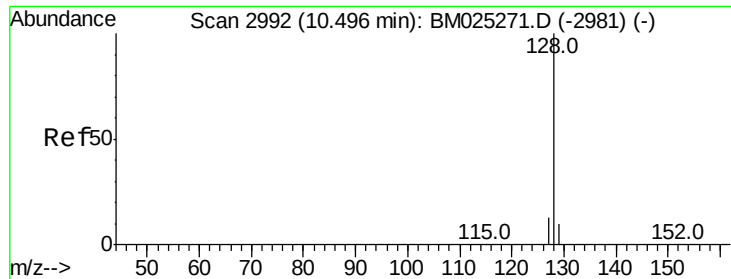

#3

Naphthalene

Concen: 0.022 ng/ul

RT: 10.49 min Scan# 2990

Delta R.T. -0.00 min

Lab File: BM025304.D

Acq: 06 Mar 2020 02:10

Instrument :

BNA_M

ClientSampled :


Tot Ion:128 Resp: 1060

Ion Ratio Lower Upper

128 100

129 20.1 17.0 25.6




127 18.9 15.7 23.5

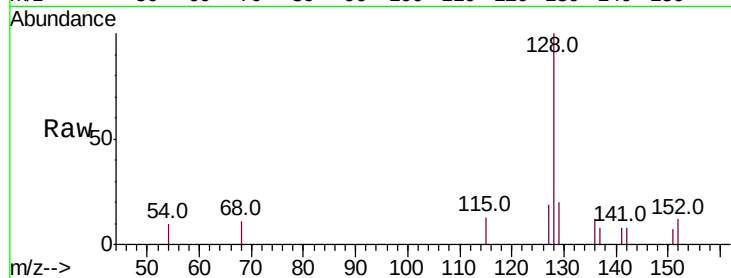

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

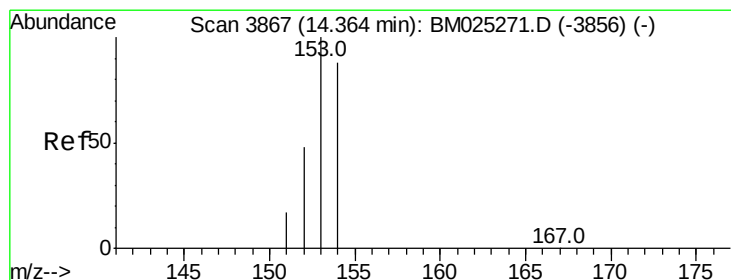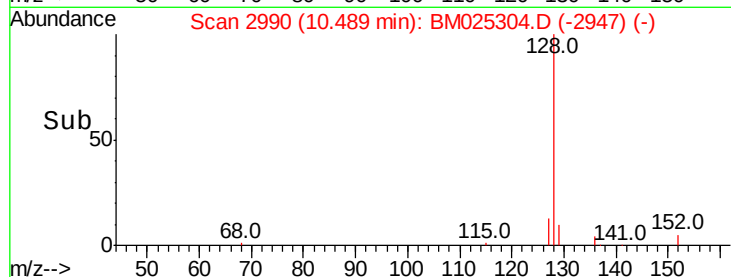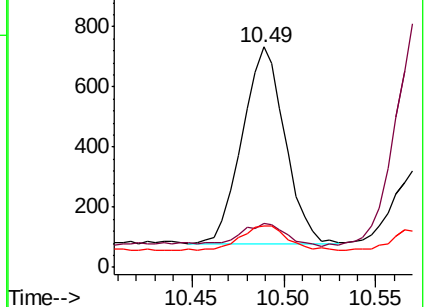

#8

Acenaphthene

Concen: 0.029 ng/ul

RT: 14.36 min Scan# 3866

Delta R.T. -0.00 min

Lab File: BM025304.D

Acq: 06 Mar 2020 02:10


Tgt Ion:153 Resp: 1241

Ion Ratio Lower Upper

153 100

152 52.0 40.0 60.0



154 91.4 71.0 106.6

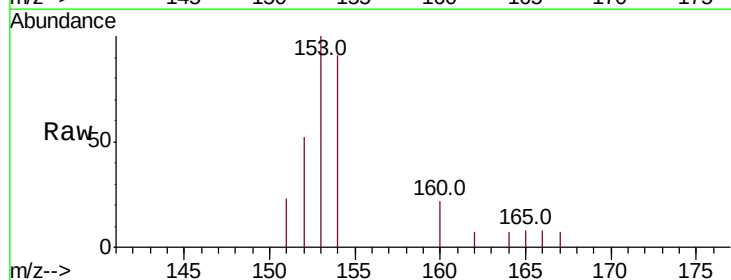


Abundance Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E

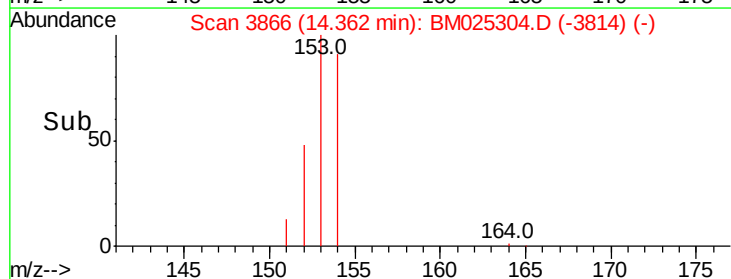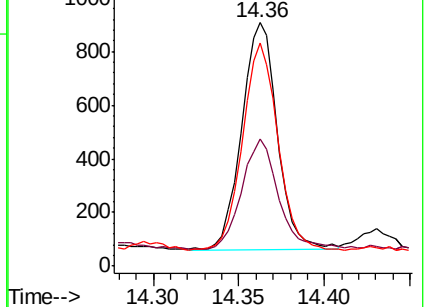


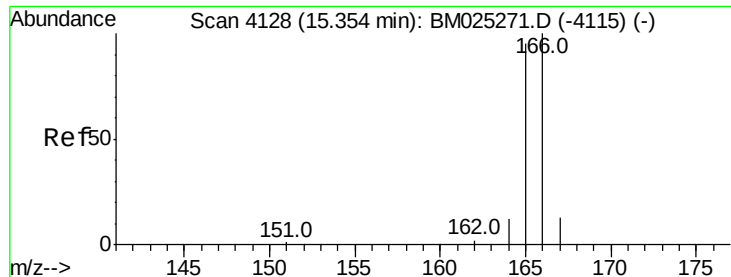




#9
Fluorene
 Concen: 0.023 ng/ul
 RT: 15.35 min Scan# 4127
 Delta R.T. -0.00 min
 Lab File: BM025304.D
 Acq: 06 Mar 2020 02:10

Instrument :
 BNA_M
 ClientSampleId :

Tot Ion:166 Resp: 1229
 Ion Ratio Lower Upper
 166 100
 165 94.8 80.0 120.0
 167 19.0 13.7 20.5

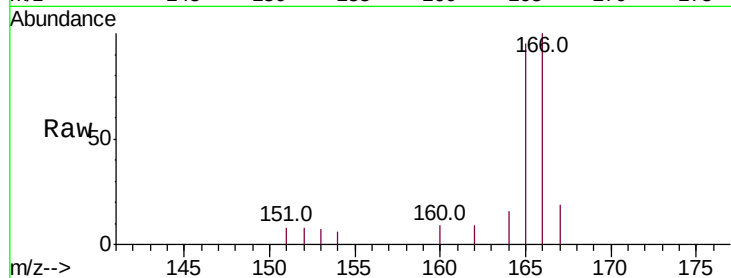


Abundance Ion 166.00 (165.70 to 166.70): E
 Ion 165.00 (164.70 to 165.70): E
 Ion 167.00 (166.70 to 167.70): E

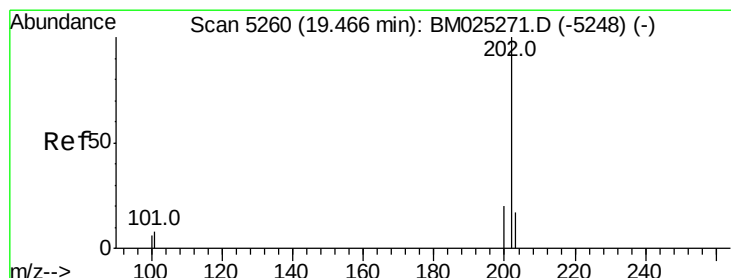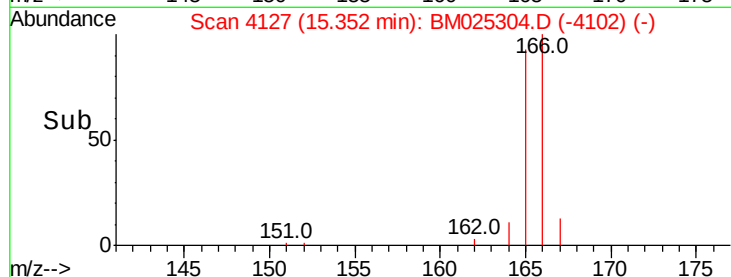
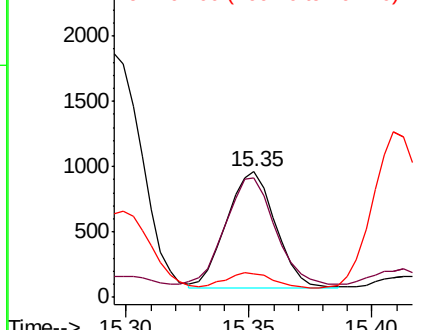



#17
Pyrene
 Concen: 0.167 ng/ul
 RT: 19.46 min Scan# 5259
 Delta R.T. -0.00 min
 Lab File: BM025304.D
 Acq: 06 Mar 2020 02:10

Tgt Ion:202 Resp: 17413
 Ion Ratio Lower Upper
 202 100
 101 9.9 8.7 13.1
 100 8.6 7.3 10.9

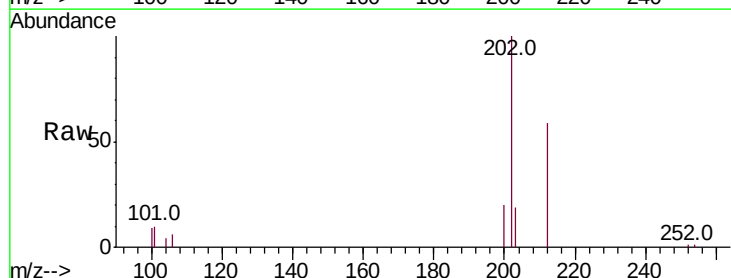

Abundance Ion 202.00 (201.70 to 202.70): E
 Ion 101.00 (100.70 to 101.70): E
 Ion 100.00 (99.70 to 100.70): E



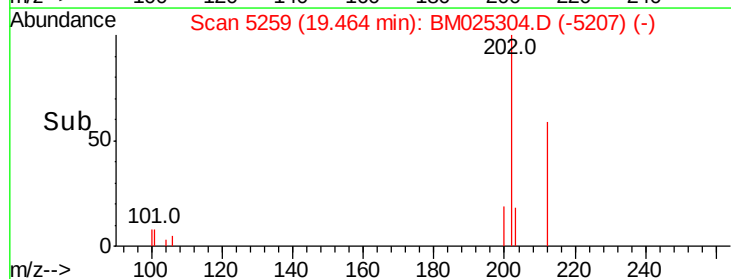
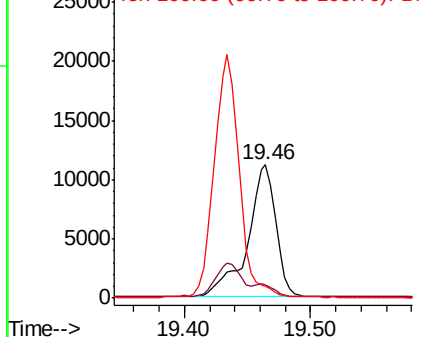


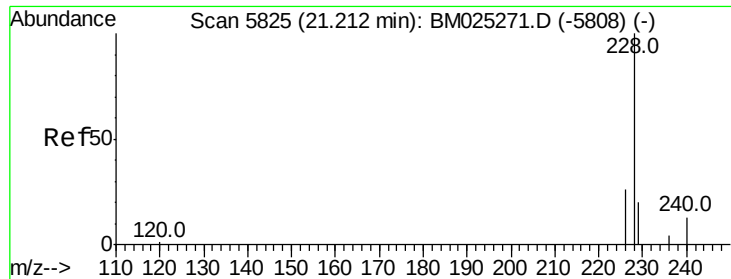

#18
Benzo(a)anthracene
Concen: 0.077 ng/ul
RT: 21.21 min Scan# 5823
Delta R.T. -0.00 min
Lab File: BM025304.D
Acq: 06 Mar 2020 02:10




Instrument :
BNA_M
ClientSampleId :


Tot Ion:228 Resp: 7793
Ion Ratio Lower Upper
228 100
229 21.8 16.6 25.0
226 28.9 21.9 32.9

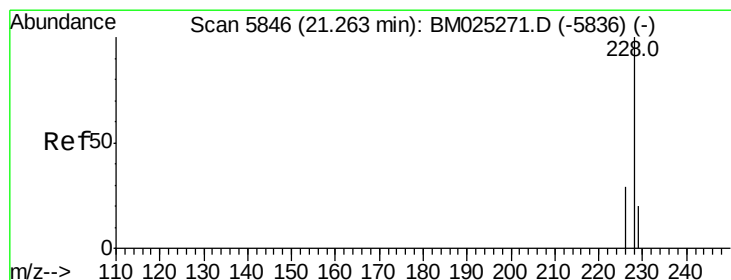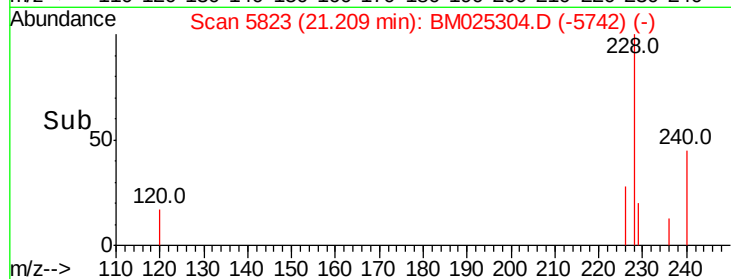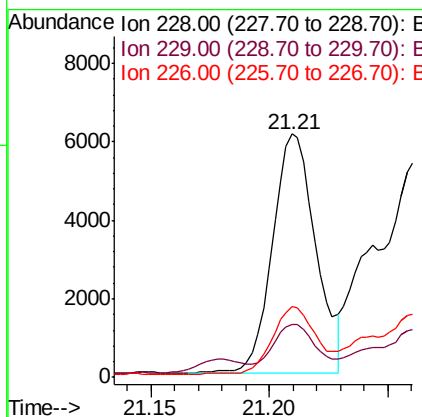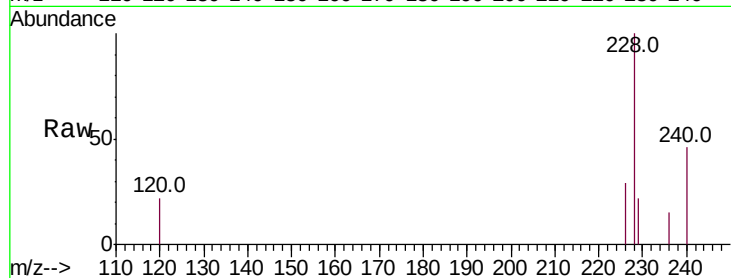

#19
Chrysene
Concen: 0.086 ng/ul
RT: 21.26 min Scan# 5844
Delta R.T. -0.01 min
Lab File: BM025304.D
Acq: 06 Mar 2020 02:10

Tgt Ion:228 Resp: 9584
Ion Ratio Lower Upper
228 100
226 29.7 23.8 35.8
229 22.3 16.9 25.3

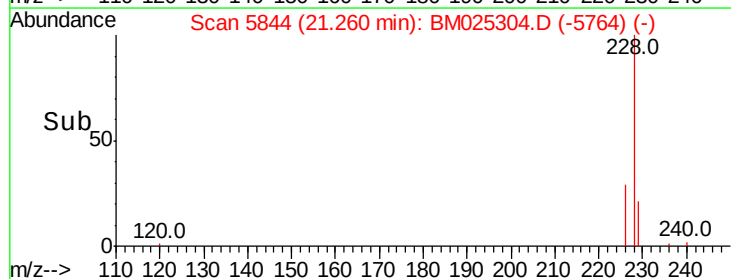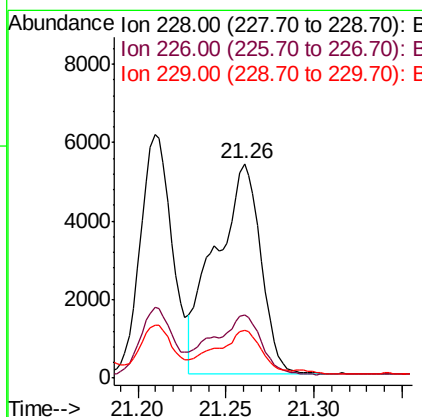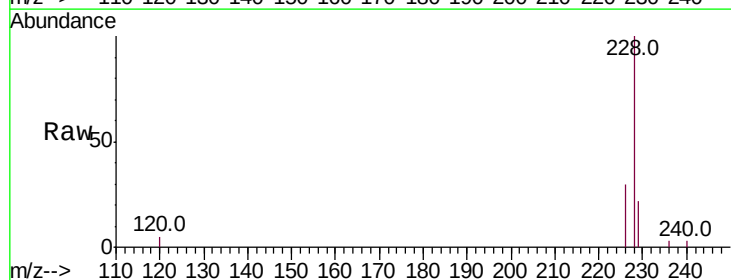

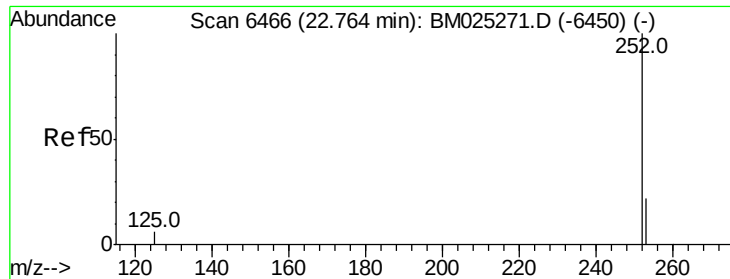

#21

Benzo(b)fluoranthene

Concen: 0.218 ng/ul

RT: 22.76 min Scan# 6464

Delta R.T. -0.01 min

Lab File: BM025304.D

Acq: 06 Mar 2020 02:10

Instrument :

BNA_M

ClientSampleId :


Tot Ion:252 Resp: 22577

Ion Ratio Lower Upper

252 100

253 27.9 0.0 49.8




125 12.6 0.0 28.6

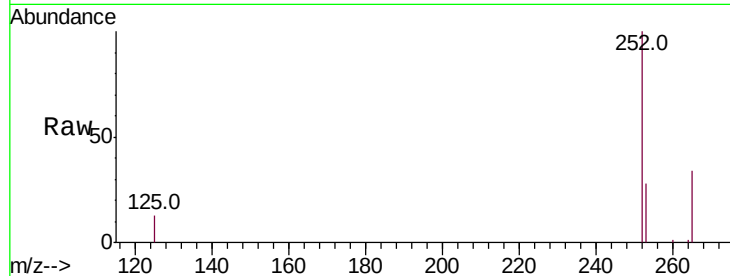

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

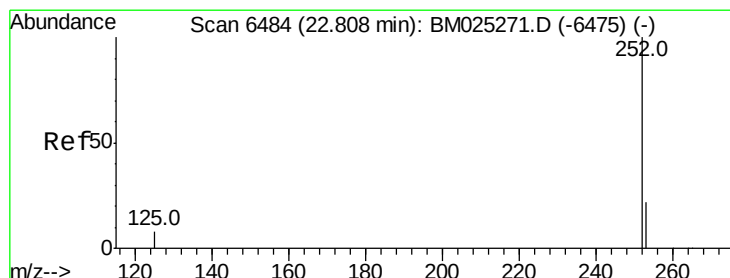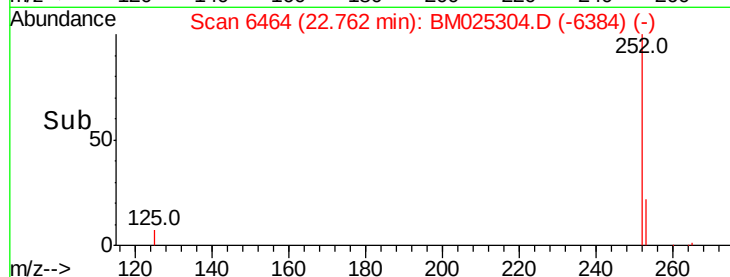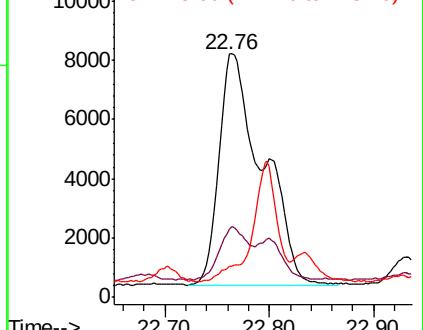

#22

Benzo(k)fluoranthene

Concen: 0.208 ng/ul

RT: 22.76 min Scan# 6464

Delta R.T. -0.05 min

Lab File: BM025304.D

Acq: 06 Mar 2020 02:10


Tgt Ion:252 Resp: 22577

Ion Ratio Lower Upper

252 100

253 27.9 19.4 29.0



125 12.6 10.7 16.1

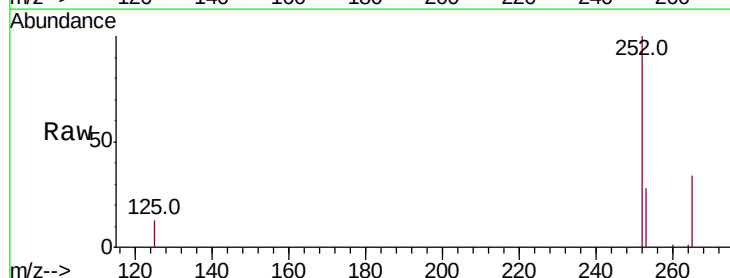


Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

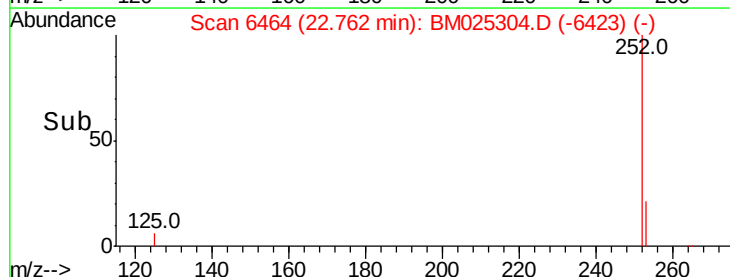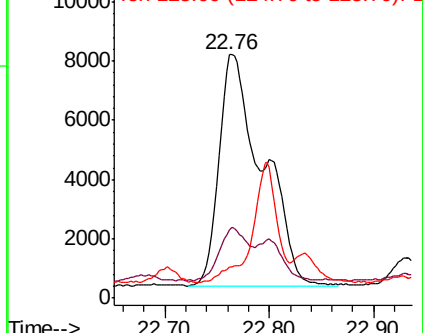

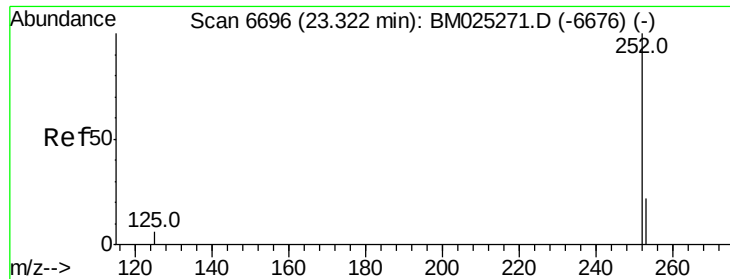

#23

Benzo(a)pyrene

Concen: 0.074 ng/ul

RT: 23.32 min Scan# 6696

Delta R.T. 0.00 min

Lab File: BM025304.D

Acq: 06 Mar 2020 02:10

Instrument :

BNA_M

ClientSampleId :


Tot Ion:252 Resp: 6460

Ion Ratio Lower Upper

252 100

253 34.1 20.3 30.5#




125 21.6 13.0 19.4#

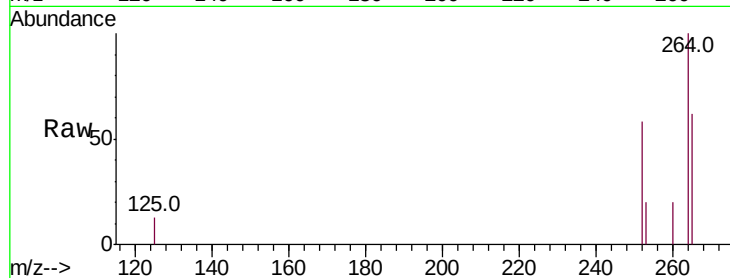

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

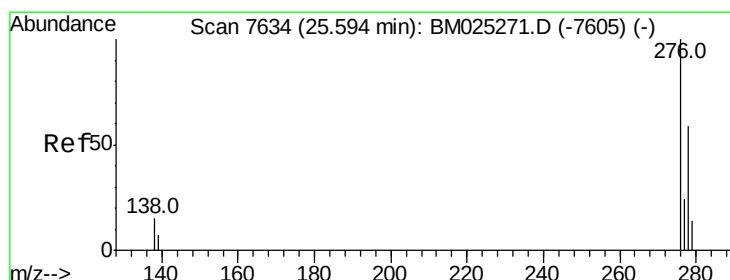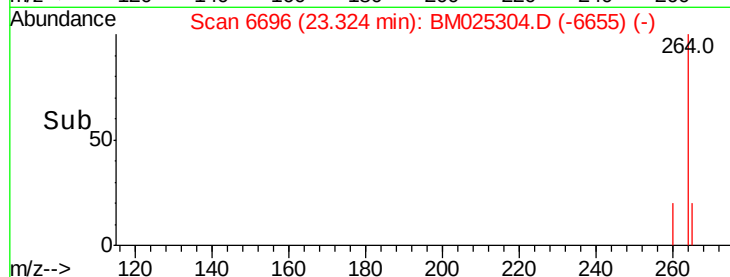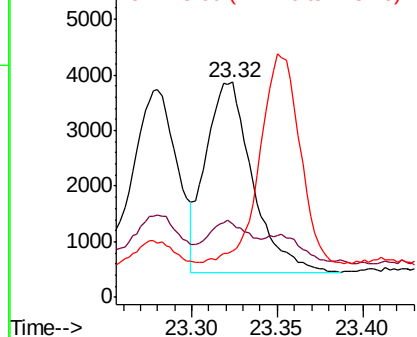

#24

Indeno(1,2,3-cd)pyrene

Concen: 0.036 ng/ul

RT: 25.59 min Scan# 7632

Delta R.T. -0.01 min

Lab File: BM025304.D

Acq: 06 Mar 2020 02:10


Tgt Ion:276 Resp: 3872

Ion Ratio Lower Upper

276 100

138 24.8 0.0 0.0#



227 0.0 0.0 0.0

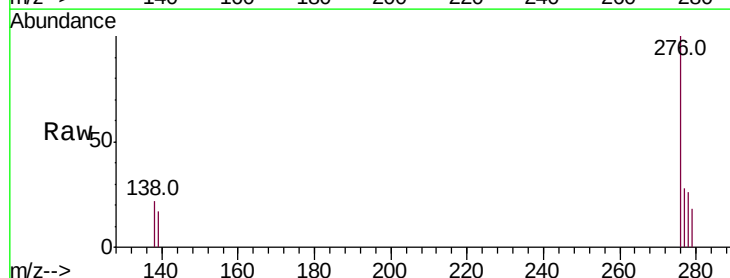


Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 227.00 (226.70 to 227.70): E

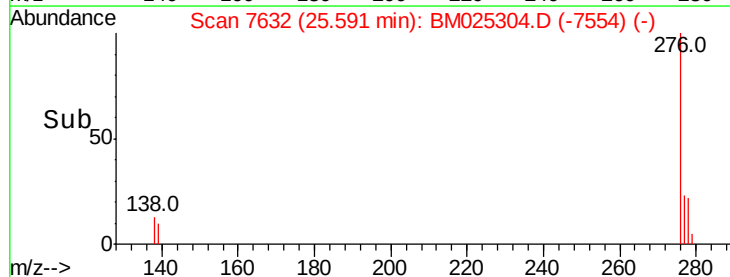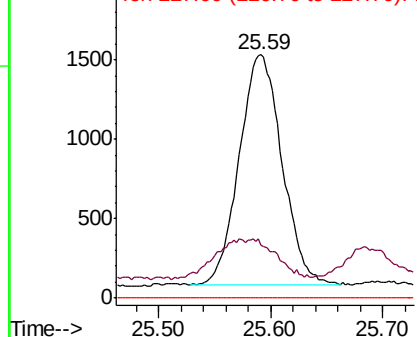

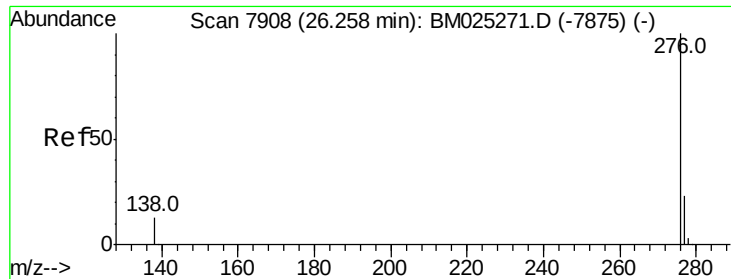

#26

Benzo(a,h,i)perylene

Concen: 0.038 ng/ul

RT: 26.26 min Scan# 7906

Delta R.T. -0.01 min

Lab File: BM025304.D

Acq: 06 Mar 2020 02:10

Instrument :

BNA_M

ClientSampleId :


Tot Ion:276 Resp: 3515

Ion Ratio Lower Upper

276 100

138 20.8 17.9 26.9

277 30.8 20.5 30.7#

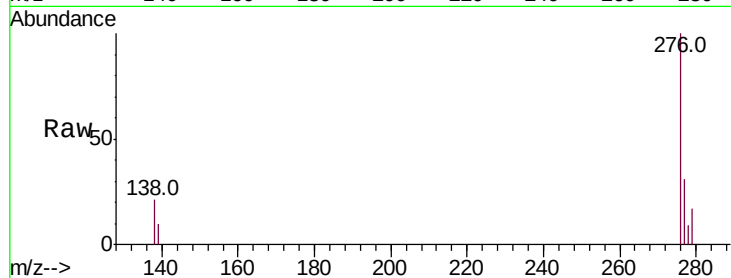

Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

