


Data File : BM025220.D  
Acq On : 03 Mar 2020 20:00  
Operator : CG/JU  
Sample : PB126890BL  
Misc :  
ALS Vial : 16 Sample Multiplier: 1

Instrument :  
BNA\_M  
Client Sampled :  
SBLK90

Quant Time: Mar 04 01:00:34 2020  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SOM-EPA-SIM-BM030320.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Mar 04 00:52:51 2020  
Response via : Initial Calibration

Manual Integrations  
APPROVED

mohammad  
3/4/2020 7:53:04 AM

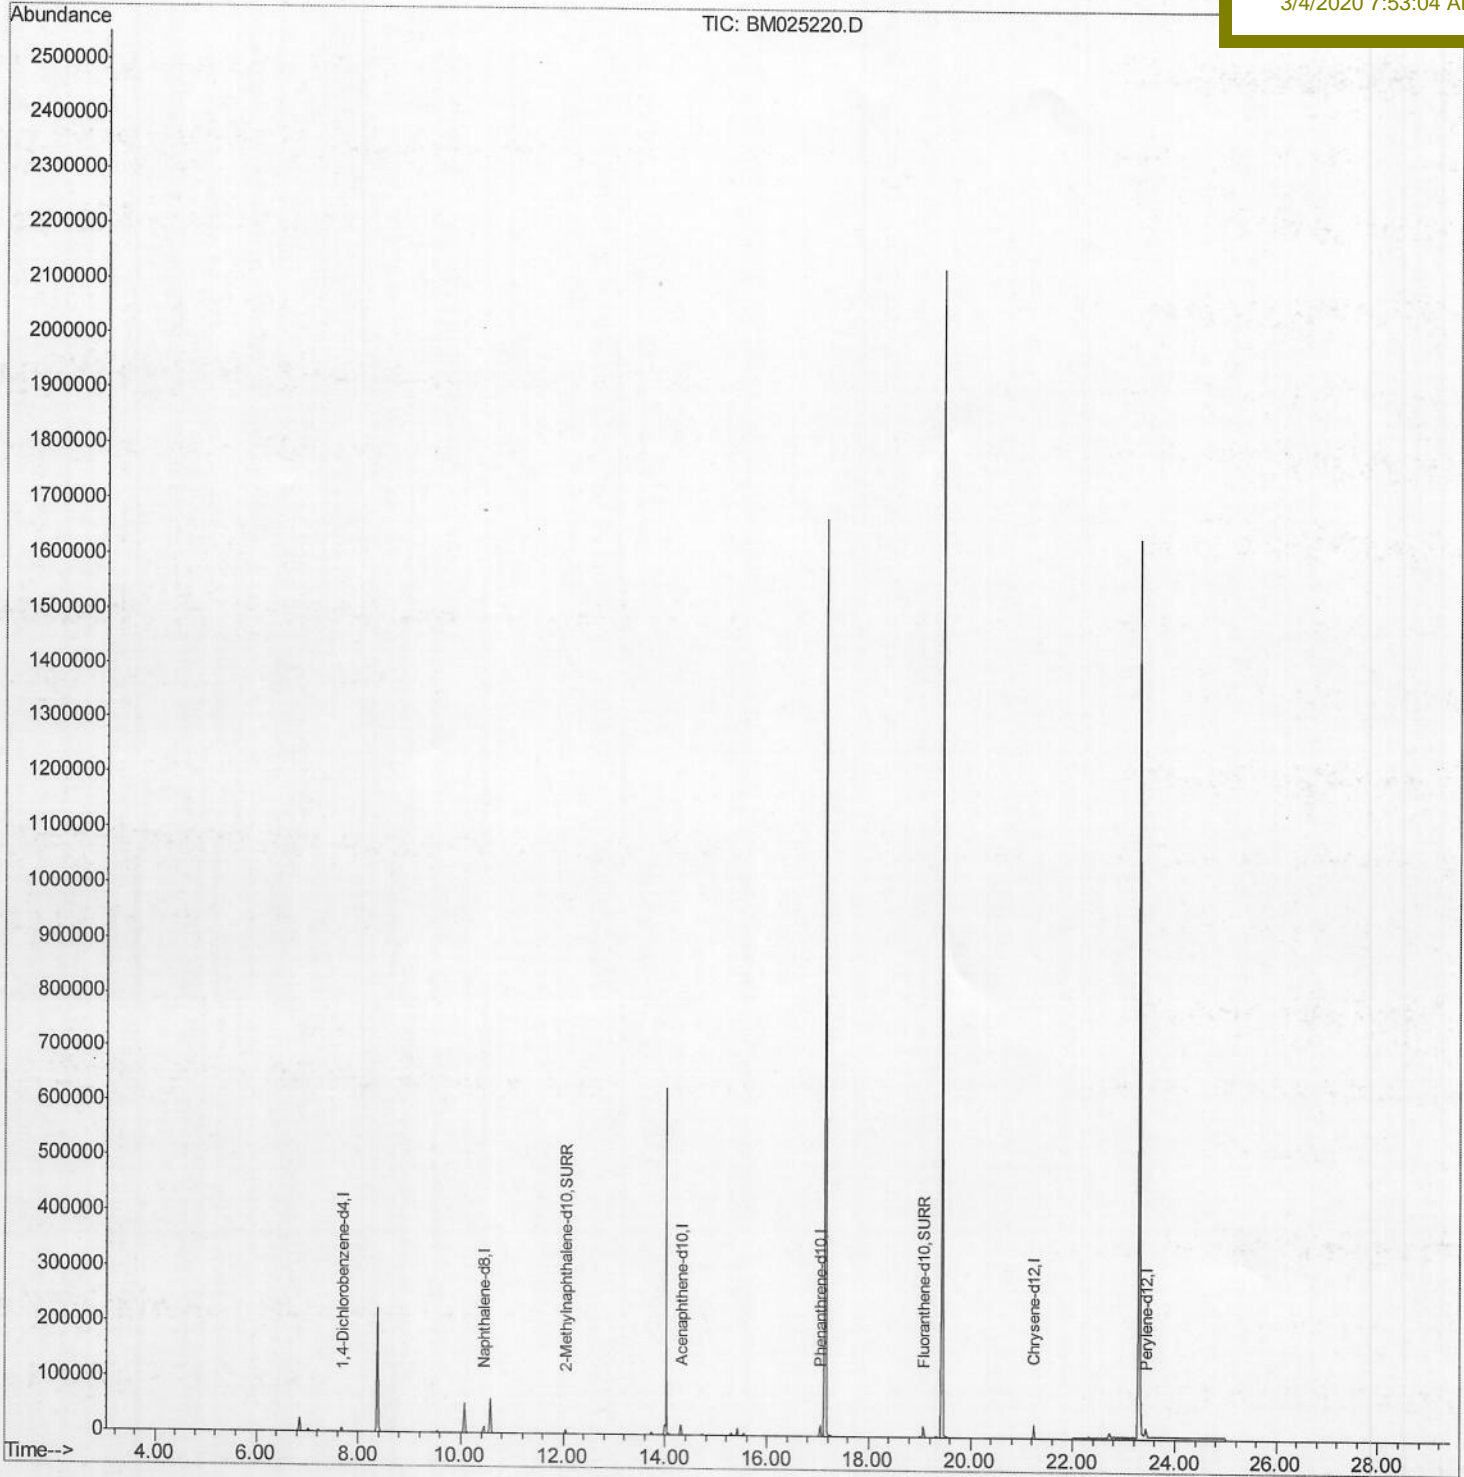

Data Path : Z:\SVOASRV\HPCHEM1\BNA\_M\DATA\BM030320\  
Quantitation Report (Qedit)




Data File : BM025220.D  
Acq On : 03 Mar 2020 20:00  
Operator : CG/JU  
Sample : PB126890BL  
Misc :  
ALS Vial : 16 Sample Multiplier: 1

Quant Time: Mar 04 00:54:50 2020  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SOM-EPA-SIM-BM030320.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Mar 04 00:52:51 2020  
Response via : Initial Calibration

Instrument :  
BNA\_M  
Client Sampled :  
SBLK90

Manual Integrations  
APPROVED

mohammad  
3/4/2020 7:53:04 AM

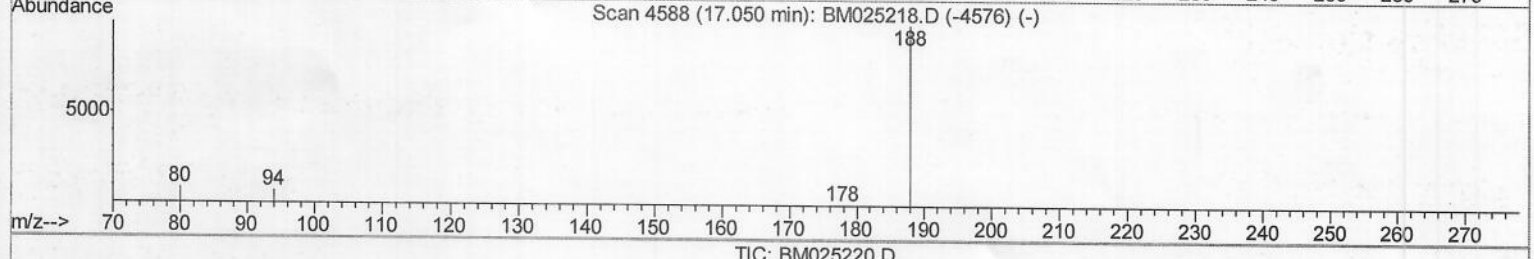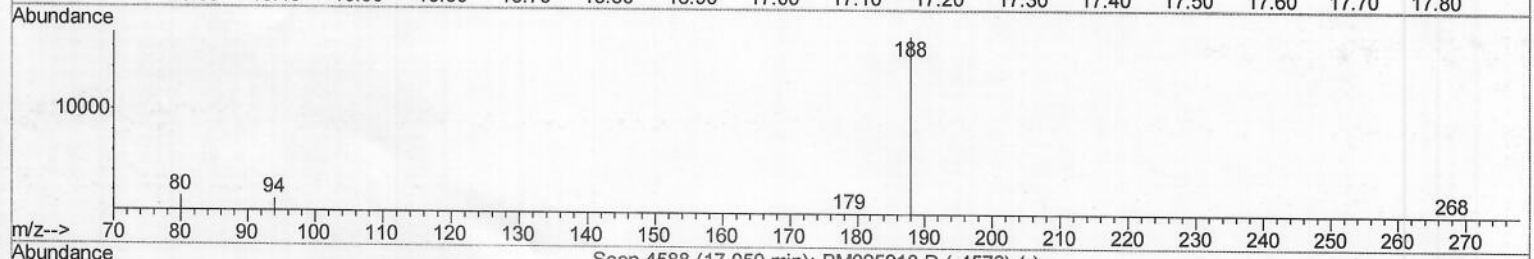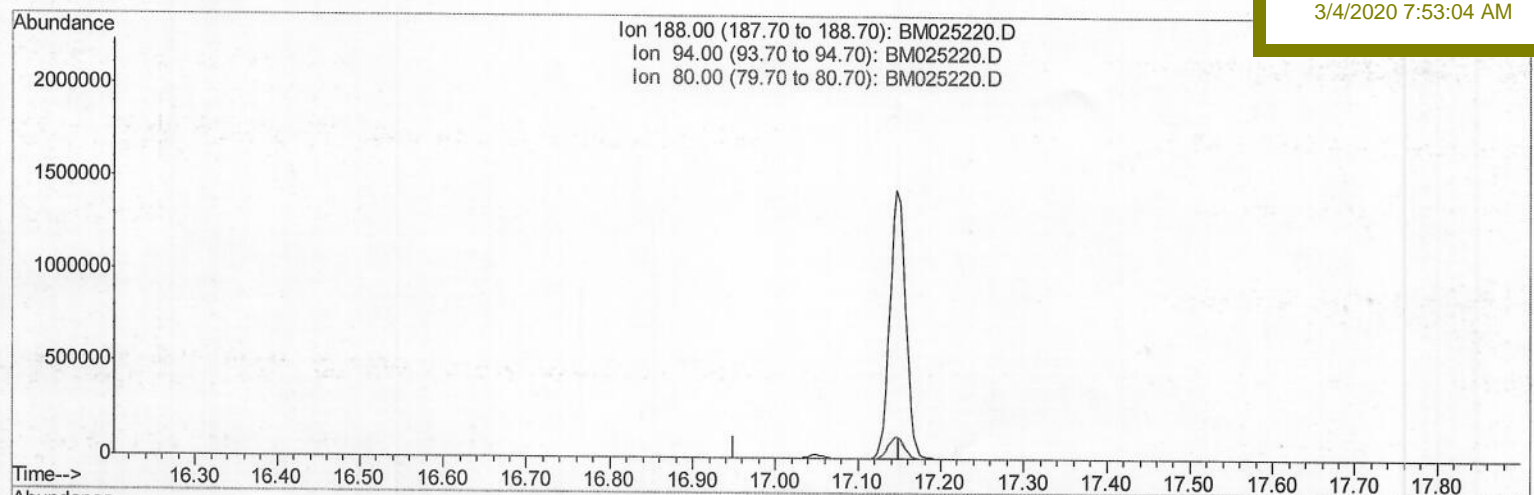

TIC: BM025220.D

(10) Phenanthrene-d10 (I)  
17.050min (-17.050) 0.00ng/ul  
response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	26.60	0.00#
80.00	22.60	0.00#
0.00	0.00	0.00



Data Path : Z:\SVOASRV\HPCHEM1\BNA\_M\DATA\BM030320\  
Quantitation Report (Qedit)




Data File : BM025220.D  
Acq On : 03 Mar 2020 20:00  
Operator : CG/JU  
Sample : PB126890BL  
Misc :  
ALS Vial : 16 Sample Multiplier: 1

Quant Time: Mar 04 00:59:55 2020  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SOM-EPA-SIM-BM030320.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Mar 04 00:52:51 2020  
Response via : Initial Calibration

Instrument :  
BNA\_M  
ClientSampleId :  
SBLK90

Manual Integrations  
APPROVED

mohammad  
3/4/2020 7:53:04 AM

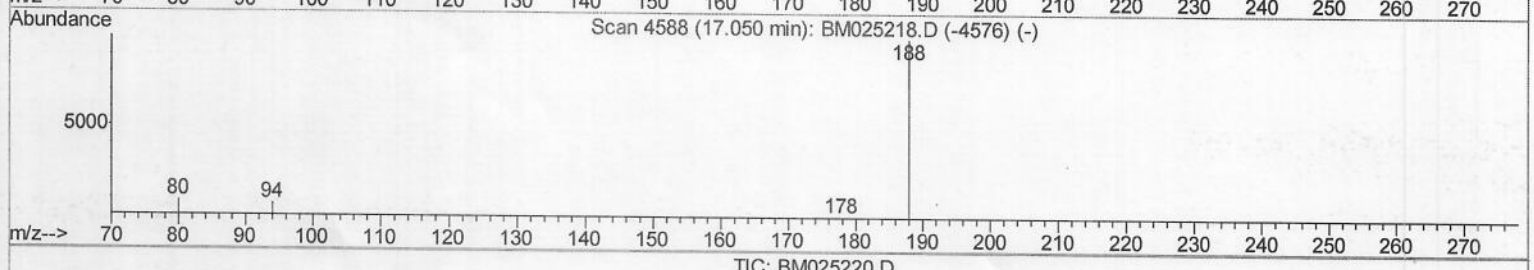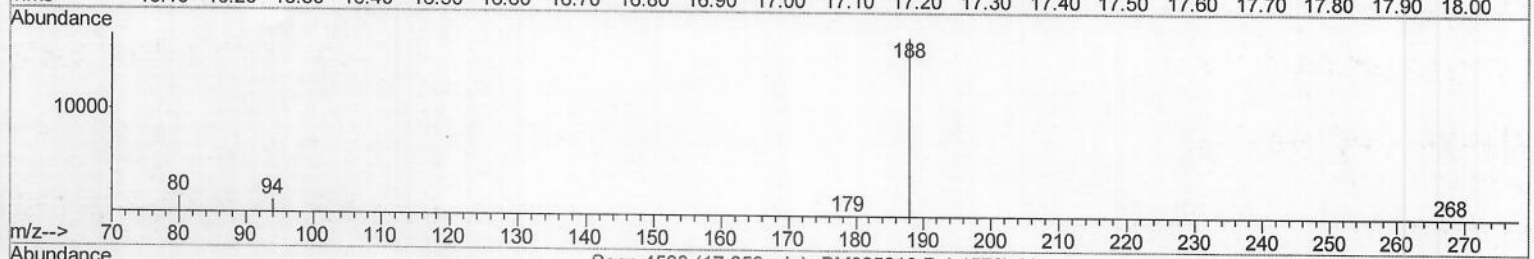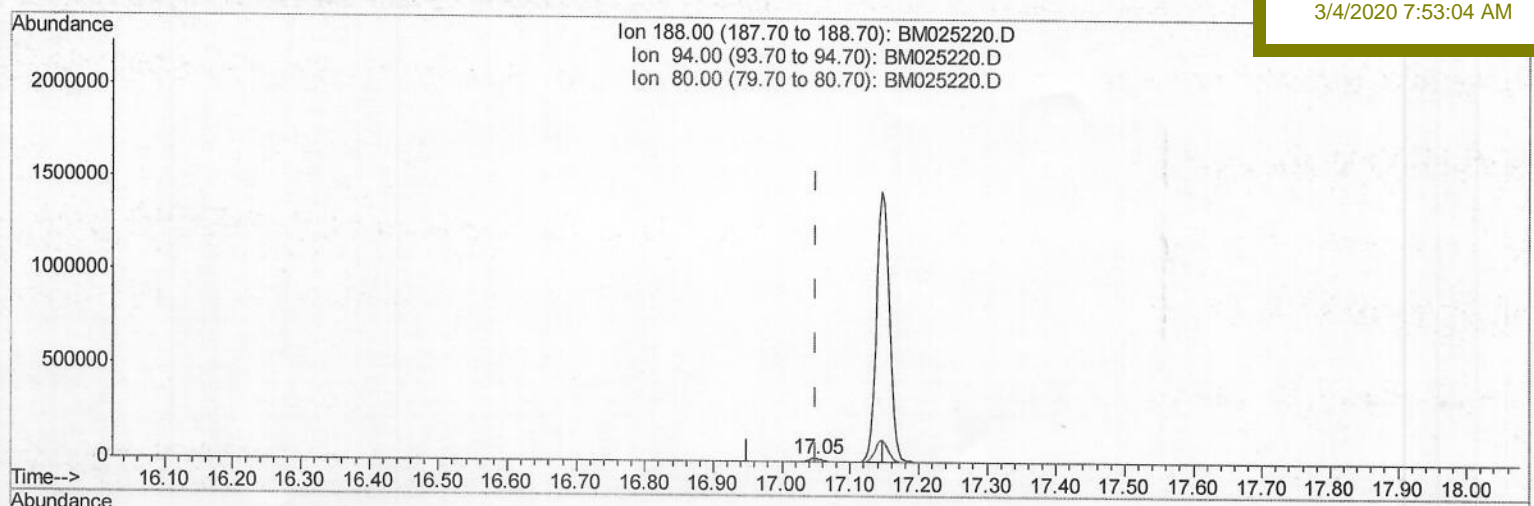

TIC: BM025220.D

(10) Phenanthrene-d10 (I)

17.050min (+0.000) 0.40ng/ul m >JU 03/05/20

response 23529

Ion	Exp%	Act%
188.00	100	100
94.00	26.60	7.39#
80.00	22.60	8.69#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA\_M\DATA\BM030320\  
Quantitation Report (QT Reviewed)

Data File : BM025220.D  
Acq On : 03 Mar 2020 20:00  
Operator : CG/JU  
Sample : PB126890BL  
Misc :  
ALS Vial : 16 Sample Multiplier: 1

Quant Time: Mar 04 01:00:34 2020  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SOM-EPA-SIM-BM030320.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Mar 04 00:52:51 2020  
Response via : Initial Calibration

Instrument :  
BNA\_M  
Client Sampled :  
SBLK90

Manual Integrations  
APPROVED

mohammad  
3/4/2020 7:53:04 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	7.68	152	3182	0.40	ng/ul	0.00
2) Naphthalene-d8	10.45	136	13270	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.31	164	10019	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.05	188	23529m	0.40	ng/ul	0.00
16) Chrysene-d12	21.24	240	22540	0.40	ng/ul	0.00
20) Perylene-d12	23.43	264	20879	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.04	152	7869	0.32	ng/ul	0.00
14) Fluoranthene-d10	19.08	212	22933	0.30	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

CG JU 03/05/20