

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM030320\
Quantitation Report (QT Reviewed)


Data File : BM025224.D
Acq On : 03 Mar 2020 22:26
Operator : CG/JU
Sample : L1542-13
Misc :
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Mar 04 01:11:20 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 04 00:52:51 2020
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
DBD49

Manual Integrations
APPROVED

mohammad
3/4/2020 7:53:54 AM

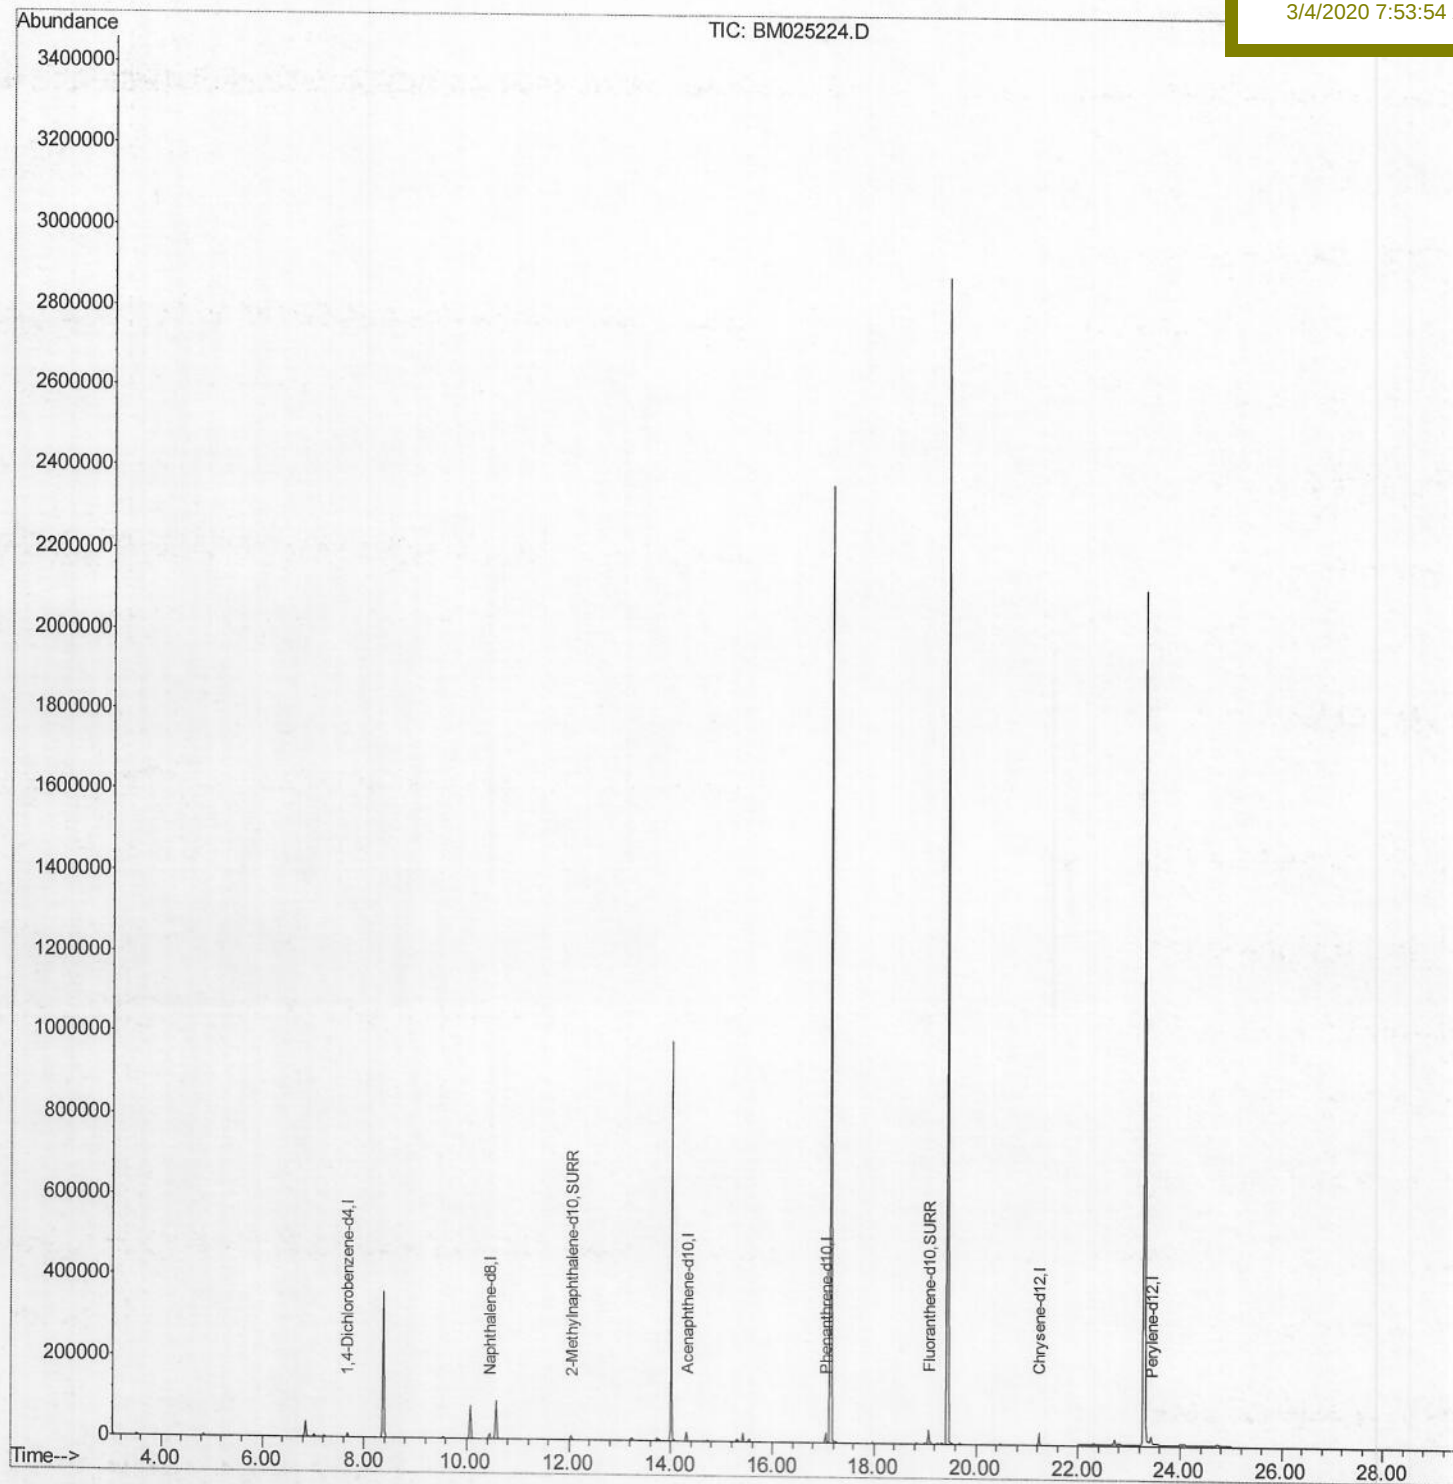

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM030320\
Quantitation Report (Qedit)




Data File : BM025224.D
Acq On : 03 Mar 2020 22:26
Operator : CG/JU
Sample : L1542-13
Misc :
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Mar 04 00:55:13 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 04 00:52:51 2020
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
DBD49

Manual Integrations
APPROVED

mohammad
3/4/2020 7:53:54 AM

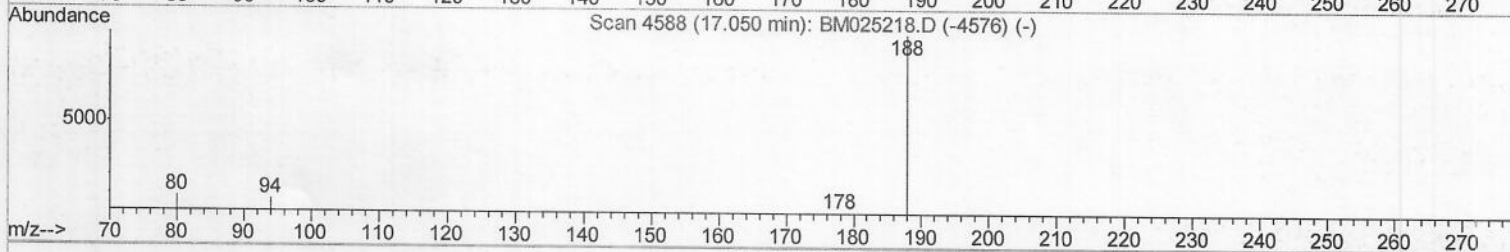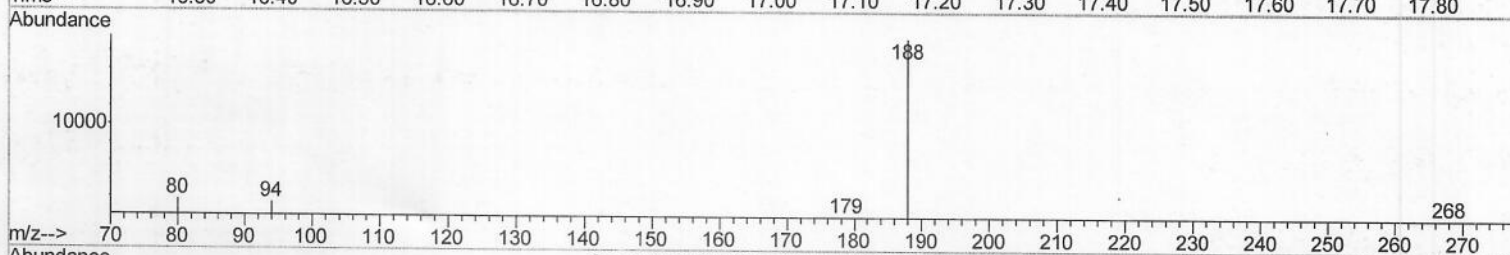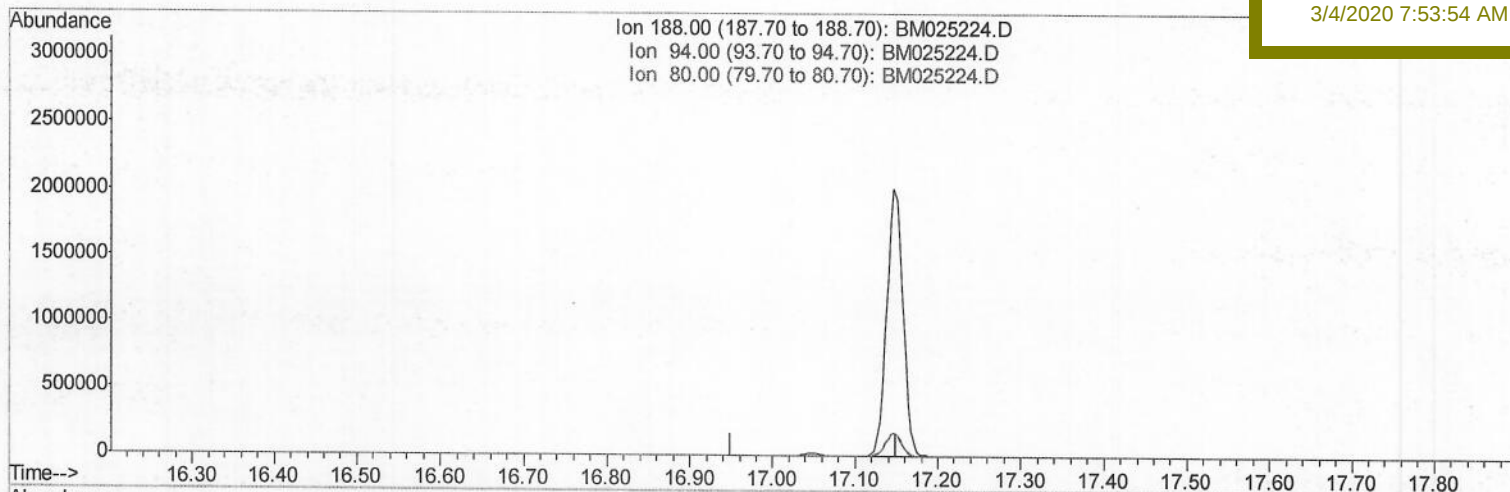

TIC: BM025224.D

(10) Phenanthrene-d10 (I)

17.050min (-17.050) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	26.60	0.00#
80.00	22.60	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM030320\
Quantitation Report (Qedit)




Data File : BM025224.D
Acq On : 03 Mar 2020 22:26
Operator : CG/JU
Sample : L1542-13
Misc :
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Mar 04 00:55:13 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 04 00:52:51 2020
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
DBD49

Manual Integrations
APPROVED

mohammad
3/4/2020 7:53:54 AM

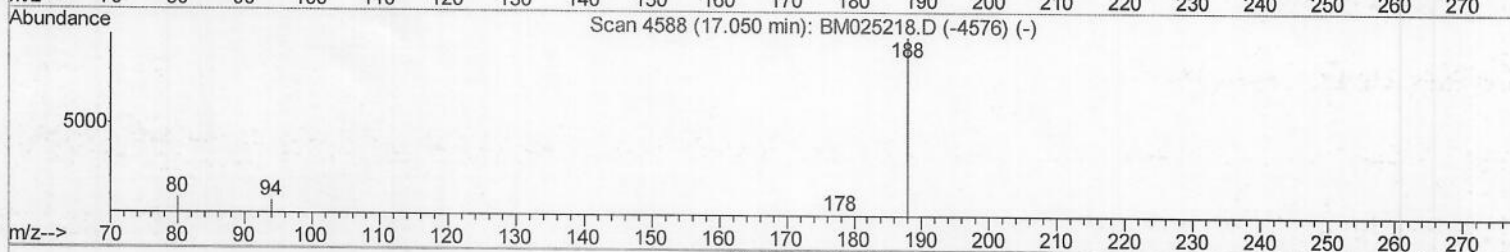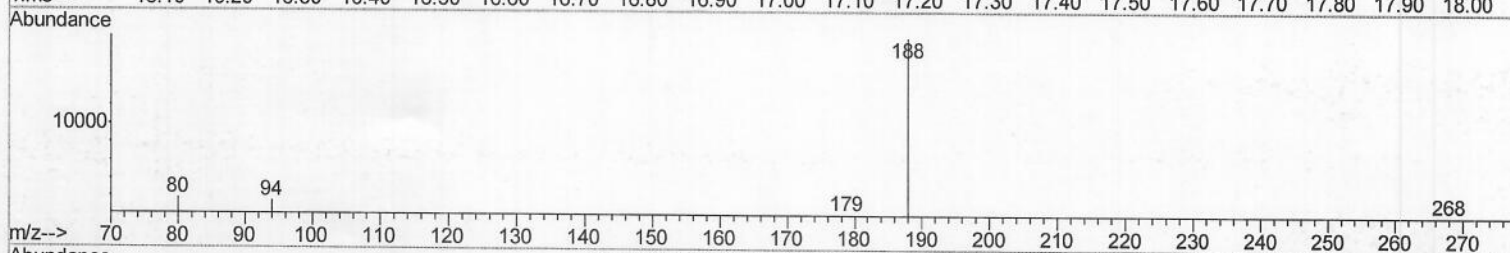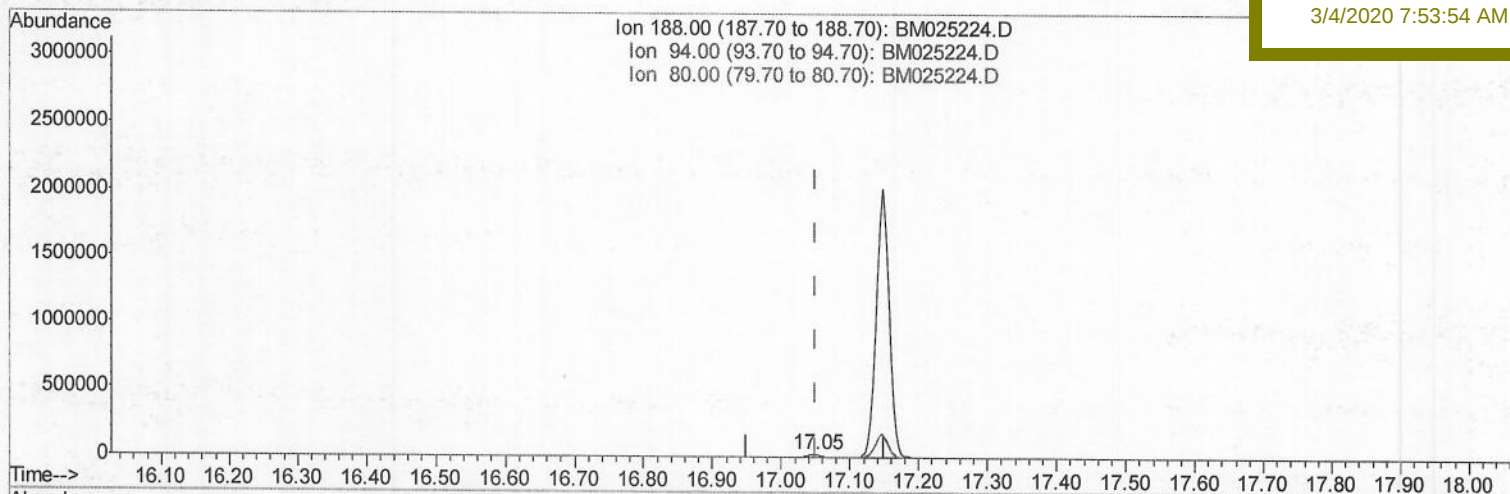

TIC: BM025224.D

(10) Phenanthrene-d10 (I)

17.050min (-0.000) 0.40ng/ul m

7 JU 03/05/20

response 26488

Ion	Exp%	Act%
188.00	100	100
94.00	26.60	7.65#
80.00	22.60	8.82#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM030320\
Quantitation Report (QT Reviewed)

Data File : BM025224.D
Acq On : 03 Mar 2020 22:26
Operator : CG/JU
Sample : L1542-13
Misc :
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Mar 04 01:11:20 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 04 00:52:51 2020
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
DBD49

Manual Integrations
APPROVED

mohammad
3/4/2020 7:53:54 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.68	152	3593	0.40	ng/ul	0.00
2) Naphthalene-d8	10.45	136	15417	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.31	164	11397	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.05	188	26488m	0.40	ng/ul	0.00
16) Chrysene-d12	21.23	240	25387	0.40	ng/ul	0.00
20) Perylene-d12	23.43	264	23539	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.04	152	12640	0.44	ng/ul	0.00
14) Fluoranthene-d10	19.08	212	35991	0.42	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

> JU 03/05/20