




Data File : BM025225.D
Acq On : 03 Mar 2020 23:02
Operator : CG/JU
Sample : L1542-21
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBD55

Manual Integrations
APPROVED

mohammad
3/4/2020 7:53:17 AM

Quant Time: Mar 04 00:55:19 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 04 00:52:51 2020
Response via : Initial Calibration

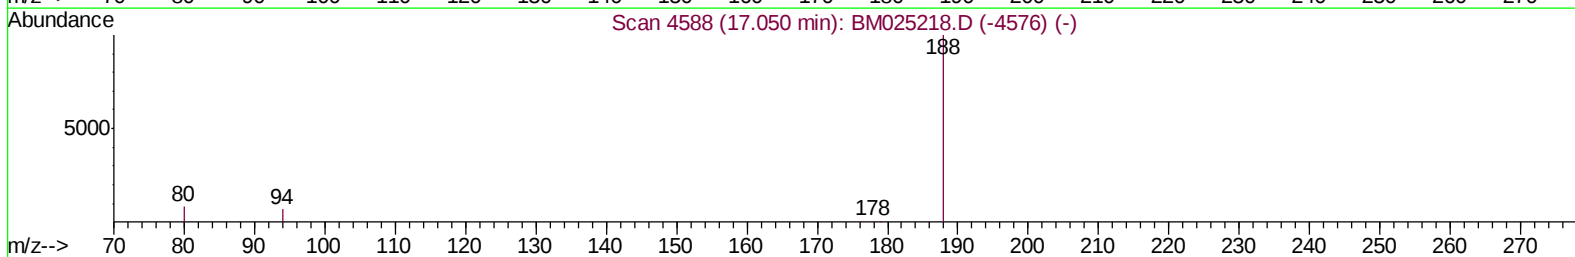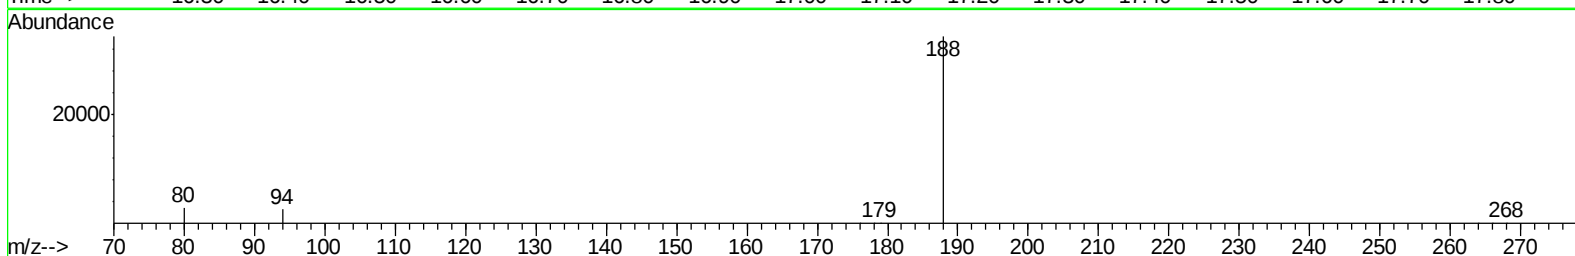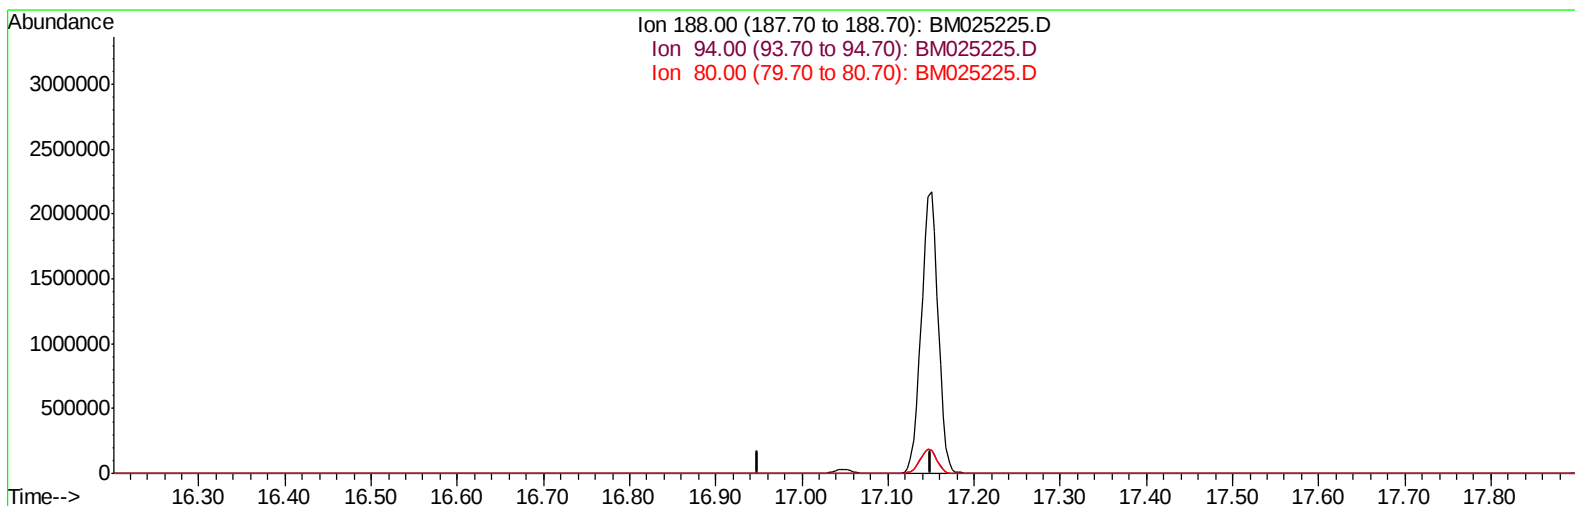

TIC: BM025225.D

(10) Phenanthrene-d10 (I)

17.050min (-17.050) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	26.60	0.00#
80.00	22.60	0.00#
0.00	0.00	0.00




Data File : BM025225.D
Acq On : 03 Mar 2020 23:02
Operator : CG/JU
Sample : L1542-21
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBD55

Manual Integrations
APPROVED

mohammad
3/4/2020 7:53:17 AM

Quant Time: Mar 04 00:55:19 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 04 00:52:51 2020
Response via : Initial Calibration

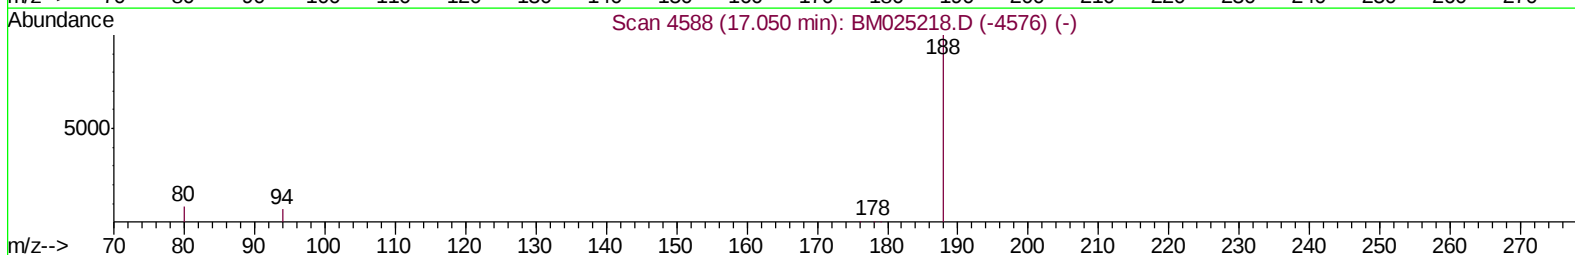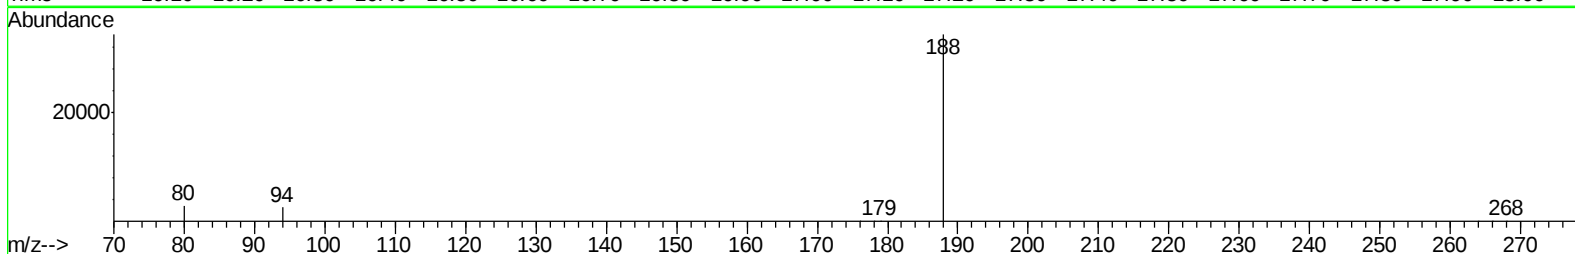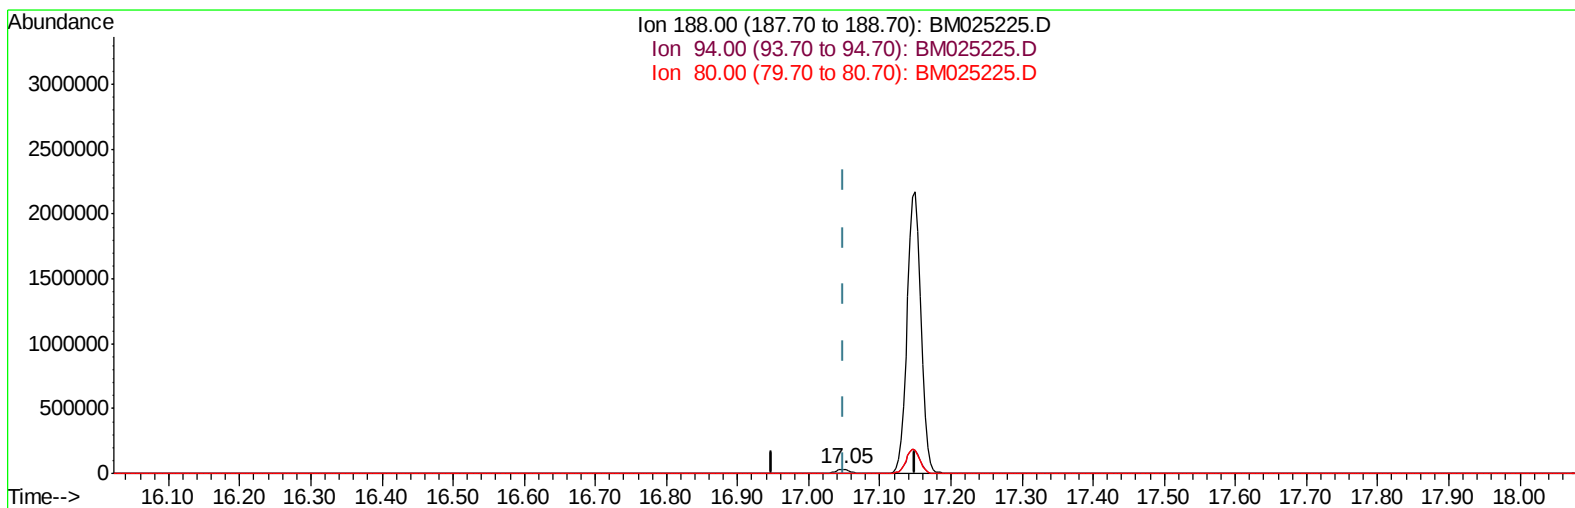

TIC: BM025225.D

(10) Phenanthrene-d10 (I)

17.049min (-0.000) 0.40ng/ul m

response 45411

Ion	Exp%	Act%
188.00	100	100
94.00	26.60	7.44#
80.00	22.60	8.54#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM030320\
Quantitation Report (QT Reviewed)

Data File : BM025225.D
Acq On : 03 Mar 2020 23:02
Operator : CG/JU
Sample : L1542-21
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBD55

Manual Integrations
APPROVED

mohammad
3/4/2020 7:53:17 AM

Quant Time: Mar 04 01:13:28 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 04 00:52:51 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.68	152	5778	0.40	ng/ul	0.00
2) Naphthalene-d8	10.45	136	25648	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.31	164	18905	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.05	188	45411m	0.40	ng/ul	0.00
16) Chrysene-d12	21.23	240	45685	0.40	ng/ul	0.00
20) Perylene-d12	23.43	264	44668	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.04	152	13375	0.28	ng/ul	0.00
14) Fluoranthene-d10	19.08	212	40227	0.27	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BM025225.D
Acq On : 03 Mar 2020 23:02
Operator : CG/JU
Sample : L1542-21
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBD55

Manual Integrations
APPROVED

mohammad
3/4/2020 7:53:17 AM

Quant Time: Mar 04 01:13:28 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 04 00:52:51 2020
Response via : Initial Calibration

