




Data File : BM025228.D
Acq On : 04 Mar 2020 00:51
Operator : CG/JU
Sample : L1542-11
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBD47

Manual Integrations
APPROVED

mohammad
3/4/2020 7:54:00 AM

Quant Time: Mar 04 04:07:59 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 04 00:52:51 2020
Response via : Initial Calibration

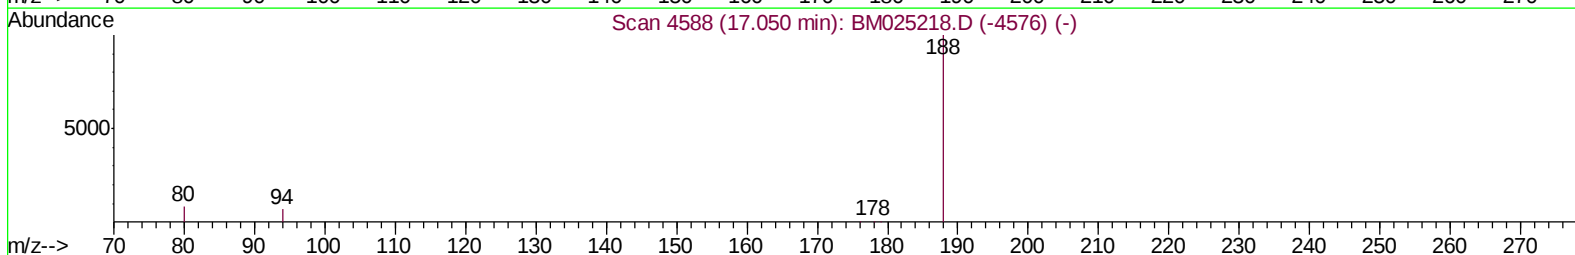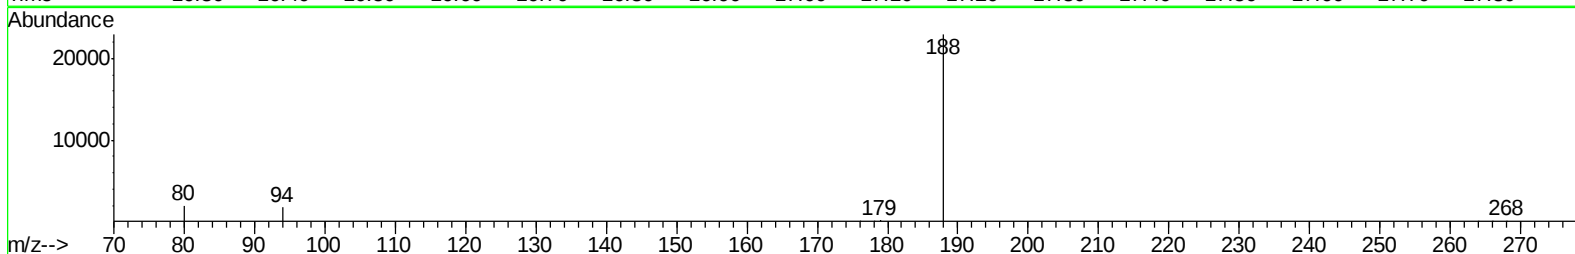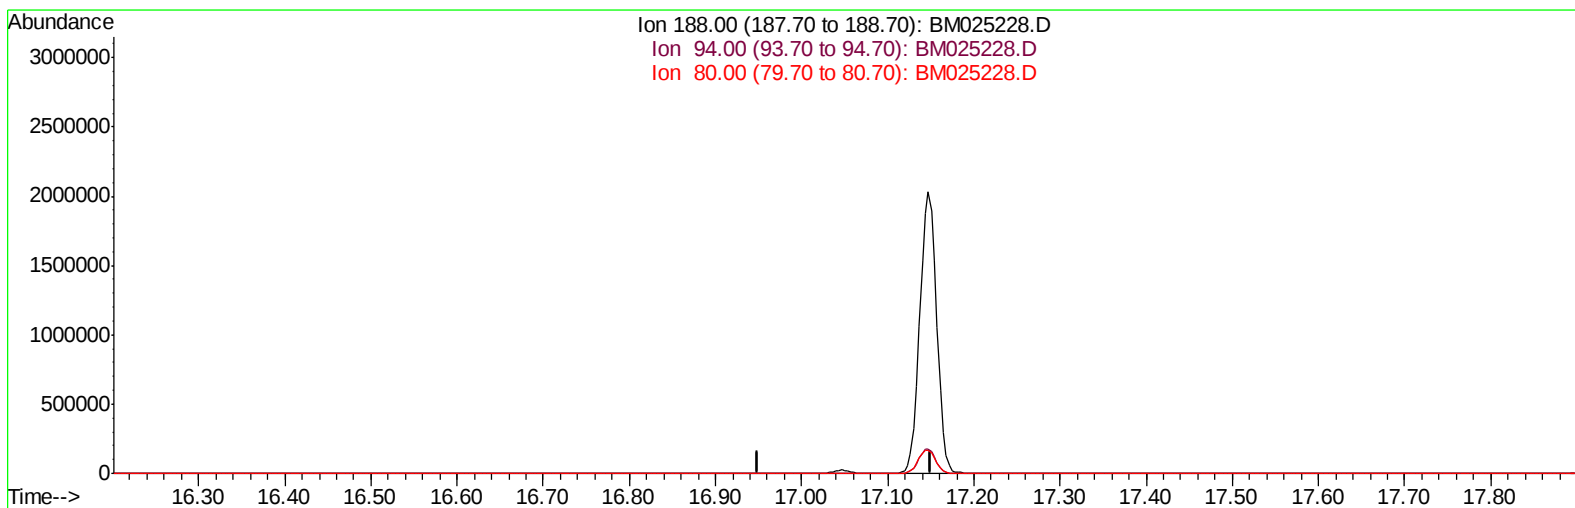

TIC: BM025228.D

(10) Phenanthrene-d10 (I)

17.050min (-17.050) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	26.60	0.00#
80.00	22.60	0.00#
0.00	0.00	0.00




Data File : BM025228.D
Acq On : 04 Mar 2020 00:51
Operator : CG/JU
Sample : L1542-11
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBD47

Manual Integrations
APPROVED

mohammad
3/4/2020 7:54:00 AM

Quant Time: Mar 04 04:07:59 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 04 00:52:51 2020
Response via : Initial Calibration

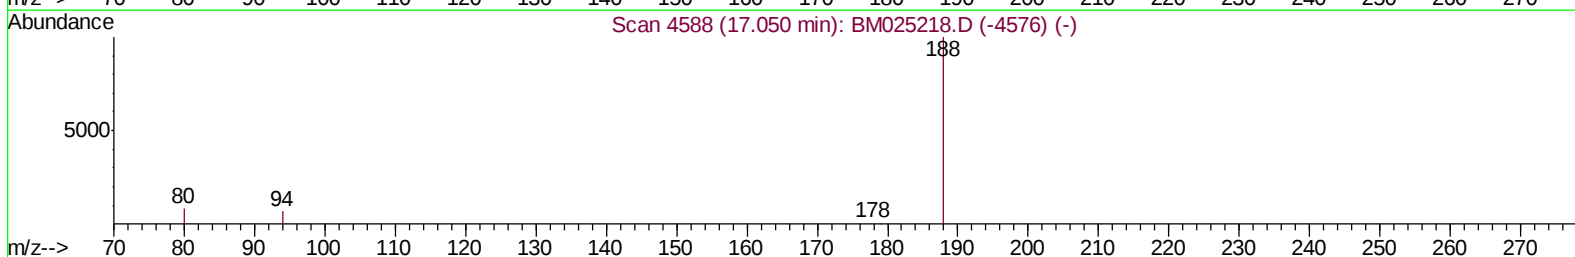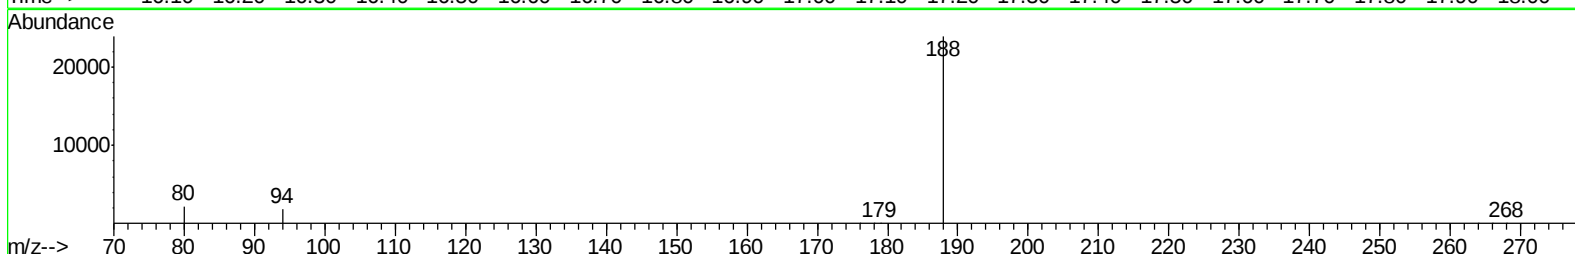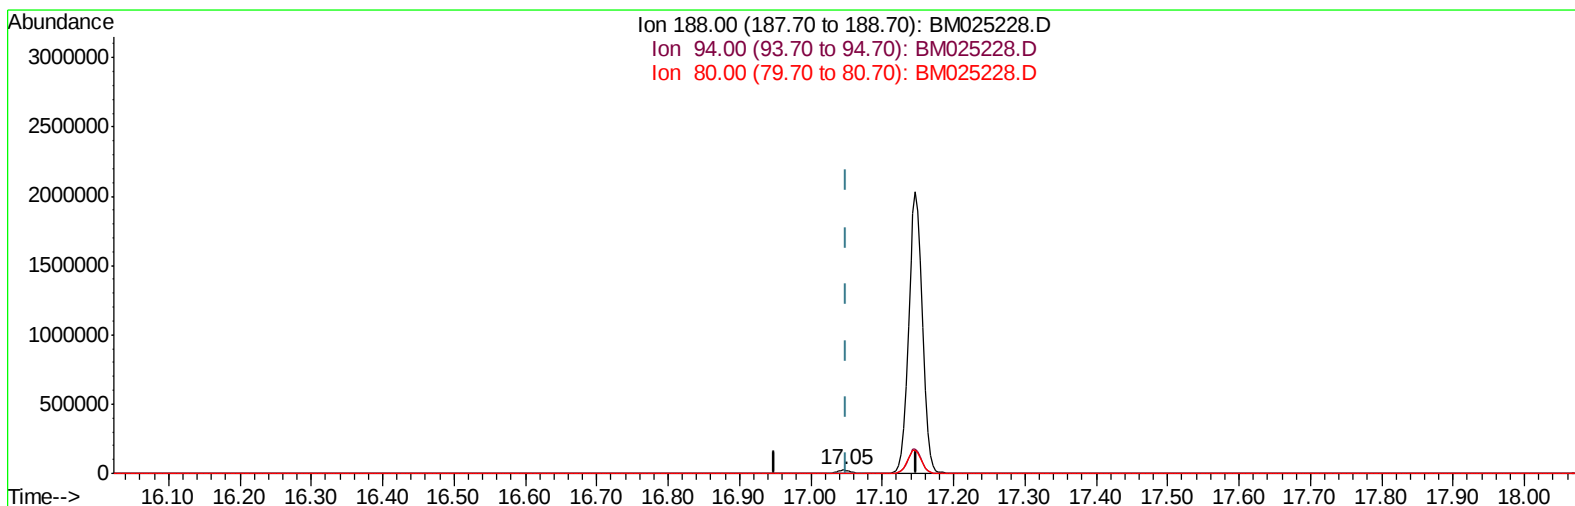

TIC: BM025228.D

(10) Phenanthrene-d10 (I)

17.046min (-0.003) 0.40ng/ul m

response 32368

Ion	Exp%	Act%
188.00	100	100
94.00	26.60	7.99#
80.00	22.60	9.16#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM030320\
Quantitation Report (QT Reviewed)

Data File : BM025228.D
Acq On : 04 Mar 2020 00:51
Operator : CG/JU
Sample : L1542-11
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBD47

Manual Integrations
APPROVED

mohammad
3/4/2020 7:54:00 AM

Quant Time: Mar 04 04:14:29 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 04 00:52:51 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.68	152	4319	0.40	ng/ul	0.00
2) Naphthalene-d8	10.44	136	18476	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.31	164	13774	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.05	188	32368m	0.40	ng/ul	0.00
16) Chrysene-d12	21.23	240	30918	0.40	ng/ul	0.00
20) Perylene-d12	23.42	264	29646	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.04	152	12686	0.37	ng/ul	0.00
14) Fluoranthene-d10	19.08	212	36532	0.35	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BM025228.D
Acq On : 04 Mar 2020 00:51
Operator : CG/JU
Sample : L1542-11
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBD47

Manual Integrations
APPROVED

mohammad
3/4/2020 7:54:00 AM

Quant Time: Mar 04 04:14:29 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 04 00:52:51 2020
Response via : Initial Calibration

