




Data File : BM025231.D
Acq On : 04 Mar 2020 02:39
Operator : CG/JU
Sample : L1542-22
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBD56

Manual Integrations
APPROVED

mohammad
3/4/2020 7:54:09 AM

Quant Time: Mar 04 04:08:20 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 04 00:52:51 2020
Response via : Initial Calibration

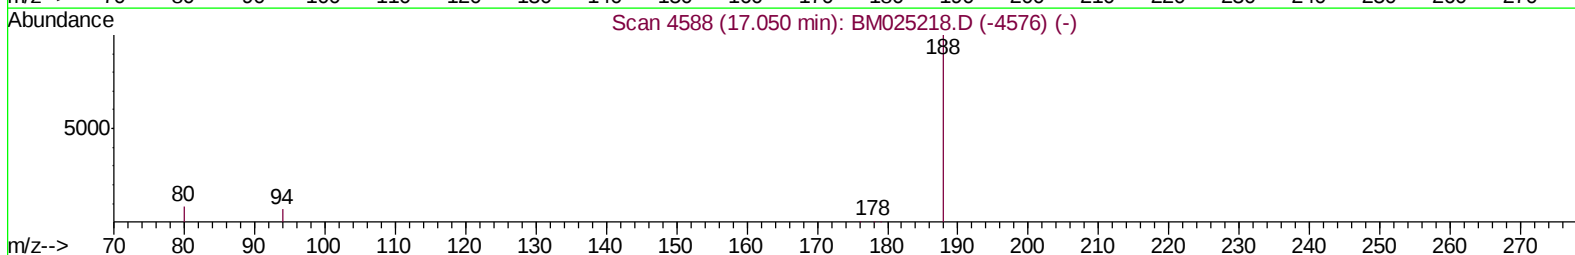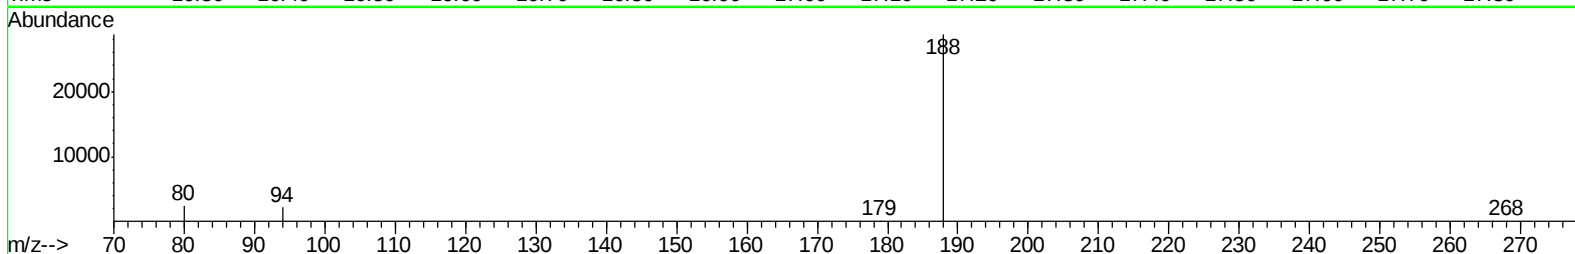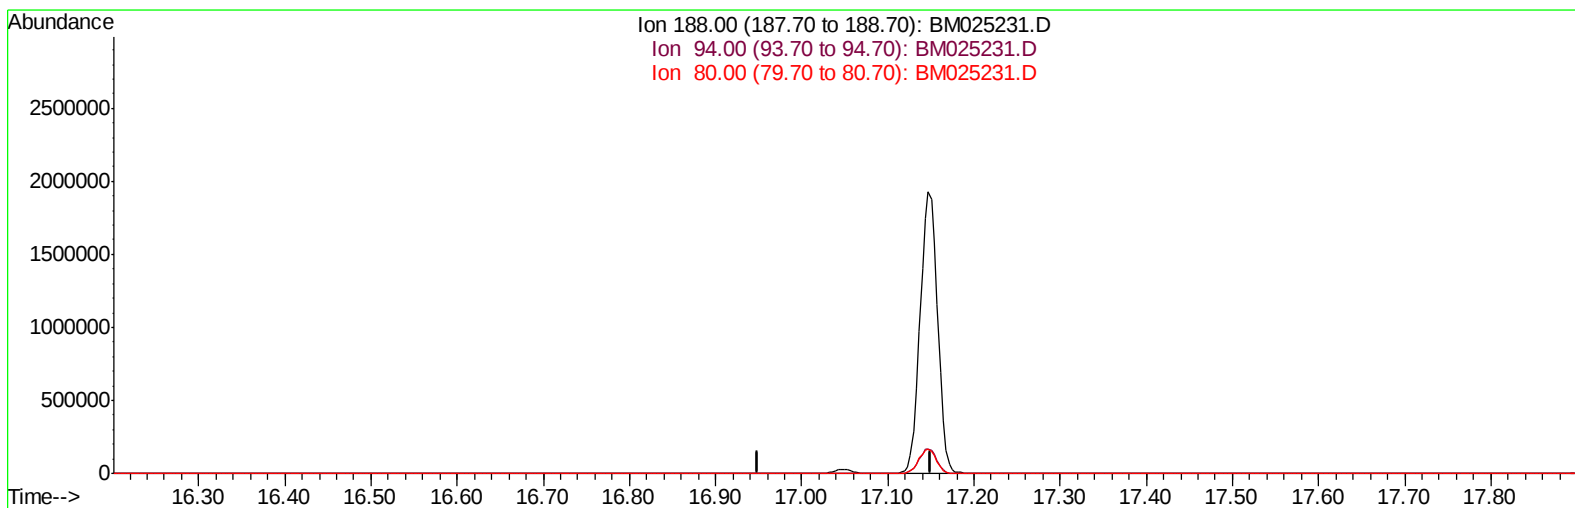

TIC: BM025231.D

(10) Phenanthrene-d10 (I)

17.050min (-17.050) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	26.60	0.00#
80.00	22.60	0.00#
0.00	0.00	0.00




Data File : BM025231.D
Acq On : 04 Mar 2020 02:39
Operator : CG/JU
Sample : L1542-22
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBD56

Manual Integrations
APPROVED

mohammad
3/4/2020 7:54:09 AM

Quant Time: Mar 04 04:08:20 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 04 00:52:51 2020
Response via : Initial Calibration

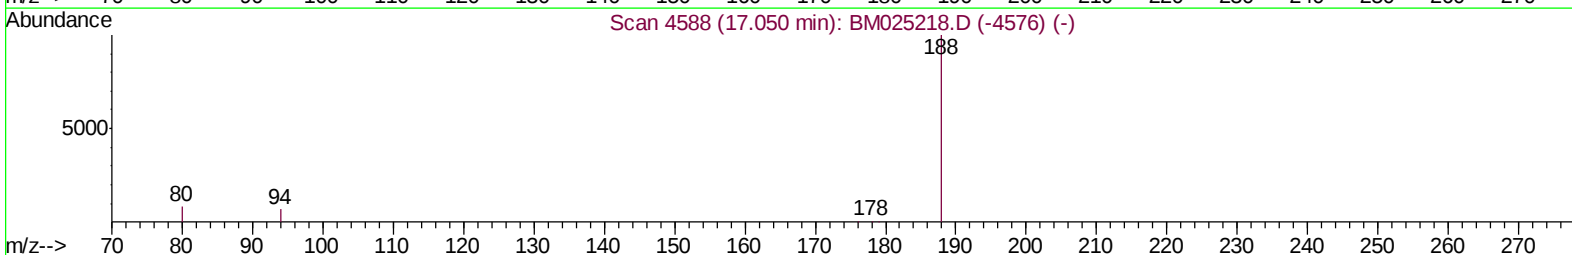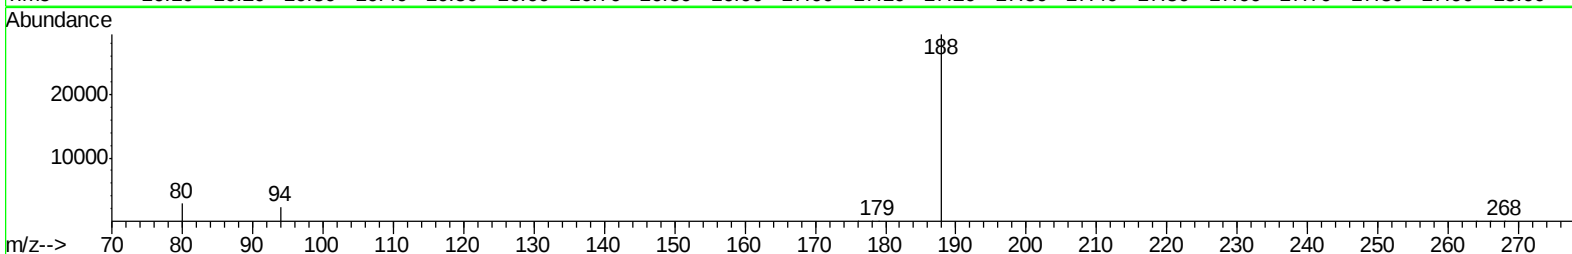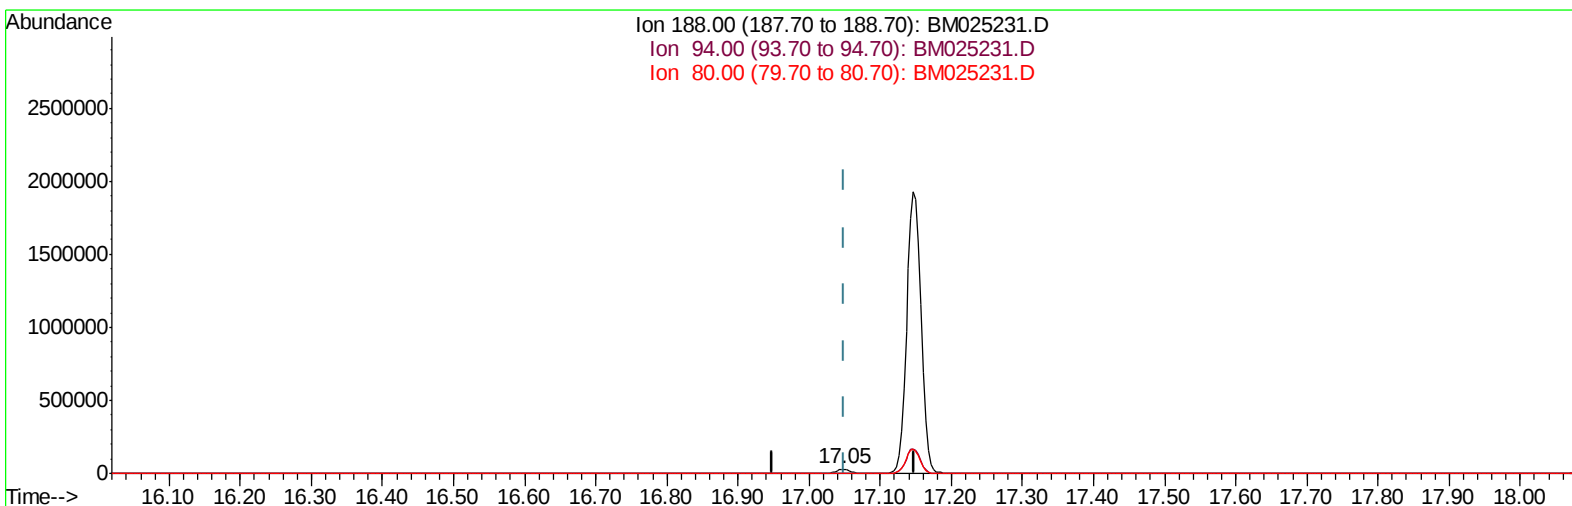

TIC: BM025231.D

(10) Phenanthrene-d10 (I)

17.046min (-0.004) 0.40ng/ul m

response 40087

Ion	Exp%	Act%
188.00	100	100
94.00	26.60	7.91#
80.00	22.60	9.44#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM030320\
Quantitation Report (QT Reviewed)

Data File : BM025231.D
Acq On : 04 Mar 2020 02:39
Operator : CG/JU
Sample : L1542-22
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBD56

Manual Integrations
APPROVED

mohammad
3/4/2020 7:54:09 AM

Quant Time: Mar 04 04:26:01 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 04 00:52:51 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.68	152	5225	0.40	ng/ul	0.00
2) Naphthalene-d8	10.45	136	22618	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.31	164	16819	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.05	188	40087m	0.40	ng/ul	0.00
16) Chrysene-d12	21.23	240	38808	0.40	ng/ul	0.00
20) Perylene-d12	23.42	264	37076	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.04	152	12481	0.29	ng/ul	0.00
14) Fluoranthene-d10	19.08	212	36193	0.28	ng/ul	0.00
Target Compounds						
12) Phenanthrene	17.09	178	2985	0.023	ng/ul	Qvalue 98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BM025231.D
Acq On : 04 Mar 2020 02:39
Operator : CG/JU
Sample : L1542-22
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBD56

Manual Integrations
APPROVED

mohammad
3/4/2020 7:54:09 AM

Quant Time: Mar 04 04:26:01 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 04 00:52:51 2020
Response via : Initial Calibration

