

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM030320\

Data File : BM025239.D

Acq On : 04 Mar 2020 08:04

Operator : CG/JU

Sample : L1516-13

Misc :

ALS Vial : 35 Sample Multiplier: 1

Quant Time: Mar 04 11:33:36 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Wed Mar 04 08:02:03 2020

Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :

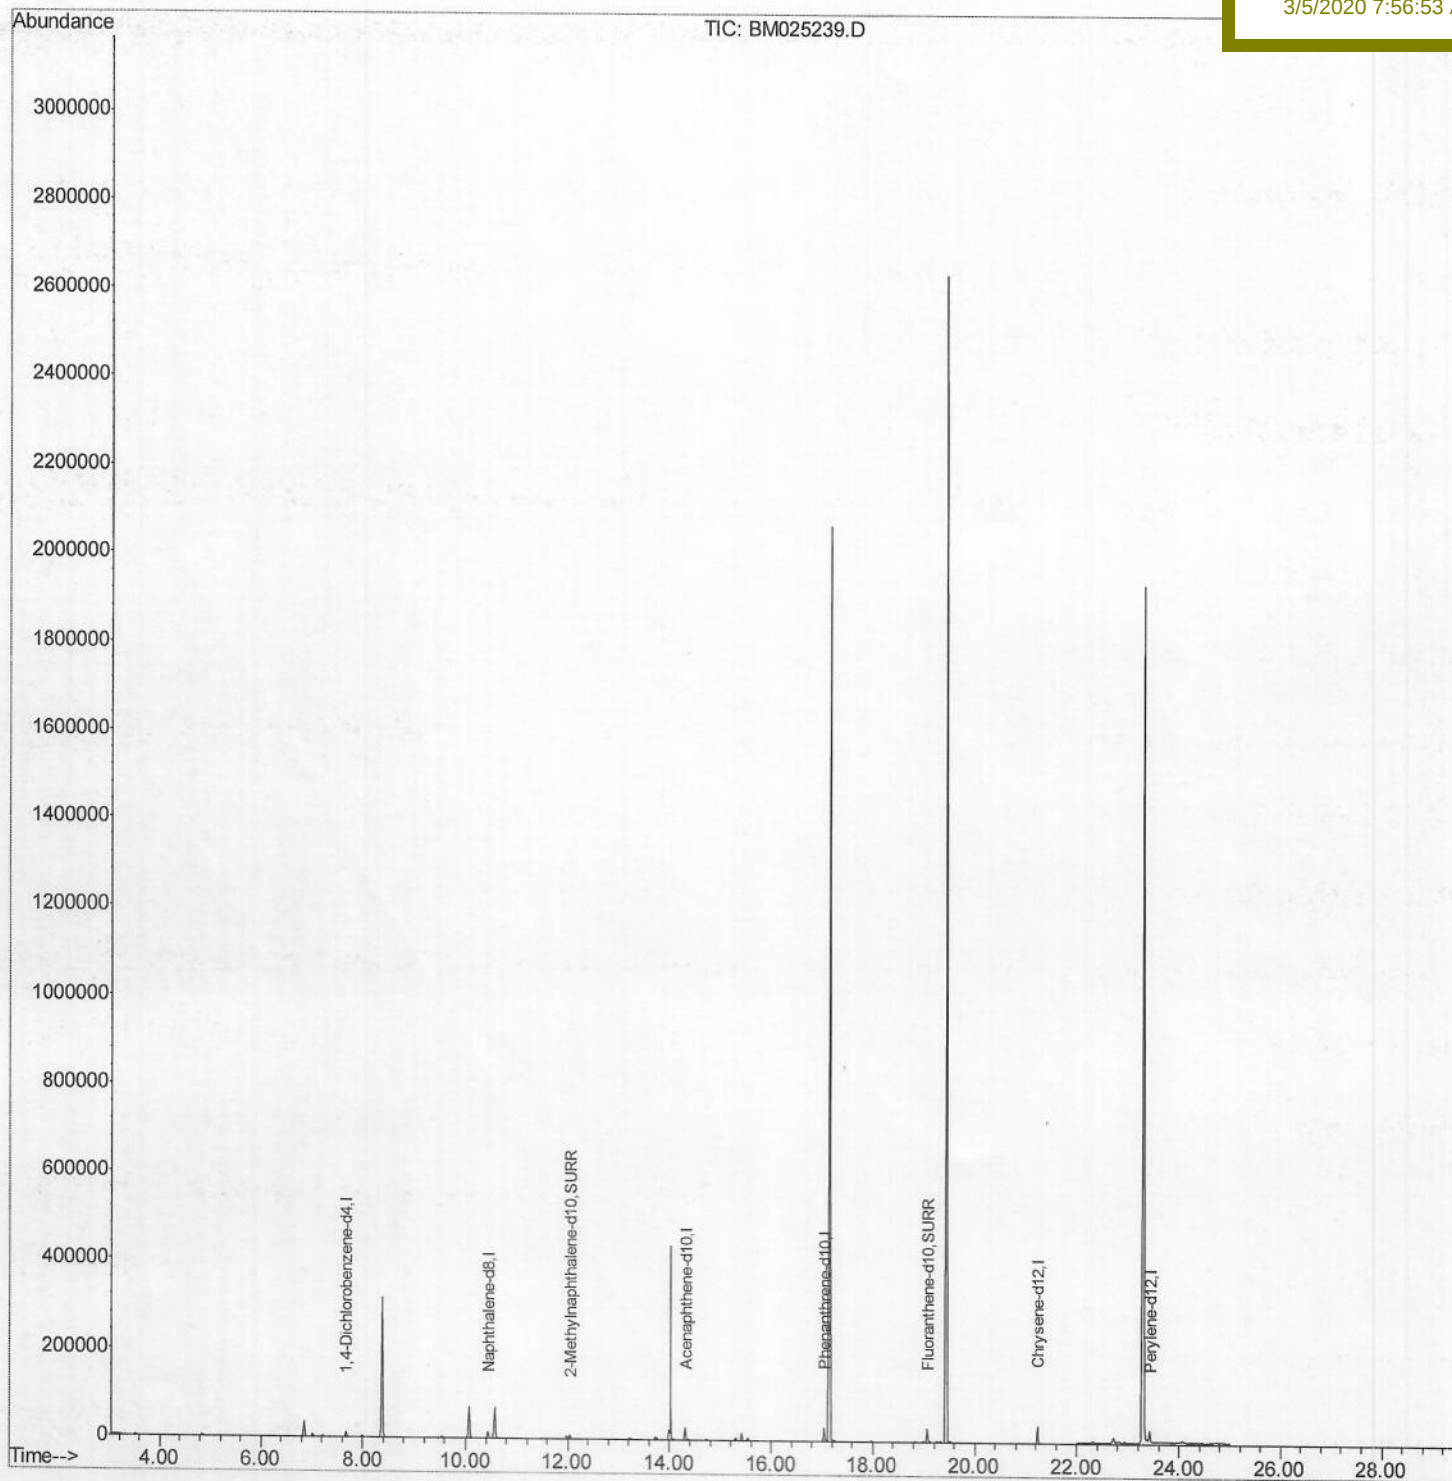
DBD31

Manual Integrations

APPROVED

mohammad

3/5/2020 7:56:53 AM



Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM030320\

Data File : BM025239.D

Acq On : 04 Mar 2020 08:04

Operator : CG/JU

Sample : L1516-13

Misc :

ALS Vial : 35 Sample Multiplier: 1

Quant Time: Mar 04 11:31:51 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Wed Mar 04 08:02:03 2020

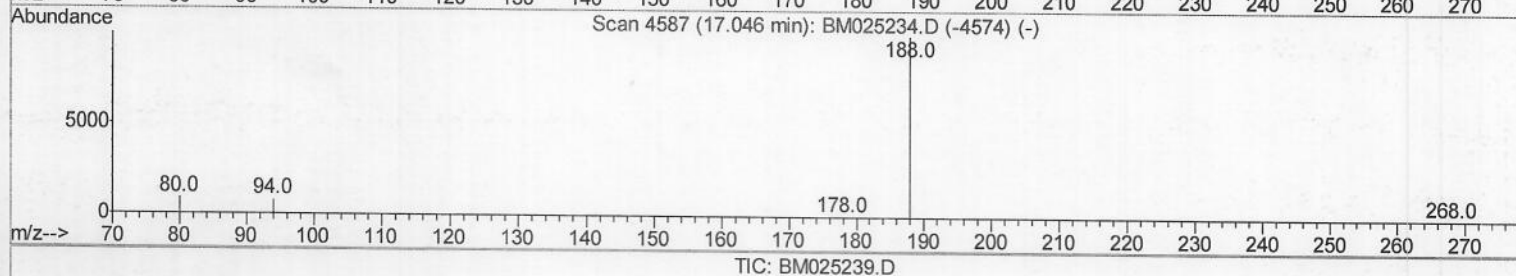
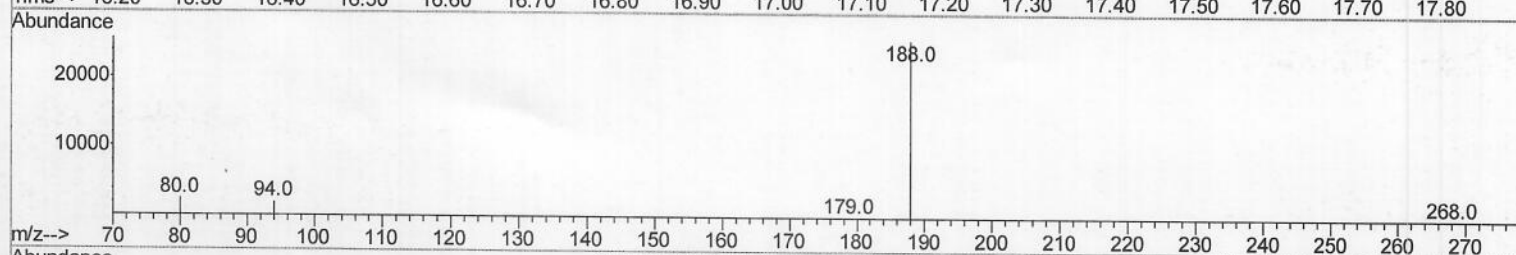
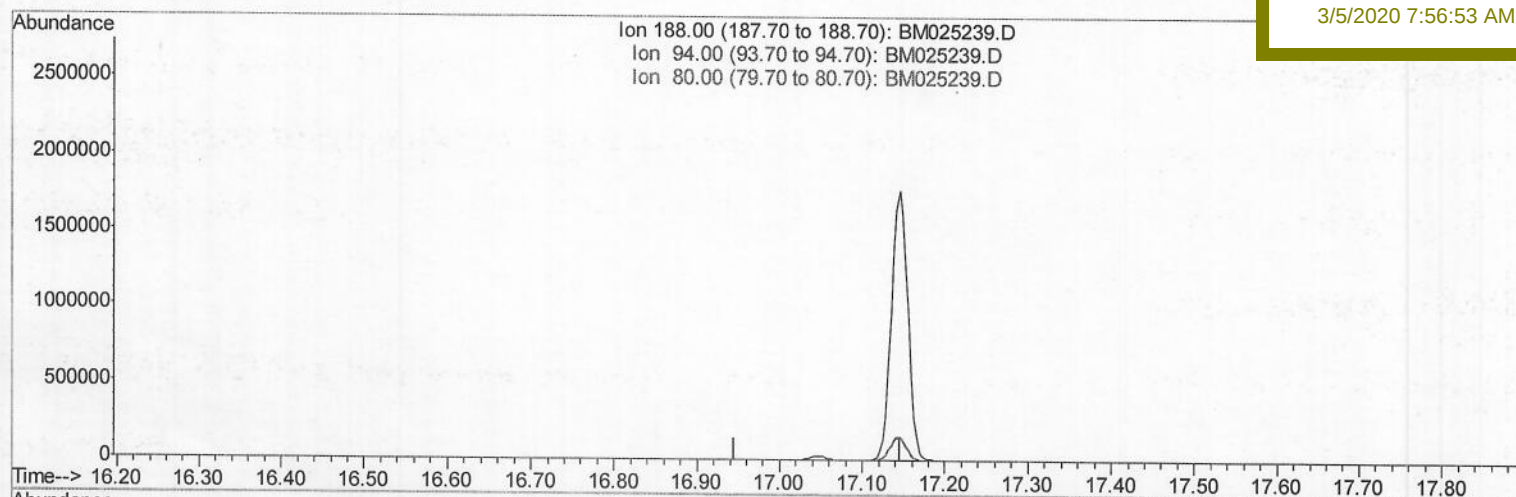
Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :

DBD31

Manual Integrations
APPROVEDmohammad
3/5/2020 7:56:53 AM

(10) Phenanthrene-d10 (I)

17.046min (-17.046) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	26.60	0.00#
80.00	22.60	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM030320\

Data File : BM025239.D

Acq On : 04 Mar 2020 08:04

Operator : CG/JU

Sample : L1516-13

Misc :

ALS Vial : 35 Sample Multiplier: 1

Quant Time: Mar 04 11:31:51 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Wed Mar 04 08:02:03 2020

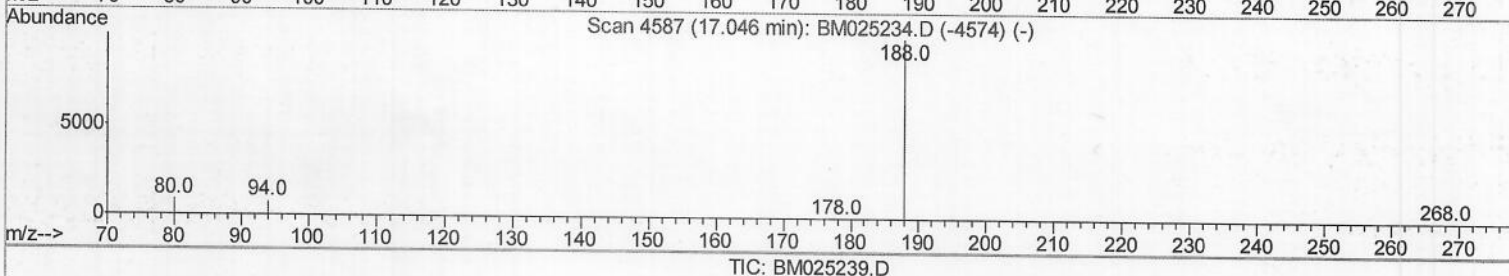
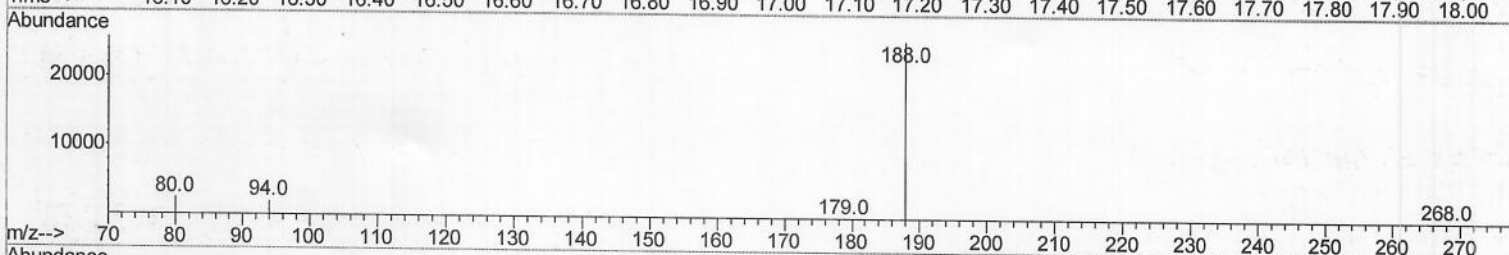
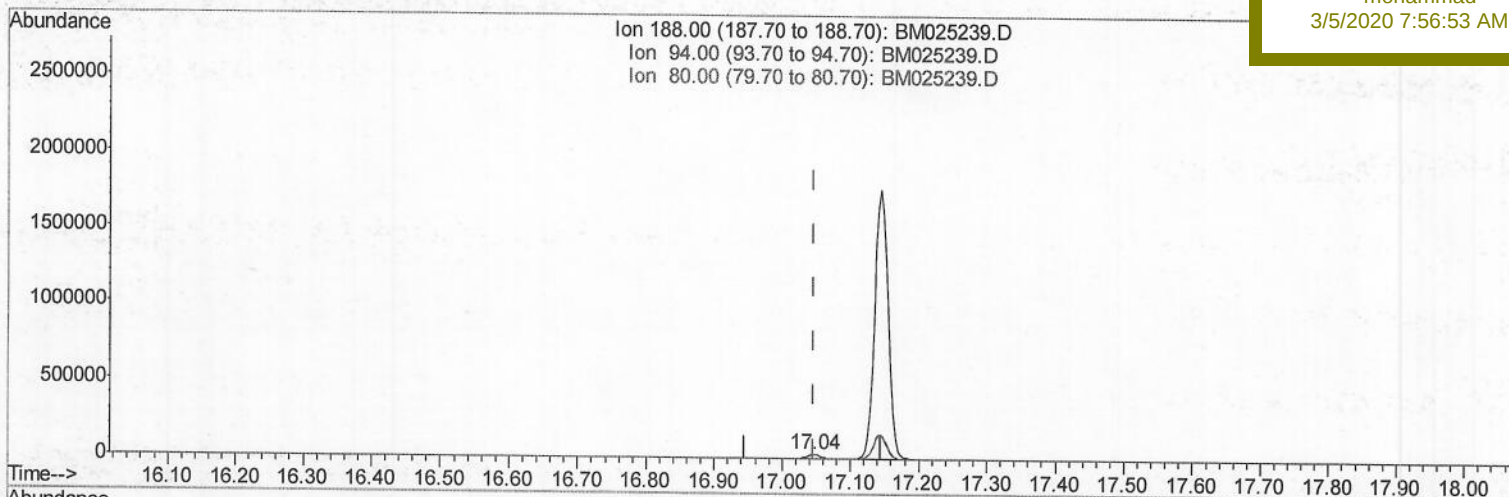
Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :

DBD31

Manual Integrations
APPROVEDmohammad
3/5/2020 7:56:53 AM

(10) Phenanthrene-d10 (l)

17.045min (-0.002) 0.40ng/ul m

CG JU 03/05/20

response 35754

Ion	Exp%	Act%
188.00	100	100
94.00	26.60	7.98#
80.00	22.60	9.63#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM030320\
Data File : BM025239.D
Acq On : 04 Mar 2020 08:04
Operator : CG/JU
Sample : L1516-13
Misc :
ALS Vial : 35 Sample Multiplier: 1

Quant Time: Mar 04 11:33:36 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 04 08:02:03 2020
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
DBD31

Manual Integrations
APPROVED

mohammad
3/5/2020 7:56:53 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.68	152	4471	0.40	ng/ul	0.00
2) Naphthalene-d8	10.45	136	19575	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.30	164	14929	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.04	188	35754m	0.40	ng/ul	0.00
16) Chrysene-d12	21.23	240	34738	0.40	ng/ul	0.00
20) Perylene-d12	23.42	264	32322	0.40	ng/ul	0.00

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	12.04	152	10788	0.29	ng/ul	0.00
14) Fluoranthene-d10	19.07	212	32411	0.28	ng/ul	0.00

Target Compounds	Ovalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

7 JU 03/20/20