


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM030320\
Data File : BM025240.D
Acq On : 04 Mar 2020 08:40
Operator : CG/JU
Sample : L1516-20
Misc :
ALS Vial : 36 Sample Multiplier: 1

Quant Time: Mar 04 11:34:57 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 04 08:02:03 2020
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
DBD78

Manual Integrations
APPROVED

mohammad
3/5/2020 7:56:37 AM

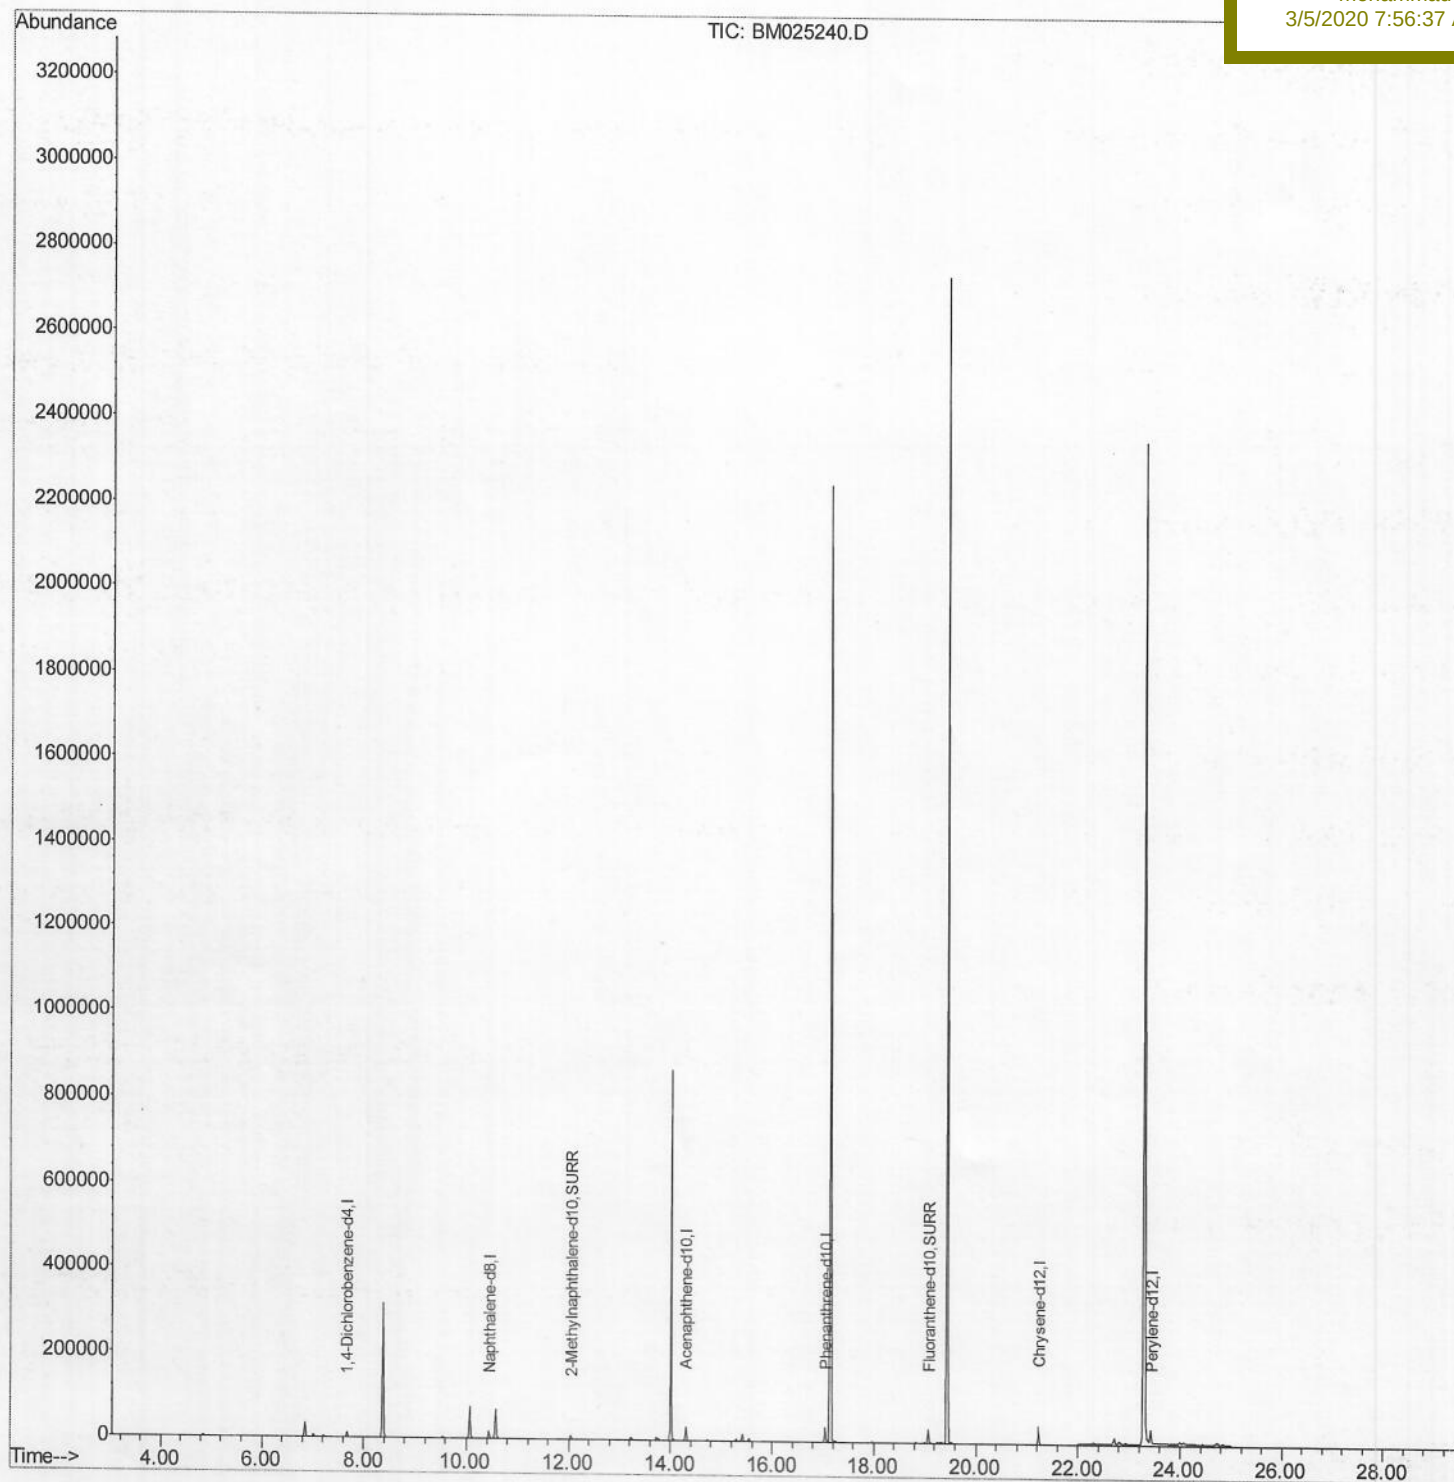

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM030320\

Data File : BM025240.D

Acq On : 04 Mar 2020 08:40

Operator : CG/JU

Sample : L1516-20

Misc :

ALS Vial : 36 Sample Multiplier: 1

Quant Time: Mar 04 11:34:11 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Wed Mar 04 08:02:03 2020

Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :




DBD78

Manual Integrations

APPROVED

mohammad

3/5/2020 7:56:37 AM

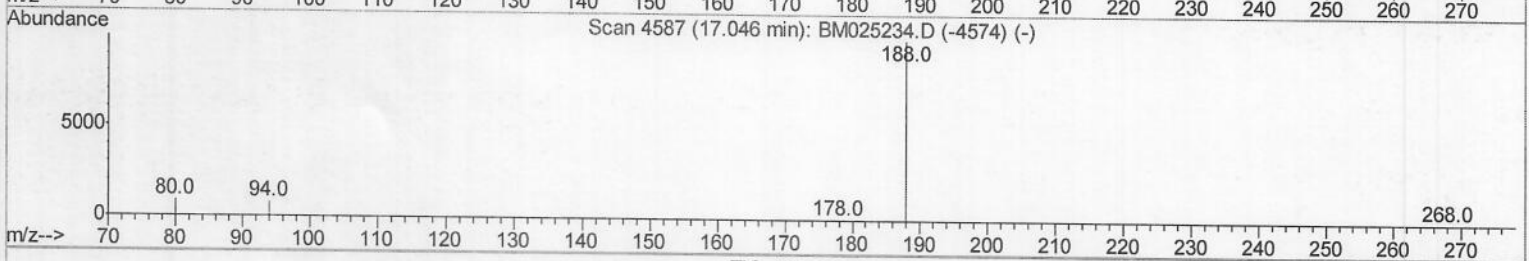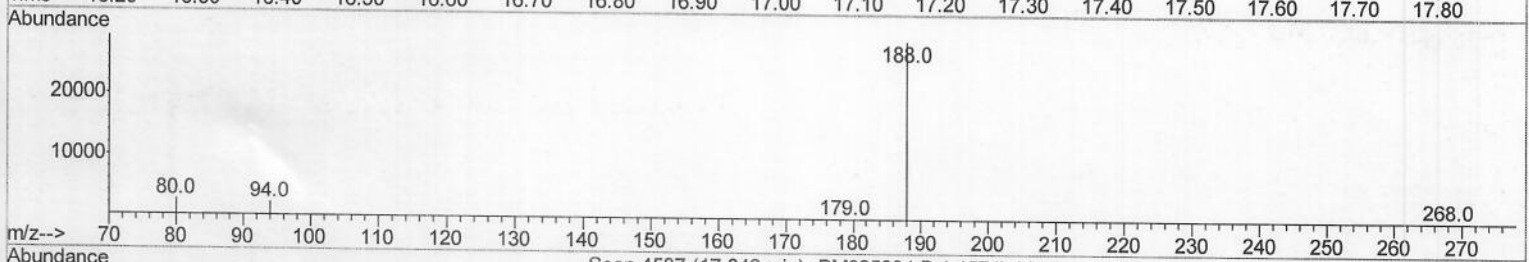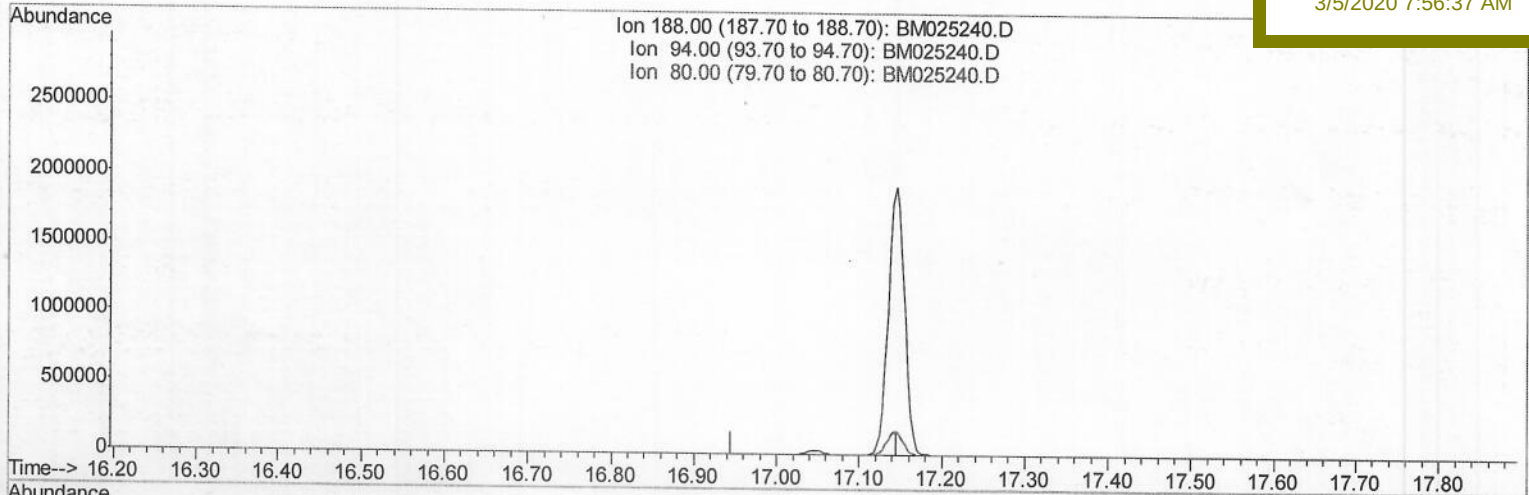

TIC: BM025240.D

(10) Phenanthrene-d10 (I)

17.046min (-17.046) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	26.60	0.00#
80.00	22.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM030320\

Data File : BM025240.D

Acq On : 04 Mar 2020 08:40

Operator : CG/JU

Sample : L1516-20

Misc :

ALS Vial : 36 Sample Multiplier: 1

Quant Time: Mar 04 11:34:11 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Wed Mar 04 08:02:03 2020

Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :




DBD78

Manual Integrations

APPROVED

mohammad

3/5/2020 7:56:37 AM

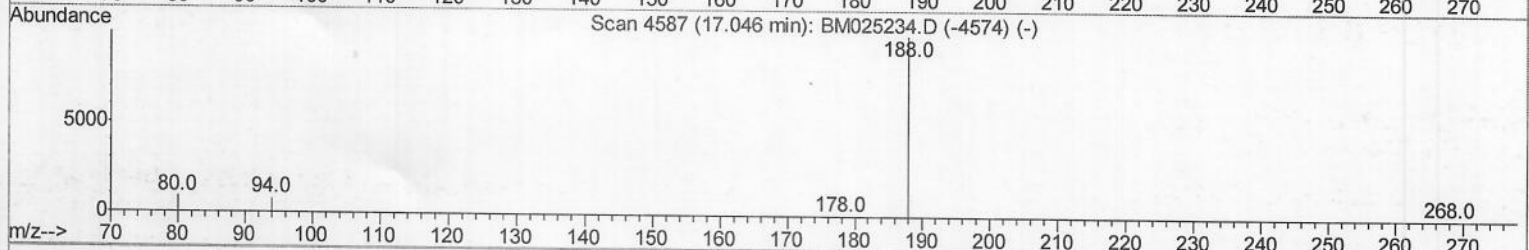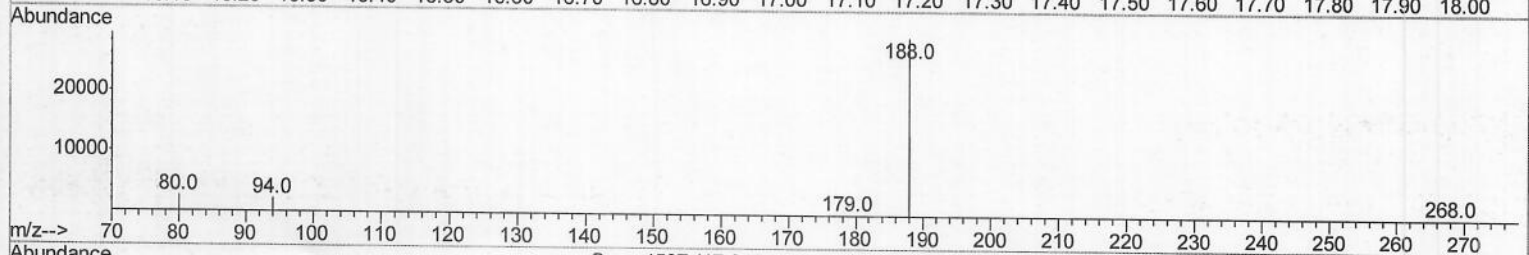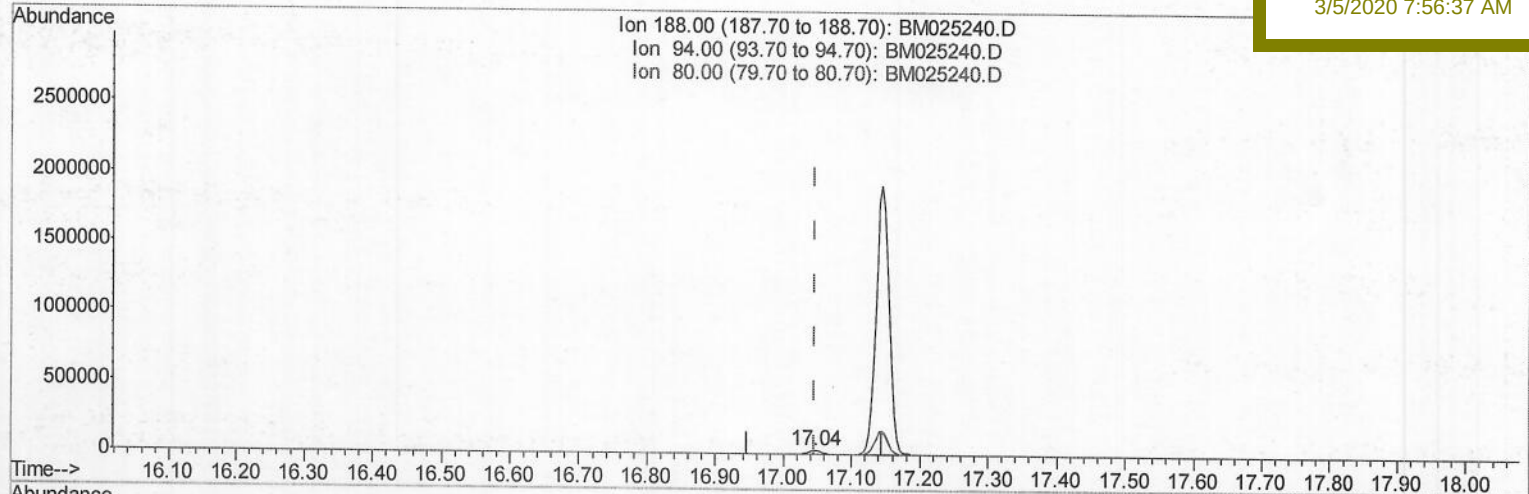

TIC: BM025240.D

(10) Phenanthrene-d10 (I)

17.045min (-0.002) 0.40ng/ul m

Handwritten signature: JU 03/05/20

response 39492

Ion	Exp%	Act%
188.00	100	100
94.00	26.60	7.70#
80.00	22.60	8.83#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM030320\
Data File : BM025240.D
Acq On : 04 Mar 2020 08:40
Operator : CG/JU
Sample : L1516-20
Misc :
ALS Vial : 36 Sample Multiplier: 1

Quant Time: Mar 04 11:34:57 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 04 08:02:03 2020
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
DBD78

Manual Integrations
APPROVED

mohammad
3/5/2020 7:56:37 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.68	152	5026	0.40	ng/ul	0.00
2) Naphthalene-d8	10.45	136	21953	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.30	164	16337	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.04	188	39492m	0.40	ng/ul	0.00
16) Chrysene-d12	21.23	240	39092	0.40	ng/ul	0.00
20) Perylene-d12	23.42	264	39704	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.04	152	11729	0.29	ng/ul	0.00
14) Fluoranthene-d10	19.07	212	34963	0.27	ng/ul	0.00

Target Compounds

Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

25003/25/20