

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM030320\

Data File : BM025247.D

Acq On : 04 Mar 2020 13:00

Operator : CG/JU

Sample : L1542-14

Misc :

ALS Vial : 43 Sample Multiplier: 1

Quant Time: Mar 04 13:44:40 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Wed Mar 04 08:02:03 2020

Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :


DBD50

Manual Integrations

APPROVED

mohammad

3/5/2020 7:57:07 AM

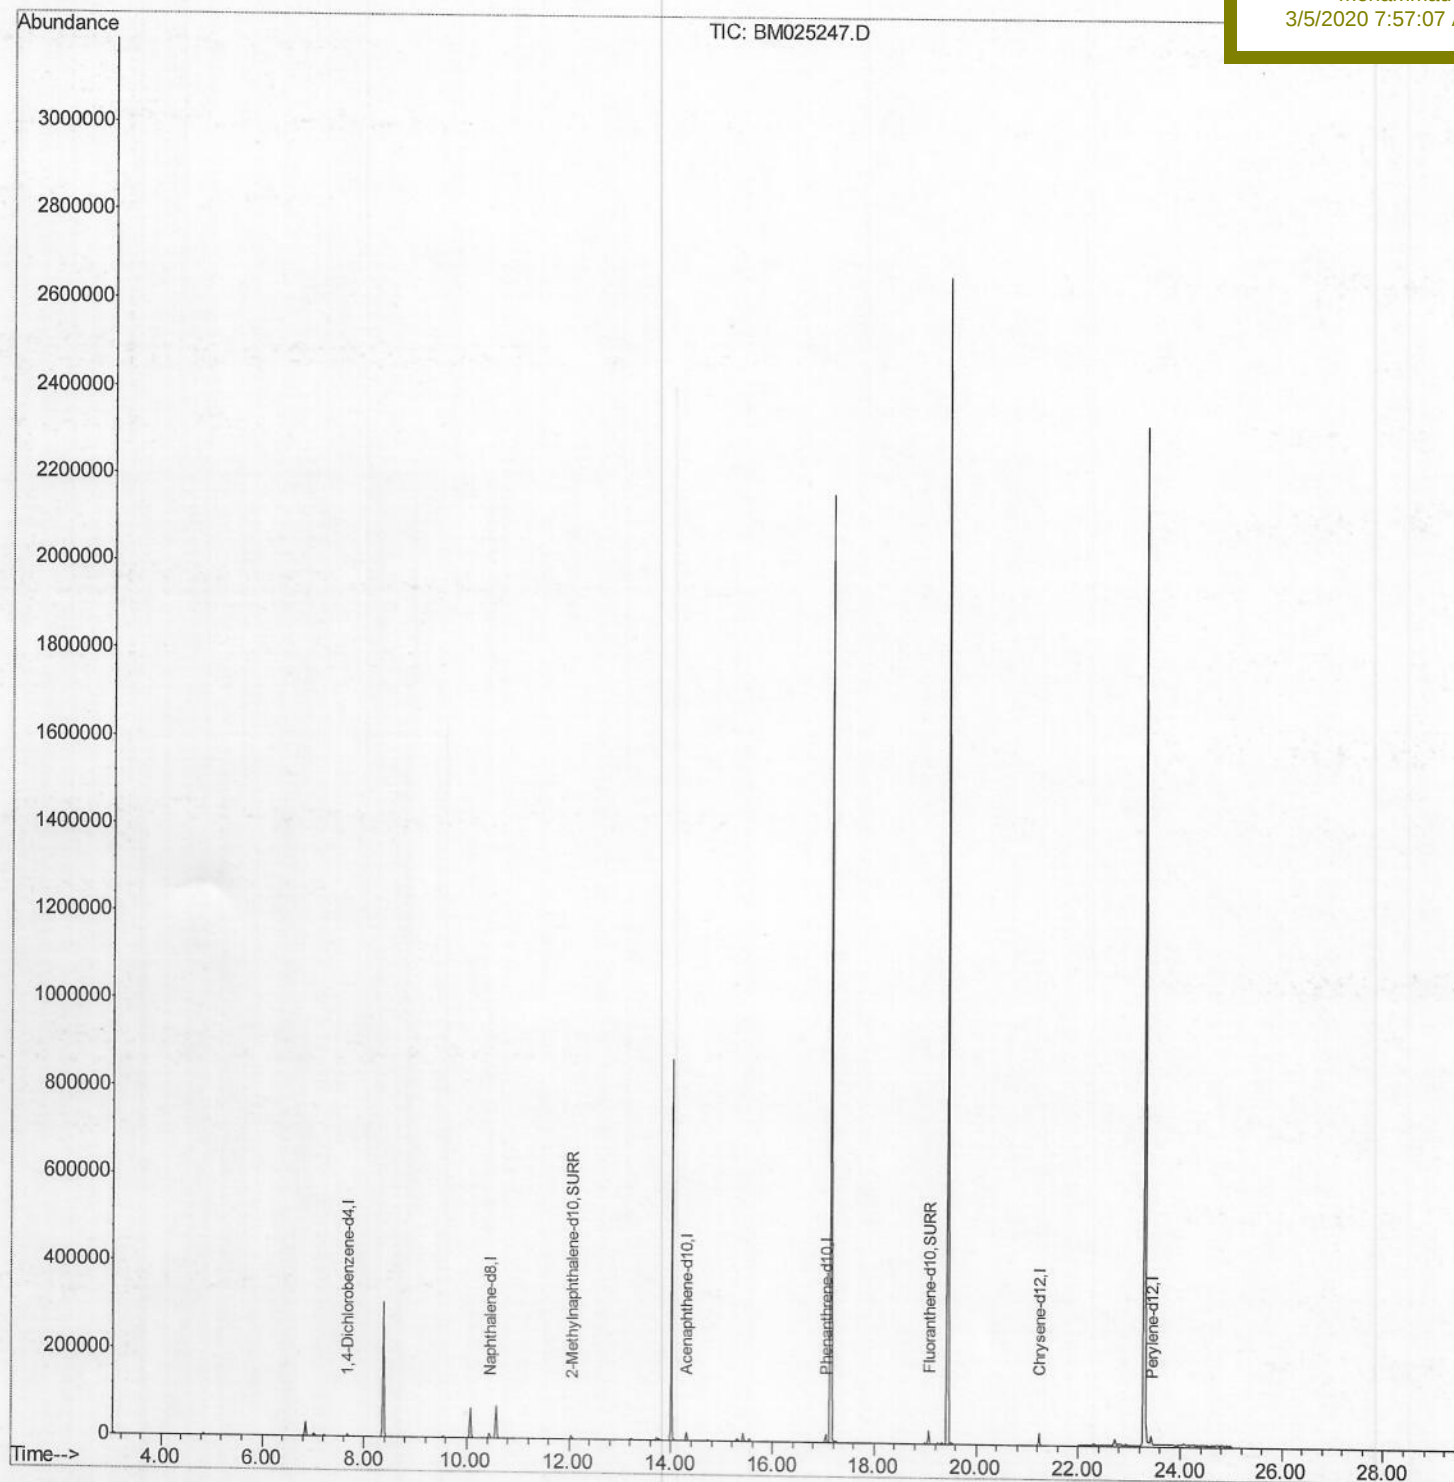

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM030320\

Data File : BM025247.D

Acq On : 04 Mar 2020 13:00

Operator : CG/JU

Sample : L1542-14

Misc :

ALS Vial : 43 Sample Multiplier: 1

Quant Time: Mar 04 13:43:40 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Wed Mar 04 08:02:03 2020

Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :




DBD50

Manual Integrations

APPROVED

mohammad

3/5/2020 7:57:07 AM

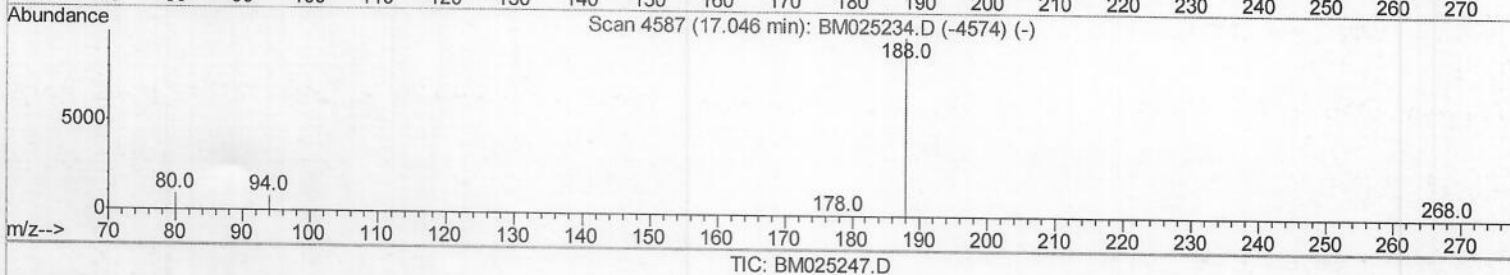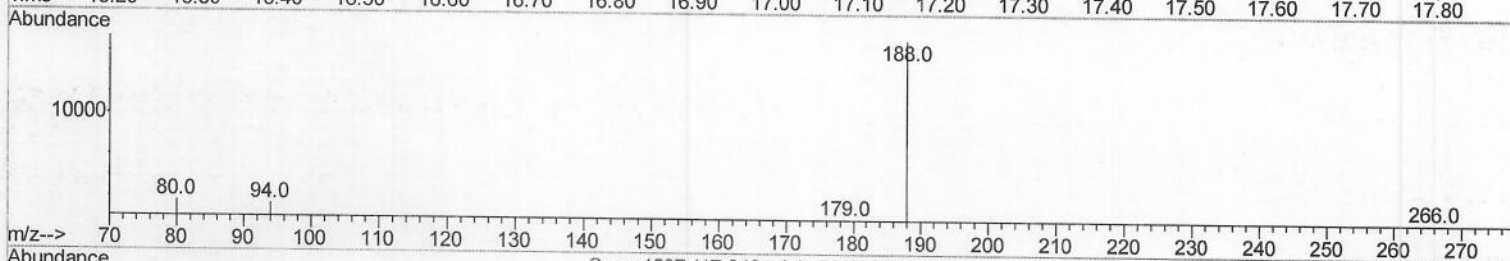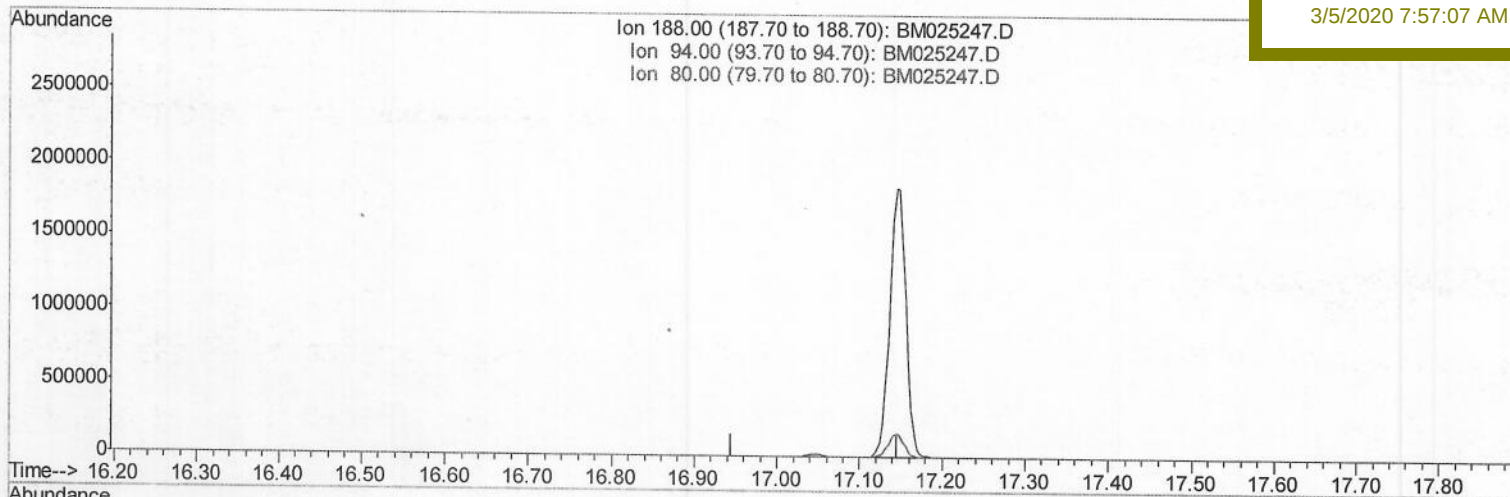

(10) Phenanthrene-d10 (I)

17.046min (-17.046) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	26.60	0.00#
80.00	22.60	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM030320\

Data File : BM025247.D

Acq On : 04 Mar 2020 13:00

Operator : CG/JU

Sample : L1542-14

Misc :

ALS Vial : 43 Sample Multiplier: 1

Quant Time: Mar 04 13:43:40 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Wed Mar 04 08:02:03 2020




Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :

DBD50

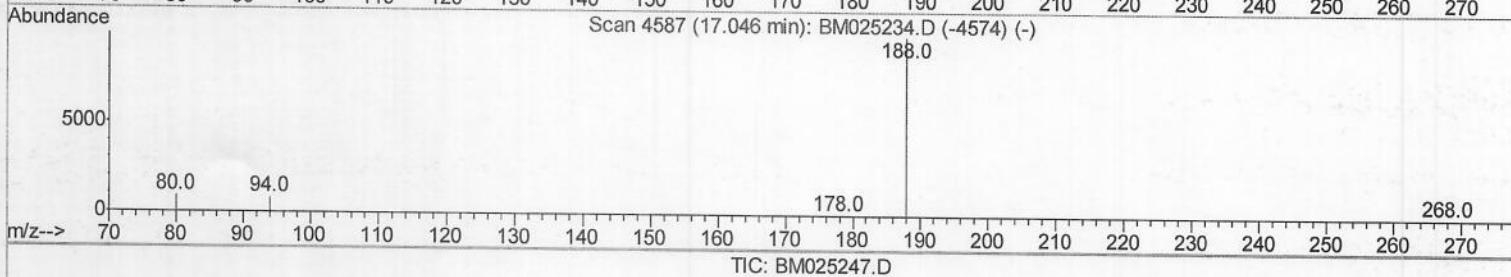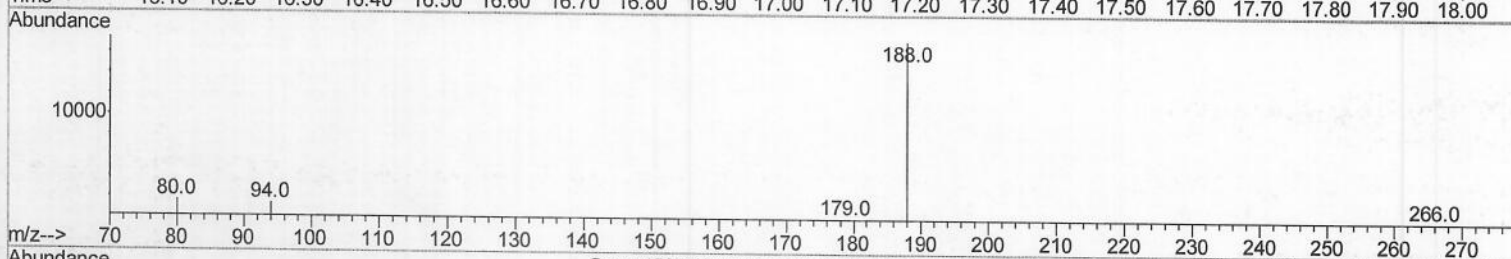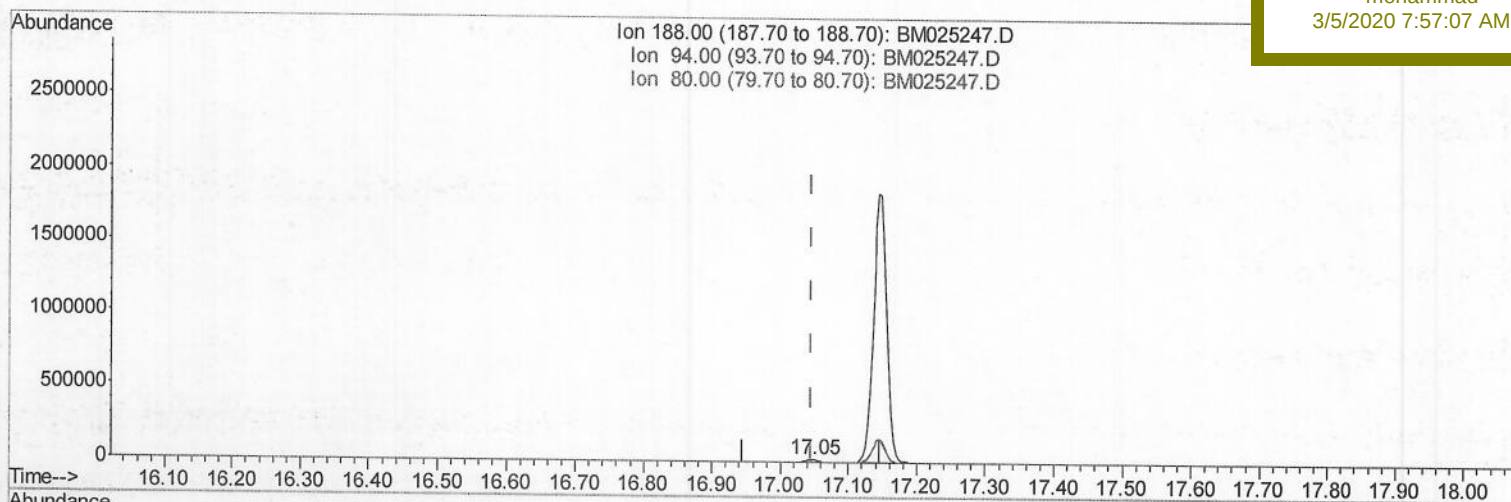Manual Integrations
APPROVEDmohammad
3/5/2020 7:57:07 AM

(10) Phenanthrene-d10 (I)

17.048min (+0.002) 0.40ng/ul m

70 09/05/20

response 24087

Ion	Exp%	Act%
188.00	100	100
94.00	26.60	7.78#
80.00	22.60	8.88#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM030320\
Data File : BM025247.D
Acq On : 04 Mar 2020 13:00
Operator : CG/JU
Sample : L1542-14
Misc :
ALS Vial : 43 Sample Multiplier: 1

Quant Time: Mar 04 13:44:40 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 04 08:02:03 2020
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
DBD50

Manual Integrations
APPROVED

mohammad
3/5/2020 7:57:07 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.68	152	2981	0.40	ng/ul	0.00
2) Naphthalene-d8	10.45	136	13158	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.30	164	10172	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.05	188	24087m	0.40	ng/ul	0.00
16) Chrysene-d12	21.23	240	24535	0.40	ng/ul	0.00
20) Perylene-d12	23.43	264	24201	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.04	152	10980	0.45	ng/ul	0.00
14) Fluoranthene-d10	19.07	212	32701	0.42	ng/ul	0.00

Target Compounds

(#) = qualifier out of range (m) = manual integration (+) = signals summed

75003/05/20