


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030320\
 Data File : BM025255.D
 Acq On : 04 Mar 2020 18:08
 Operator : CG/JU
 Sample : L1516-12
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBD30

Manual Integrations
 APPROVED

mohammad
 3/5/2020 7:57:29 AM

Quant Time: Mar 05 00:58:11 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 04 08:02:03 2020
 Response via : Initial Calibration

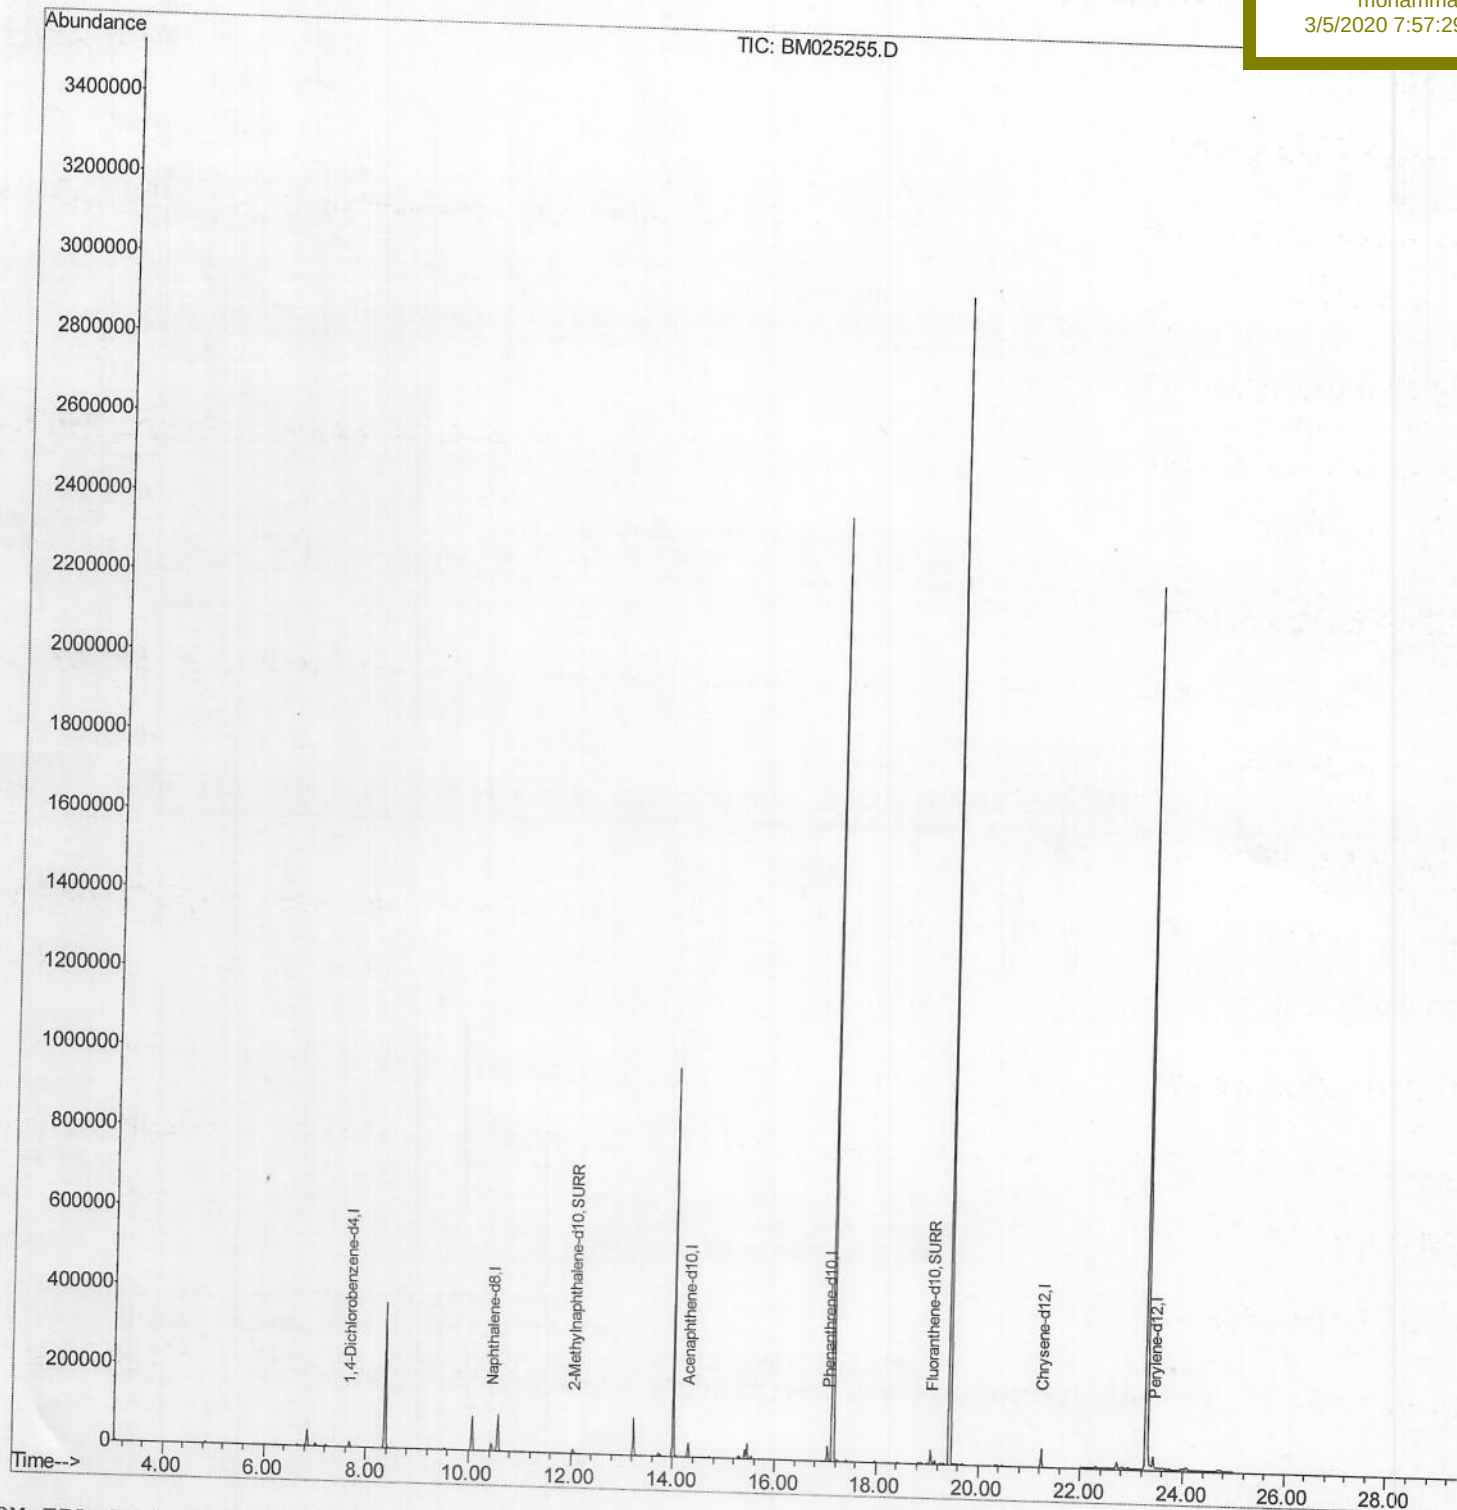

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030320\
 Data File : BM025255.D
 Acq On : 04 Mar 2020 18:08
 Operator : CG/JU
 Sample : L1516-12
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampleId :
 DBD30

Manual Integrations
APPROVED

mohammad
 3/5/2020 7:57:29 AM

Quant Time: Mar 05 00:36:42 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 04 08:02:03 2020
 Response via : Initial Calibration

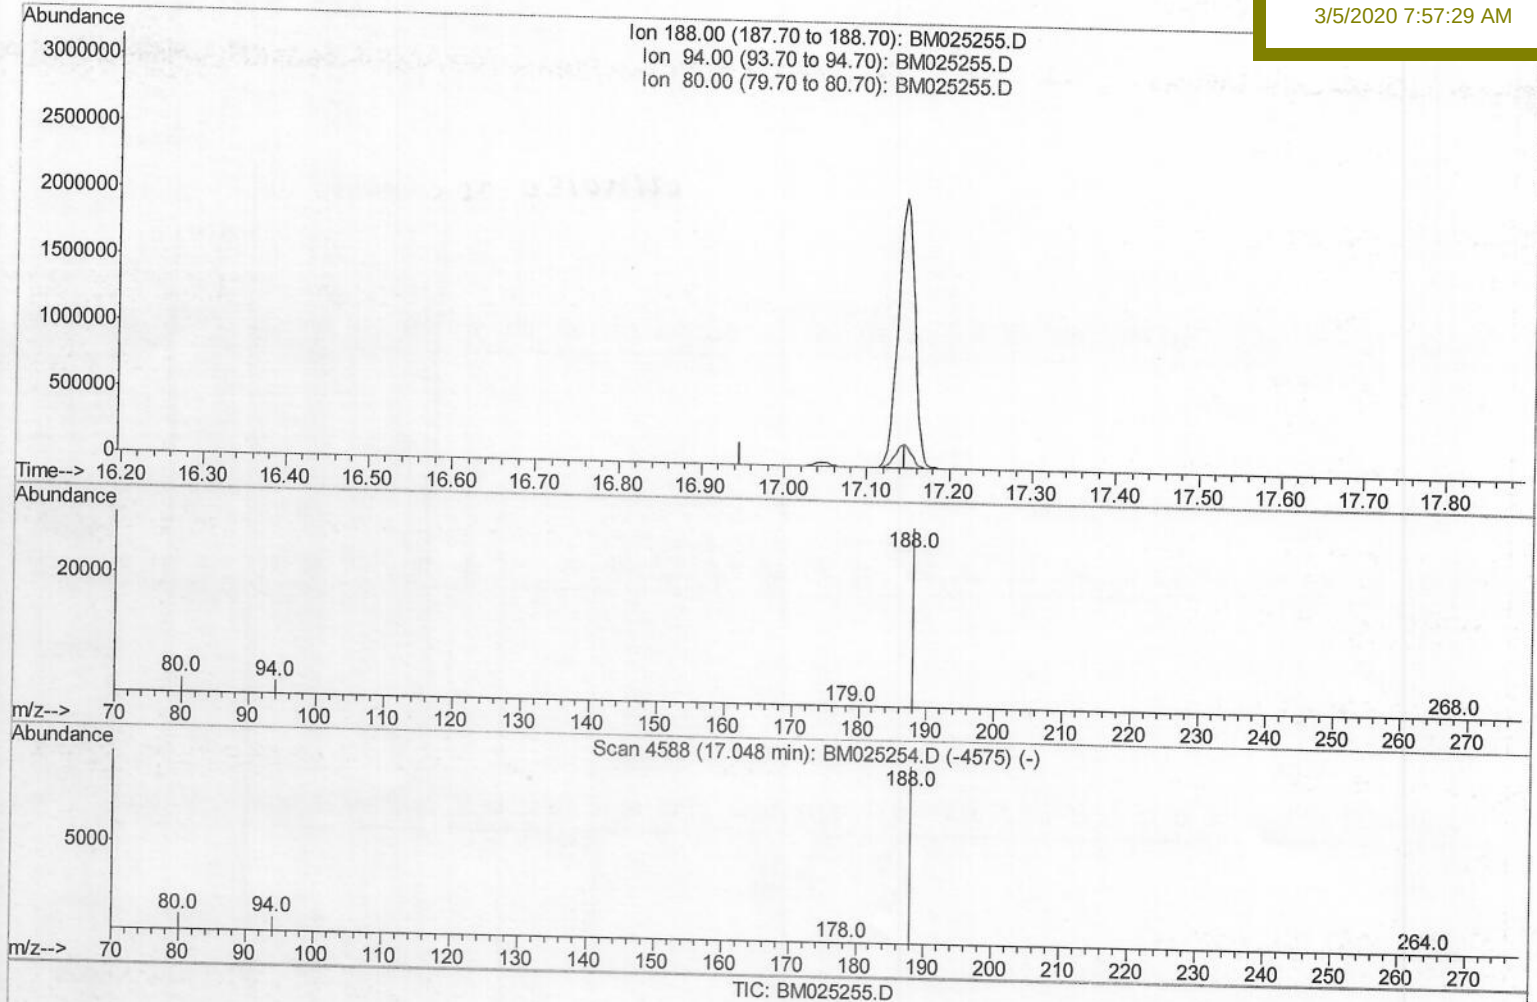

(10) Phenanthrene-d10 (I)

17.046min (-17.046) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	26.60	0.00#
80.00	22.60	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030320\

Data File : BM025255.D

Acq On : 04 Mar 2020 18:08

Operator : CG/JU

Sample : L1516-12

Misc :

ALS Vial : 51 Sample Multiplier: 1

Quant Time: Mar 05 00:36:42 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Wed Mar 04 08:02:03 2020

Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :




DBD30

Manual Integrations

APPROVED

mohammad

3/5/2020 7:57:29 AM

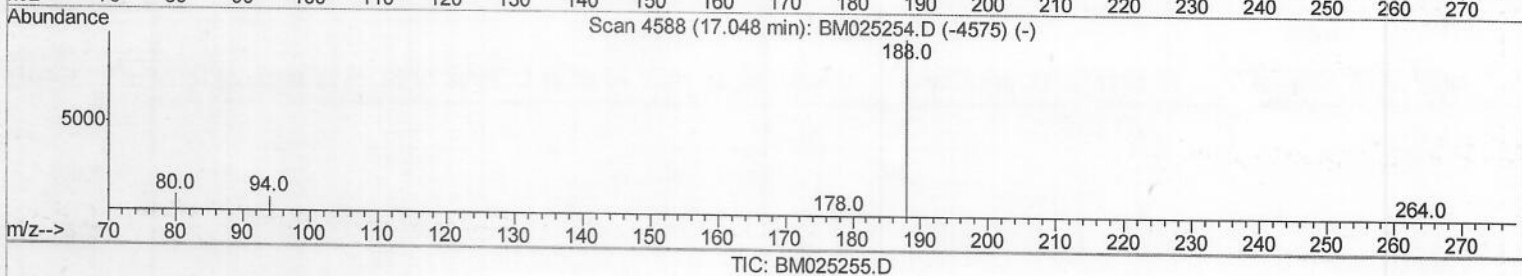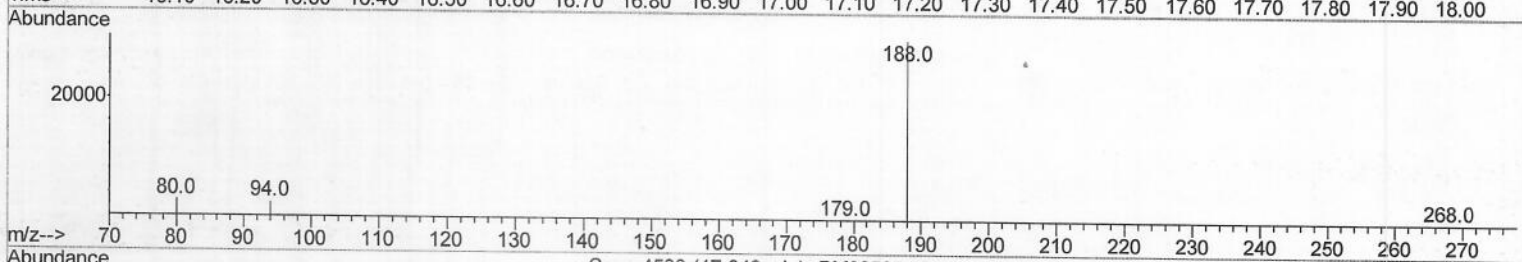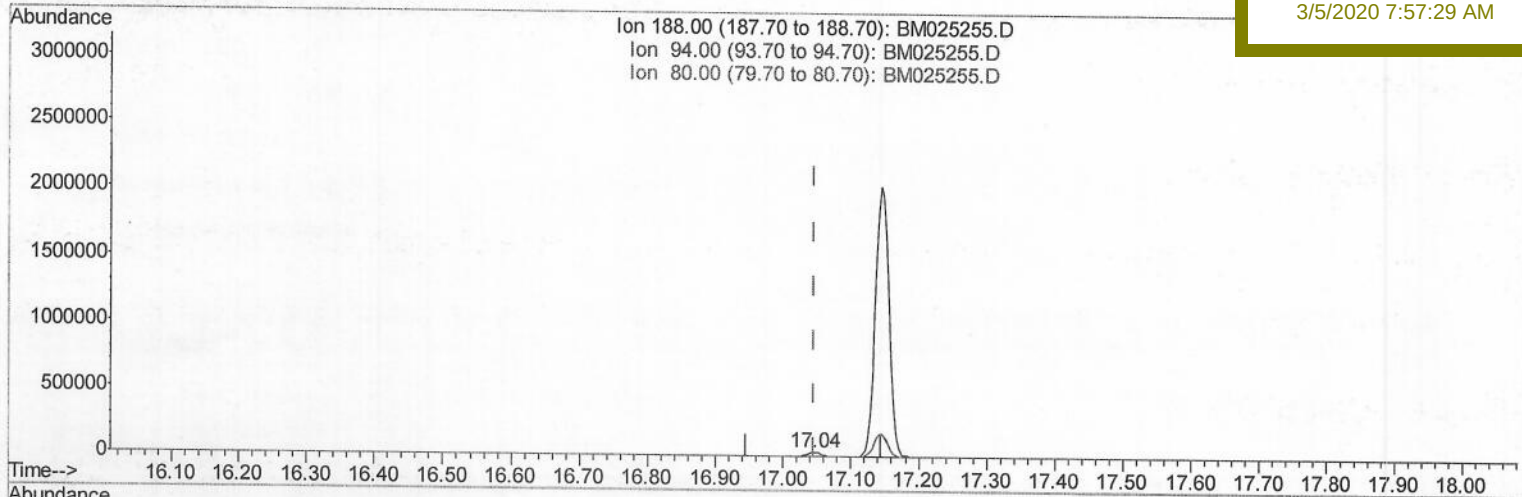

(10) Phenanthrene-d10 (I)

17.044min (-0.002) 0.40ng/ul m 206 03105/40

response 41455

Ion	Exp%	Act%
188.00	100	100
94.00	26.60	7.86#
80.00	22.60	8.83#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030320\
 Data File : BM025255.D
 Acq On : 04 Mar 2020 18:08
 Operator : CG/JU
 Sample : L1516-12
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Quant Time: Mar 05 00:58:11 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 04 08:02:03 2020
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 DBD30

Manual Integrations
 APPROVED

mohammad
 3/5/2020 7:57:29 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	7.68	152	5483	0.40	ng/ul	0.00
2) Naphthalene-d8	10.45	136	23770	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.30	164	17417	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.04	188	41455m	0.40	ng/ul	0.00
16) Chrysene-d12	21.23	240	40571	0.40	ng/ul	0.00
20) Perylene-d12	23.42	264	37557	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev (Min)
4) 2-Methylnaphthalene-d10	12.04	152	12919	0.29	ng/ul	0.00
14) Fluoranthene-d10	19.07	212	38597	0.29	ng/ul	0.00

Target Compounds	Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed