


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030320\
Data File : BM025261.D
Acq On : 04 Mar 2020 21:46
Operator : CG/JU
Sample : L1516-18
Misc :
ALS Vial : 57 Sample Multiplier: 1

Quant Time: Mar 05 01:22:58 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
OLast Update : Wed Mar 04 08:02:03 2020
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
DBD76

Manual Integrations
APPROVED

mohammad
3/5/2020 7:57:47 AM

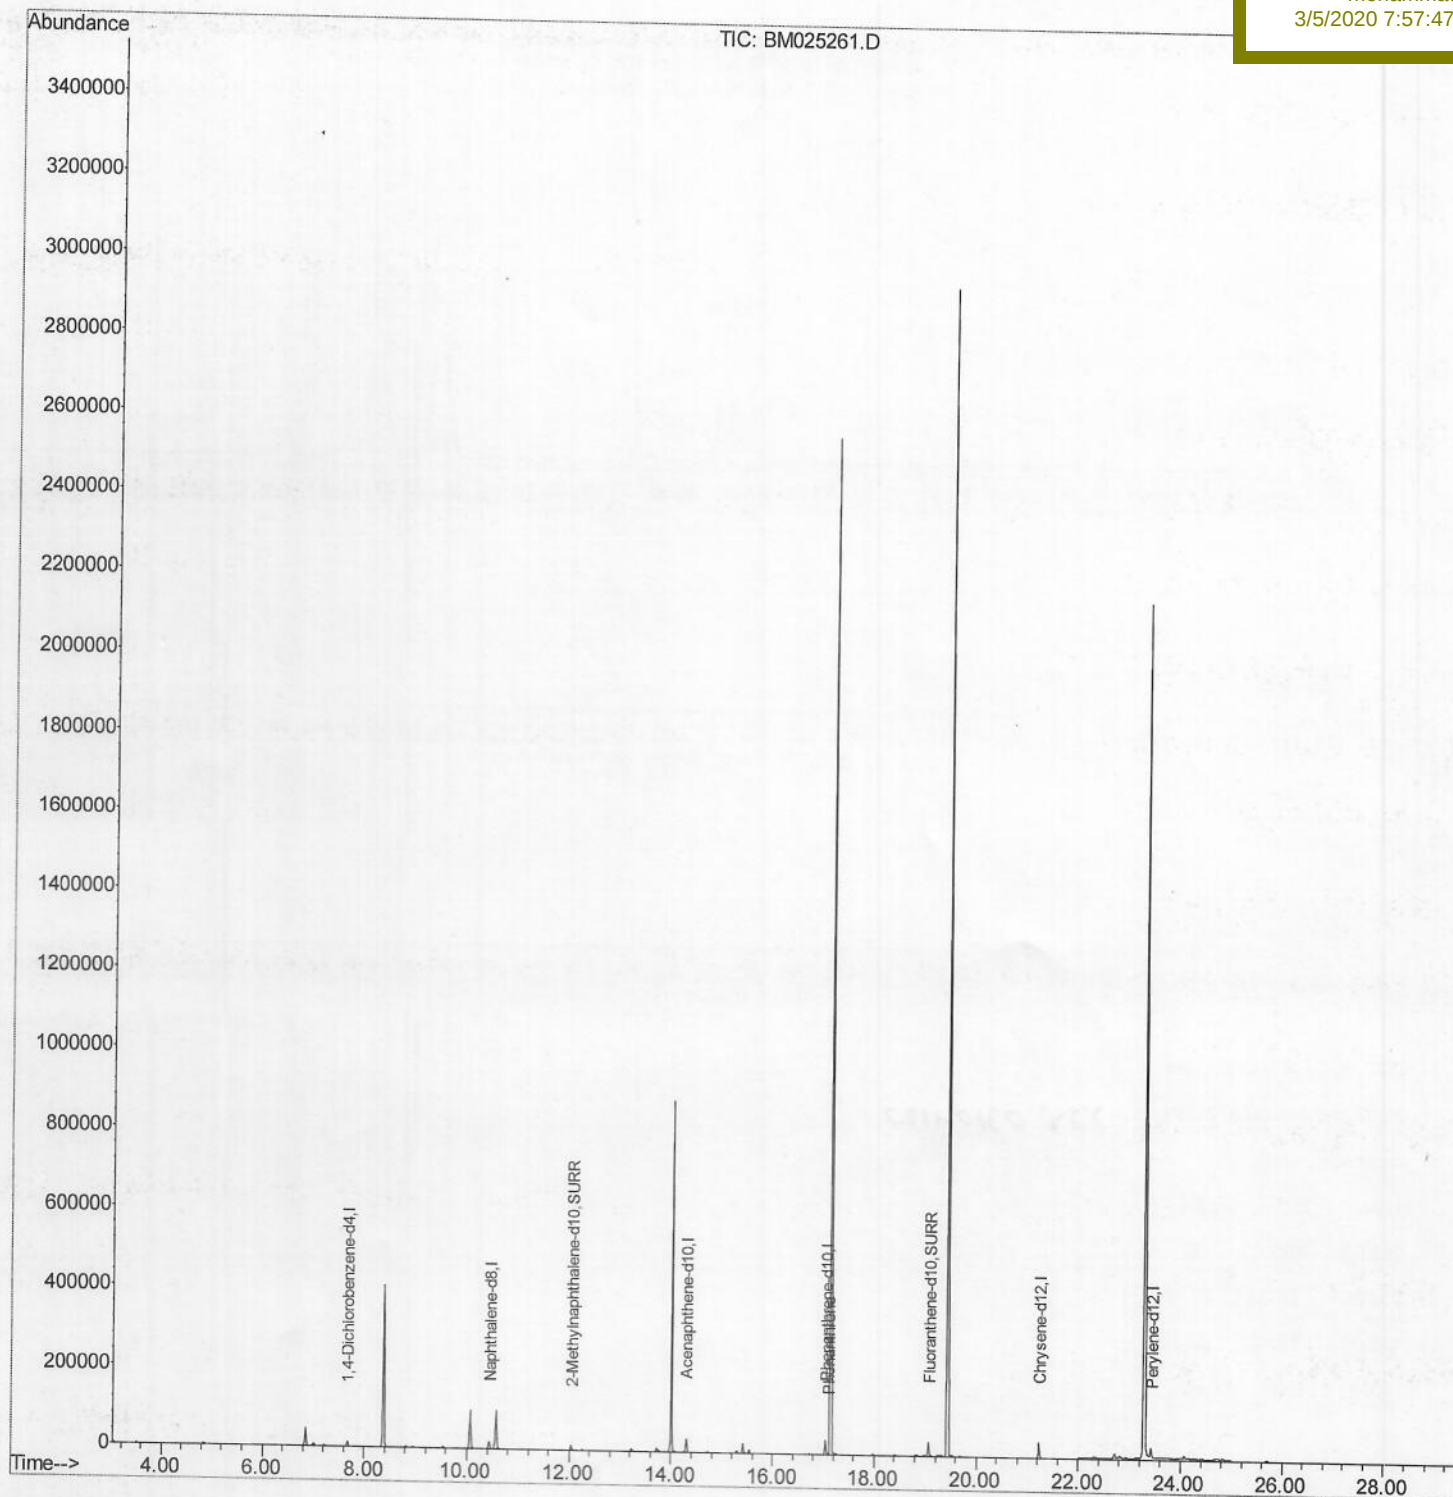

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030320\

Data File : BM025261.D

Acq On : 04 Mar 2020 21:46

Operator : CG/JU

Sample : L1516-18

Misc :

ALS Vial : 57 Sample Multiplier: 1

Quant Time: Mar 05 00:37:06 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Wed Mar 04 08:02:03 2020




Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :

DBD76

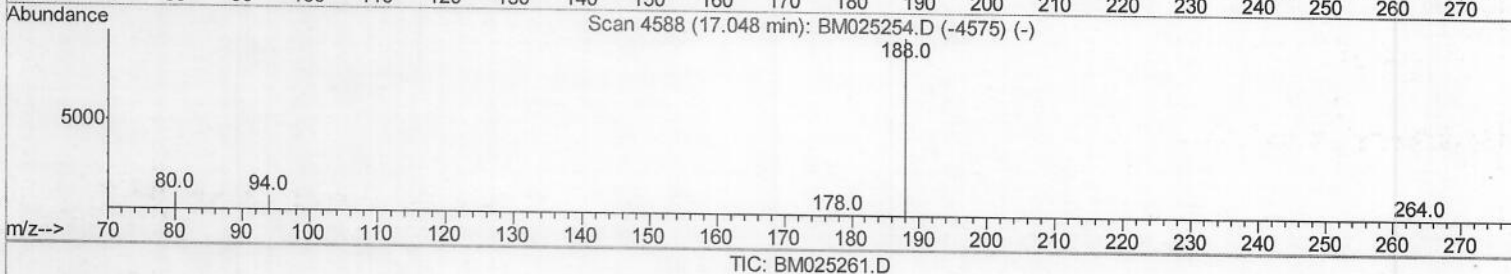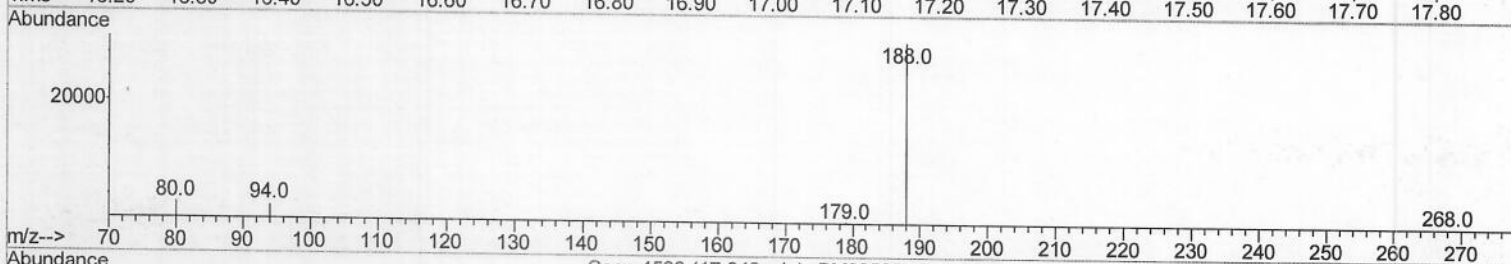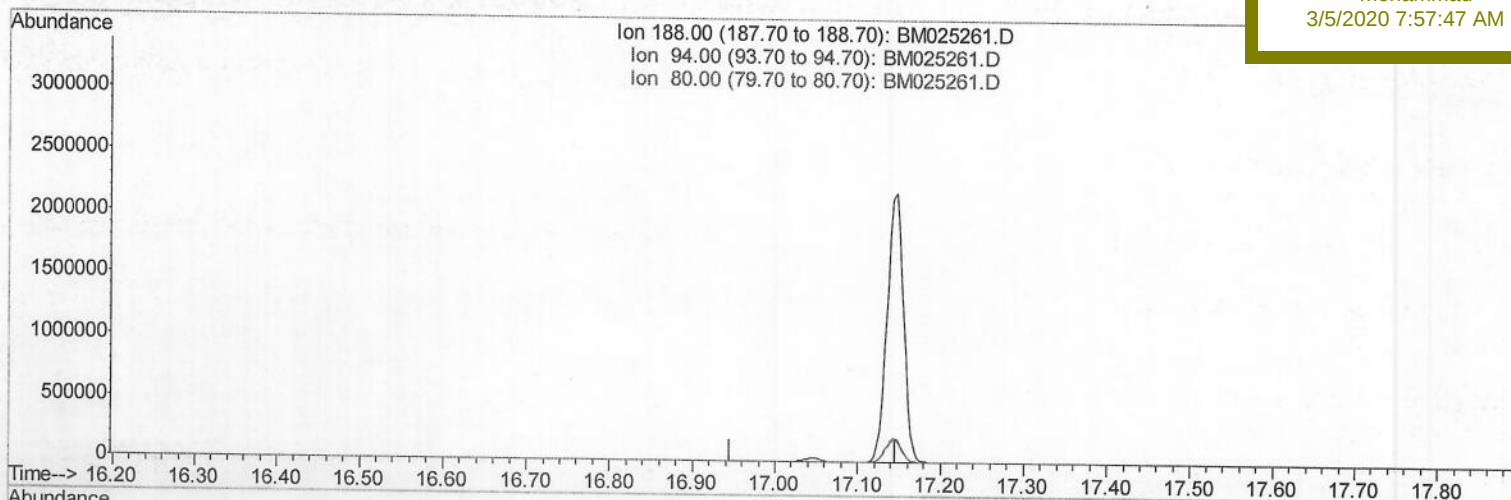Manual Integrations
APPROVEDmohammad
3/5/2020 7:57:47 AM

(10) Phenanthrene-d10 (I)

17.046min (-17.046) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	26.60	0.00#
80.00	22.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030320\
 Data File : BM025261.D
 Acq On : 04 Mar 2020 21:46
 Operator : CG/JU
 Sample : L1516-18
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Quant Time: Mar 05 00:37:06 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 04 08:02:03 2020
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 DBD76

Manual Integrations
 APPROVED

mohammad
 3/5/2020 7:57:47 AM

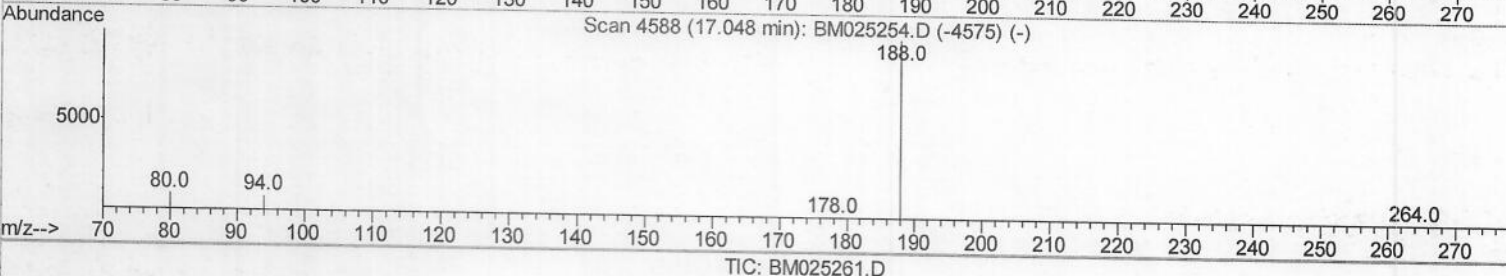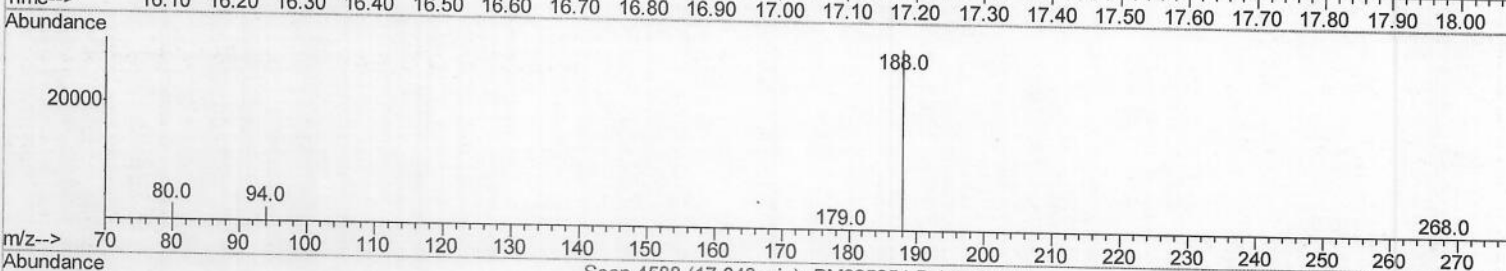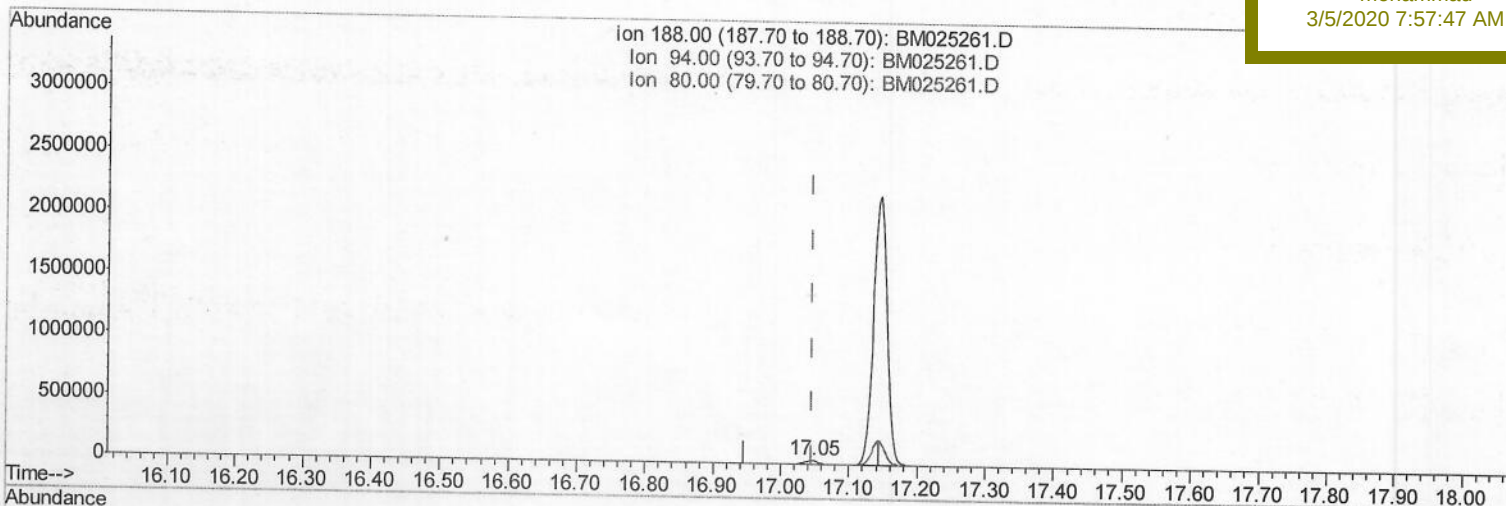

(10) Phenanthrene-d10 (I)

17.046min (-0.000) 0.40ng/ul m>JU 03/05/20

response 41874

Ion	Exp%	Act%
188.00	100	100
94.00	26.60	7.76#
80.00	22.60	8.76#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030320\
 Data File : BM025261.D
 Acq On : 04 Mar 2020 21:46
 Operator : CG/JU
 Sample : L1516-18
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Quant Time: Mar 05 01:22:58 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 04 08:02:03 2020
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 DBD76

Manual Integrations
 APPROVED

mohammad
 3/5/2020 7:57:47 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.68	152	5851	0.40	ng/ul	0.00
2) Naphthalene-d8	10.44	136	25549	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.30	164	18451	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.05	188	41874m)	0.40	ng/ul	0.00
16) Chrysene-d12	21.23	240	34292	0.40	ng/ul	0.00
20) Perylene-d12	23.42	264	32633	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.04	152	15092	0.32	ng/ul	0.00
14) Fluoranthene-d10	19.07	212	39137	0.29	ng/ul	0.00
Target Compounds						
12) Phenanthrene	17.08	178	2749	0.020	ng/ul	Ovalue 98

(#) = qualifier out of range (m) = manual integration (+) = signals summed