


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030320\
Data File : BM025266.D
Acq On : 05 Mar 2020 00:48
Operator : CG/JU
Sample : L1708-05
Misc :
ALS Vial : 62 Sample Multiplier: 1

Quant Time: Mar 05 01:31:44 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 05 00:55:12 2020
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampled :
C0CE2

Manual Integrations
APPROVED

mohammad
3/5/2020 7:58:00 AM

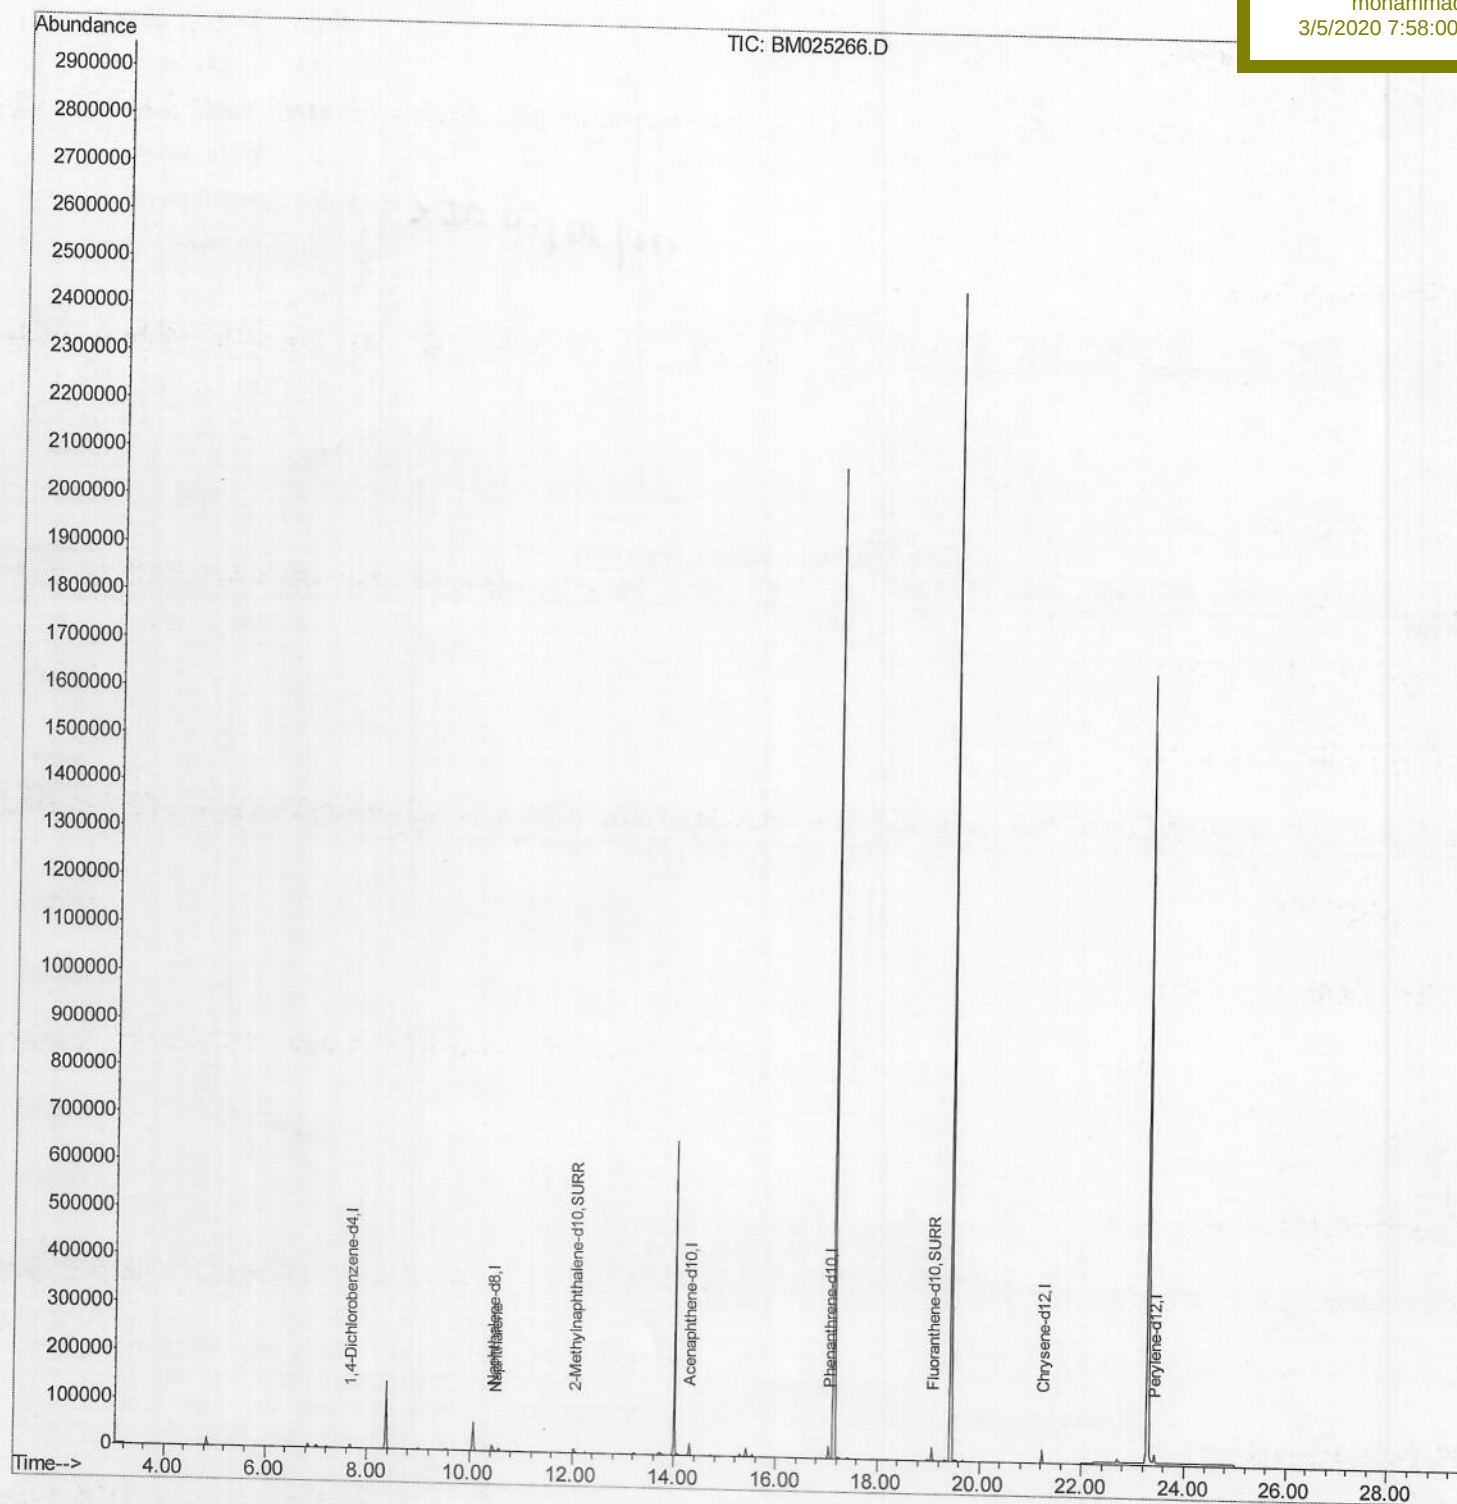

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030320\
 Data File : BM025266.D
 Acq On : 05 Mar 2020 00:48
 Operator : CG/JU
 Sample : L1708-05
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Quant Time: Mar 05 01:30:44 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 05 00:55:12 2020
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 C0CE2

Manual Integrations
 APPROVED

mohammad
 3/5/2020 7:58:00 AM

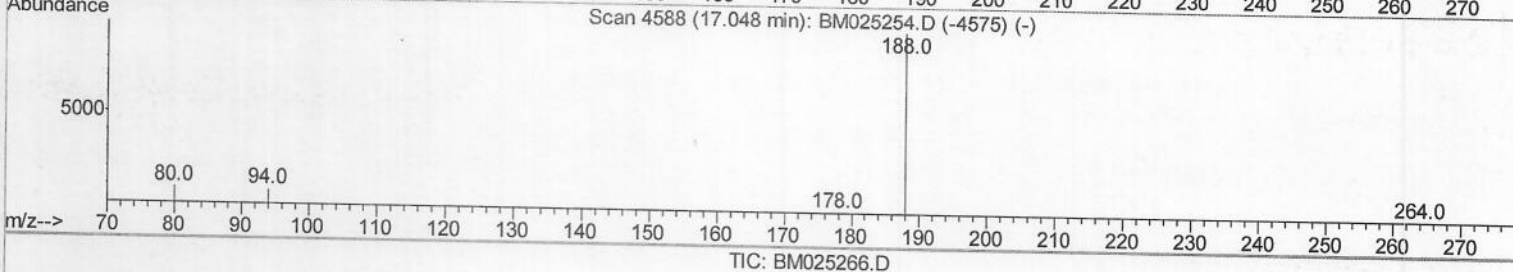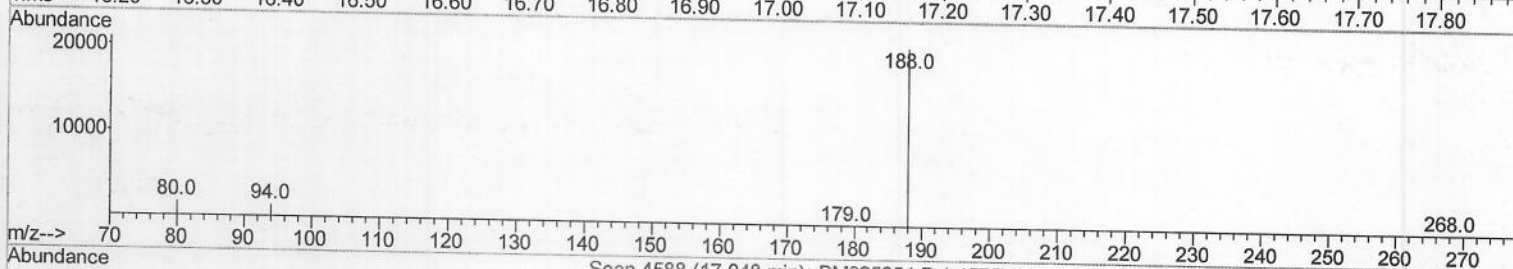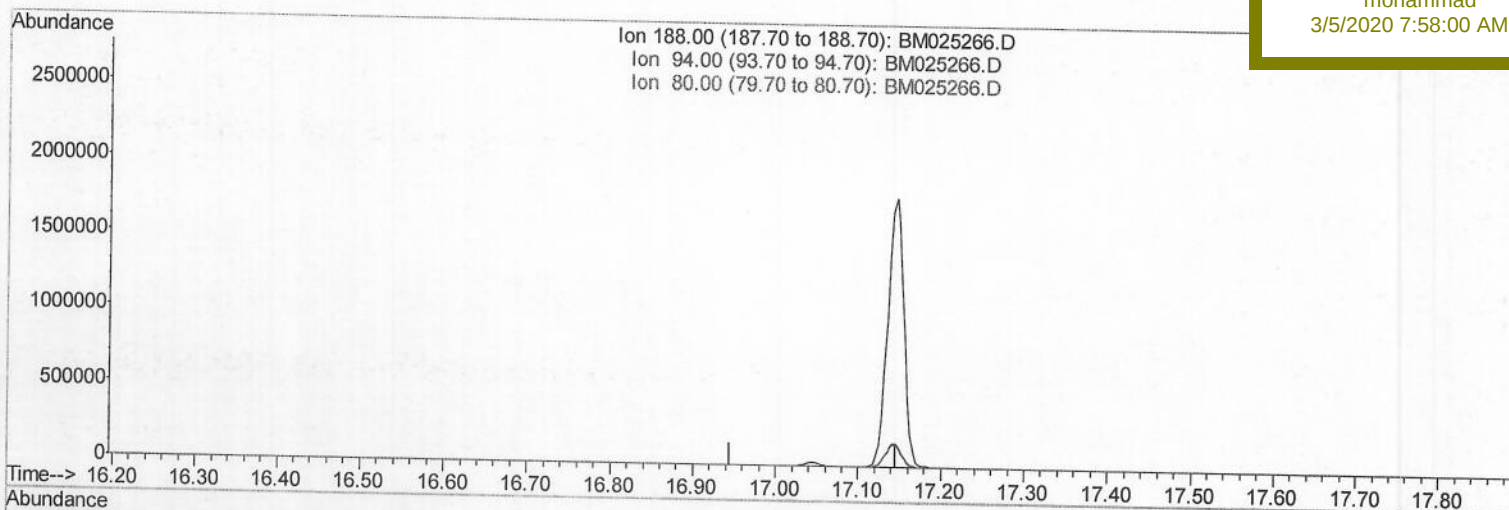

(10) Phenanthrene-d10 (I)
 17.046min (-17.046) 0.00ng/ul
 response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	26.60	0.00#
80.00	22.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030320\
 Data File : BM025266.D
 Acq On : 05 Mar 2020 00:48
 Operator : CG/JU
 Sample : L1708-05
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Quant Time: Mar 05 01:30:44 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 05 00:55:12 2020
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 C0CE2

Manual Integrations
 APPROVED

mohammad
 3/5/2020 7:58:00 AM

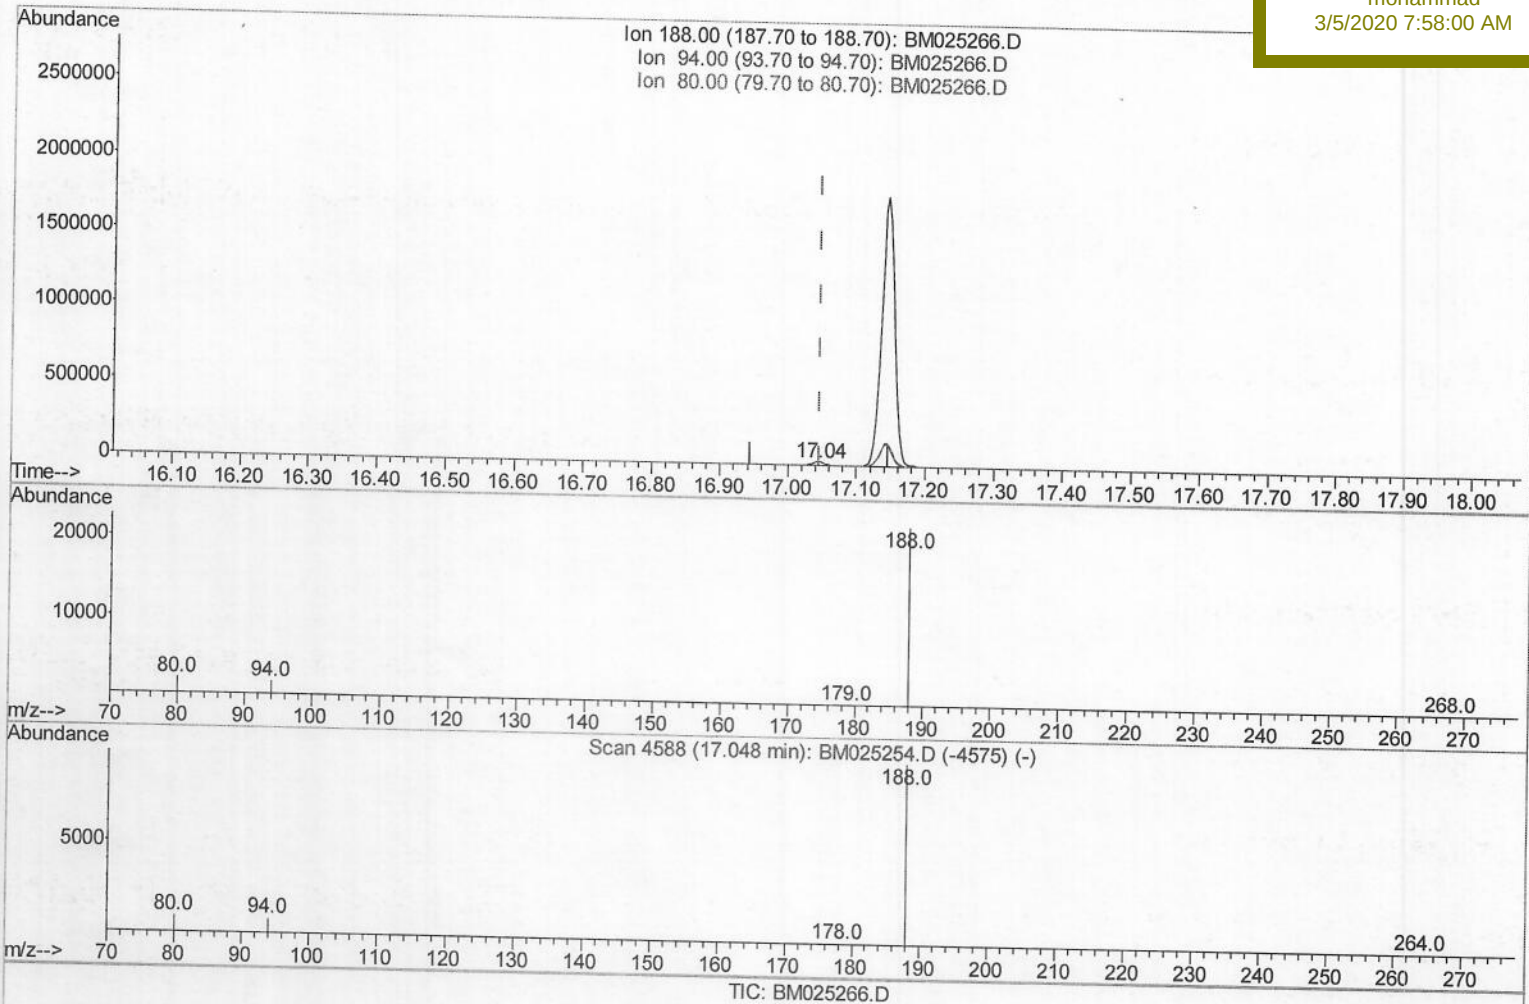

(10) Phenanthrene-d10 (I)

17.044min (-0.002) 0.40ng/ul m > 50 03105120

response 29776

Ion	Exp%	Act%
188.00	100	100
94.00	26.60	7.70#
80.00	22.60	8.92#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030320\
 Data File : BM025266.D
 Acq On : 05 Mar 2020 00:48
 Operator : CG/JU
 Sample : L1708-05
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0CE2

Quant Time: Mar 05 01:31:44 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 05 00:55:12 2020
 Response via : Initial Calibration

Manual Integrations
 APPROVED

mohammad
 3/5/2020 7:58:00 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.68	152	4052	0.40	ng/ul	0.00
2) Naphthalene-d8	10.44	136	17401	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.30	164	13018	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.04	188	29776m	0.40	ng/ul	0.00
16) Chrysene-d12	21.23	240	25000	0.40	ng/ul	0.00
20) Perylene-d12	23.42	264	22872	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.04	152	10364	0.32	ng/ul	0.00
14) Fluoranthene-d10	19.07	212	30215	0.31	ng/ul	0.00
Target Compounds						
3) Naphthalene	10.49	128	1069	0.020	ng/ul	Ovalue 97

(#) = qualifier out of range (m) = manual integration (+) = signals summed