


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030320\
Data File : BM025267.D
Acq On : 05 Mar 2020 01:24
Operator : CG/JU
Sample : L1708-02
Misc :
ALS Vial : 63 Sample Multiplier: 1

Quant Time: Mar 05 04:25:24 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 05 00:55:12 2020
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampled :
C0C98

Manual Integrations
APPROVED

mohammad
3/5/2020 7:58:03 AM

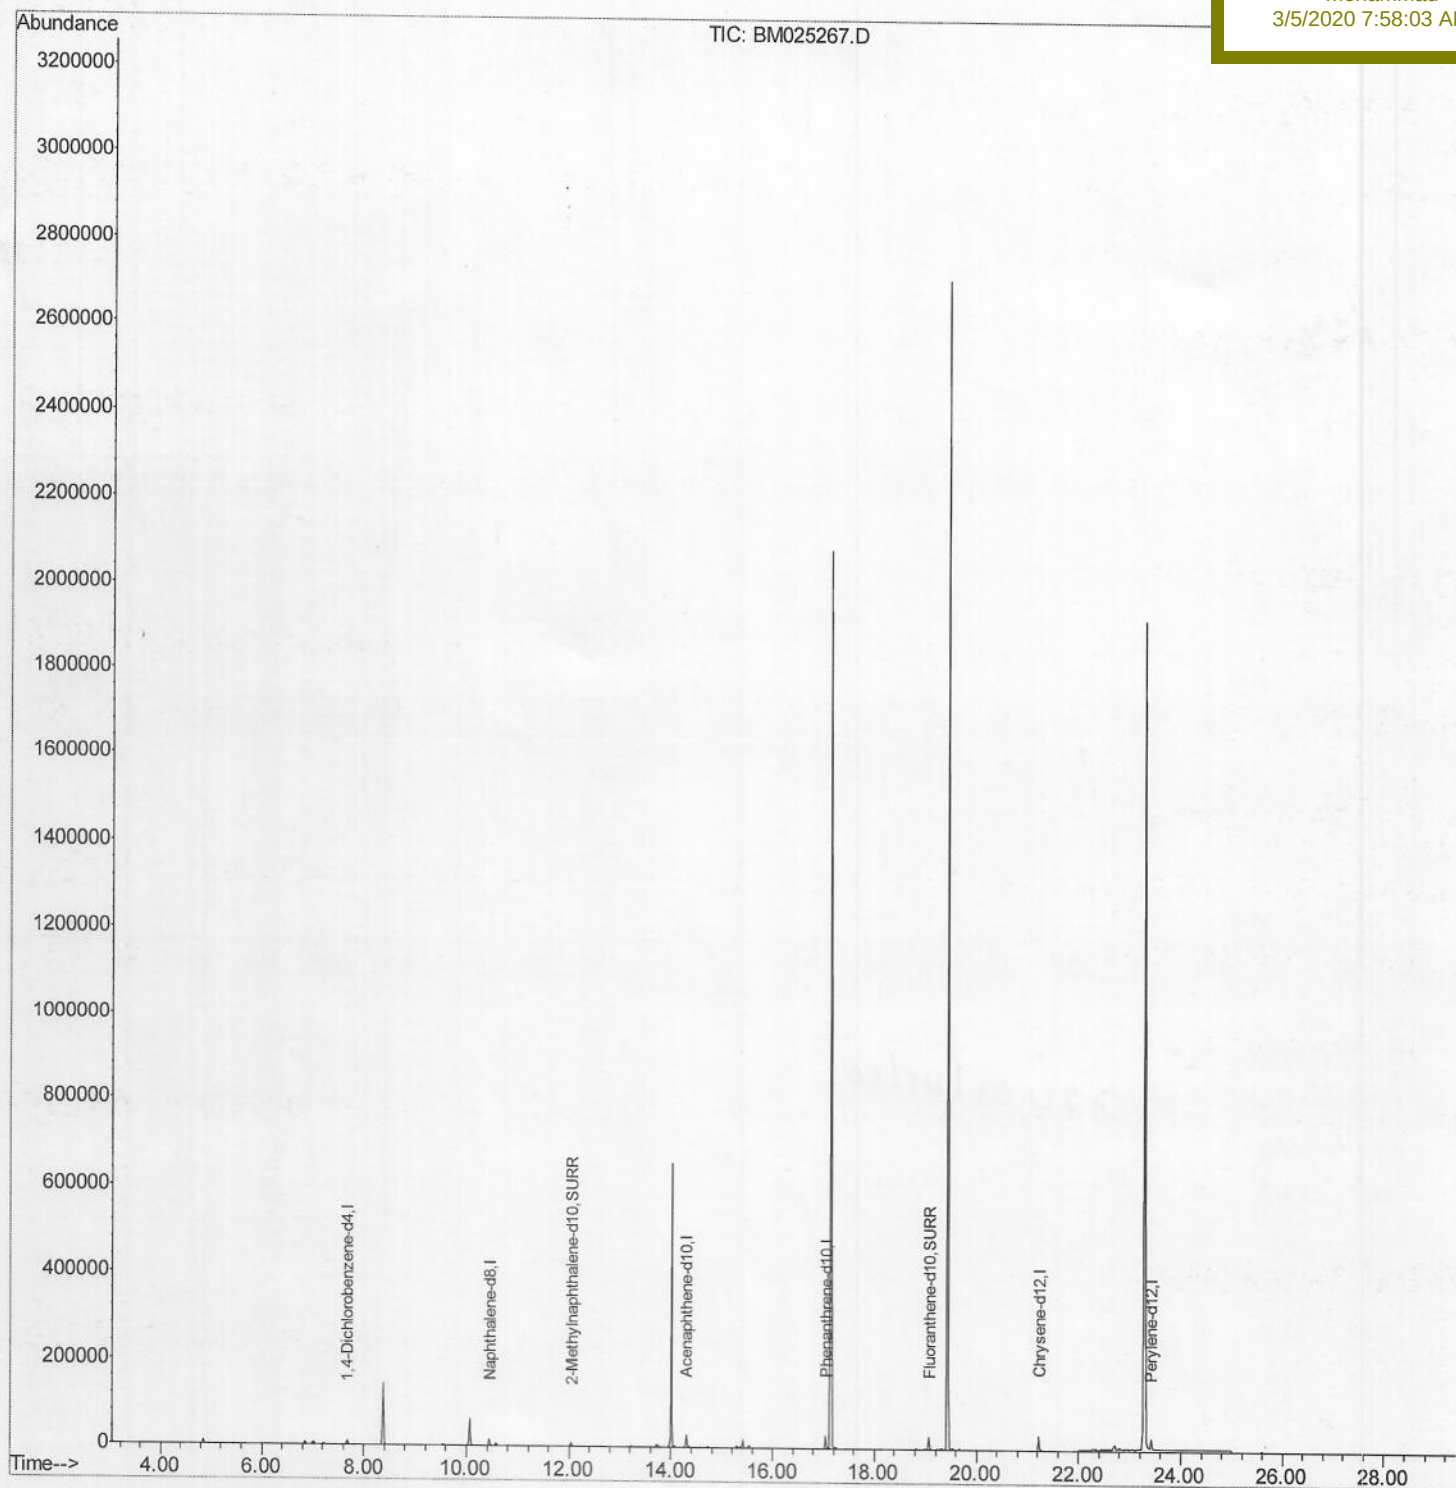

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030320\

Data File : BM025267.D

Acq On : 05 Mar 2020 01:24

Operator : CG/JU

Sample : L1708-02

Misc :

ALS Vial : 63 Sample Multiplier: 1

Quant Time: Mar 05 04:24:19 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Thu Mar 05 00:55:12 2020




Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :

C0C98

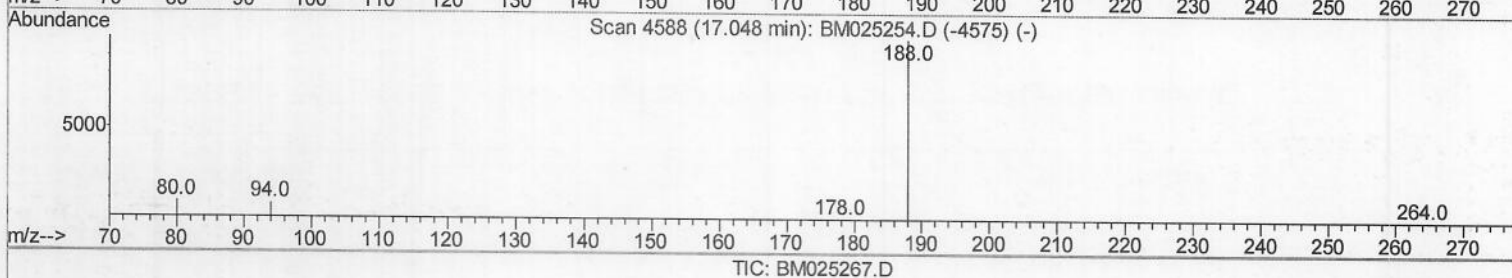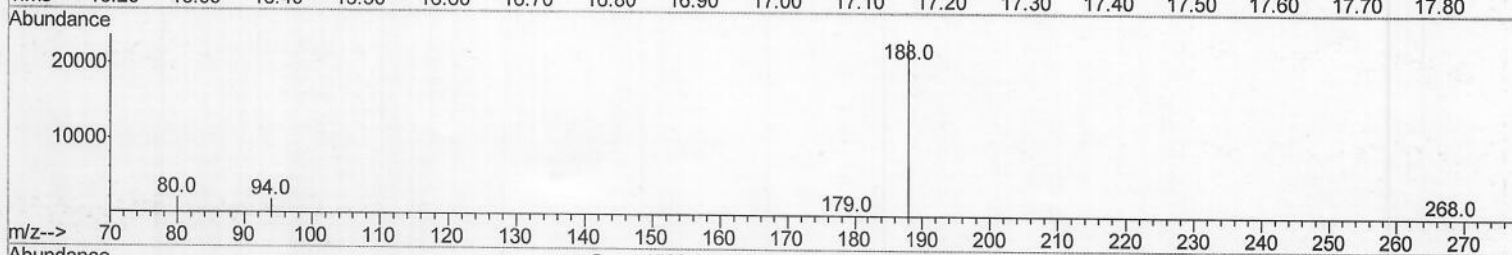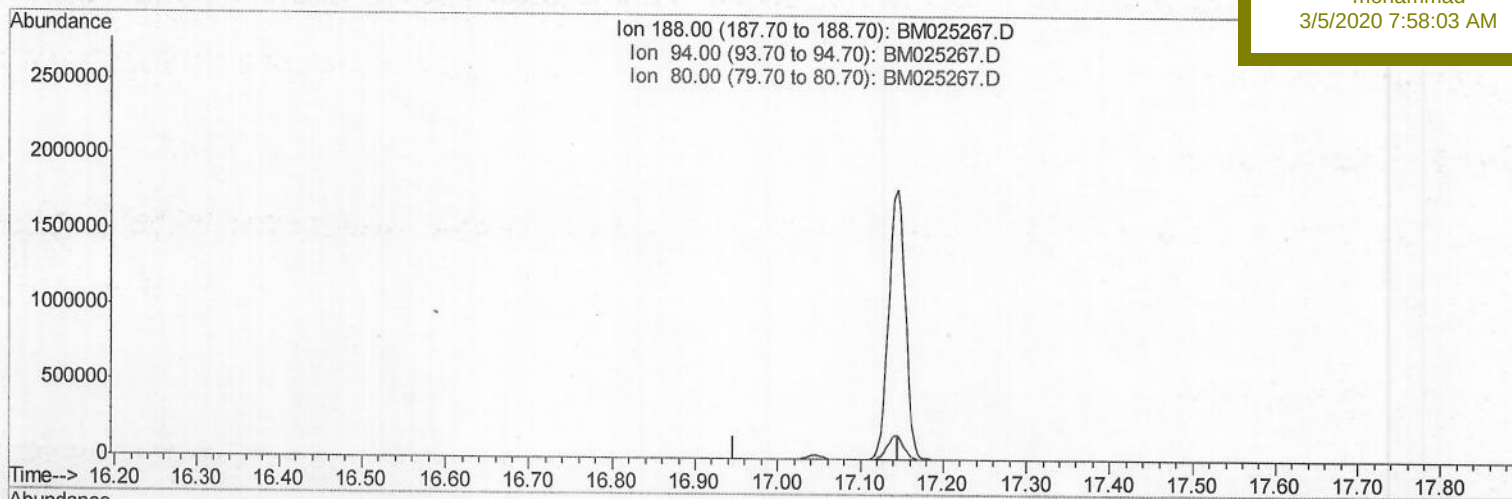Manual Integrations
APPROVEDmohammad
3/5/2020 7:58:03 AM

(10) Phenanthrene-d10 (I)

17.046min (-17.046) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	26.60	0.00#
80.00	22.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030320\

Data File : BM025267.D

Acq On : 05 Mar 2020 01:24

Operator : CG/JU

Sample : L1708-02

Misc :

ALS Vial : 63 Sample Multiplier: 1

Quant Time: Mar 05 04:24:19 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Thu Mar 05 00:55:12 2020

Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :




C0C98

Manual Integrations

APPROVED

mohammad

3/5/2020 7:58:03 AM

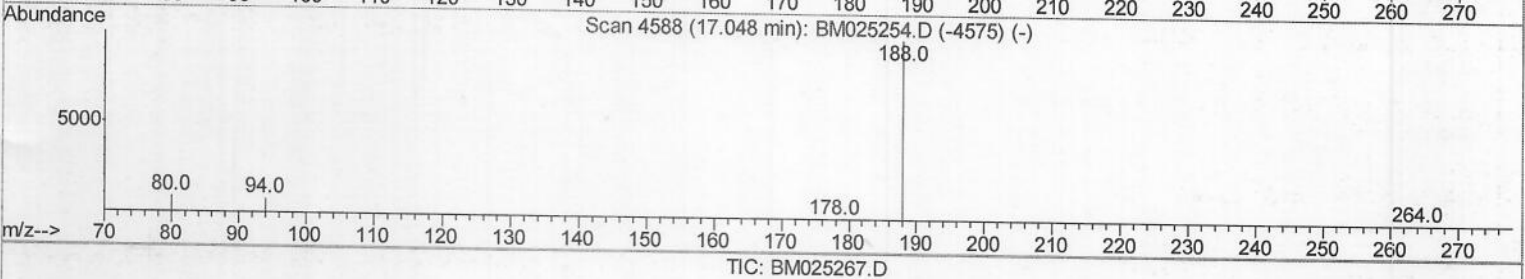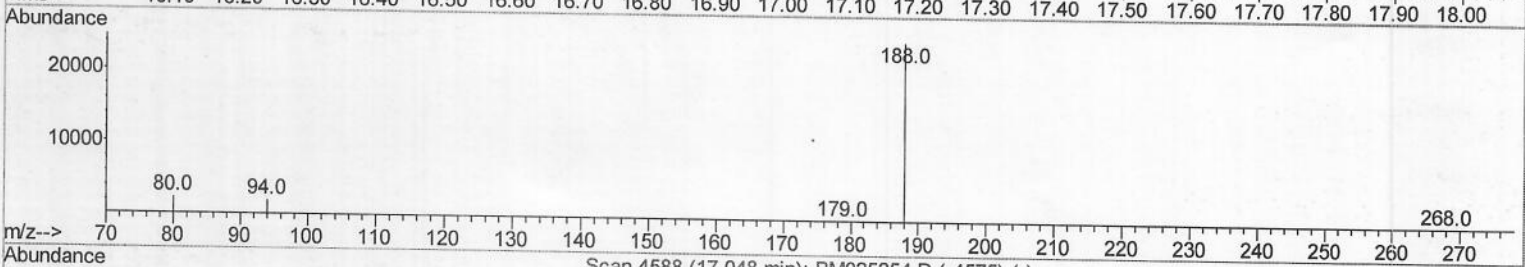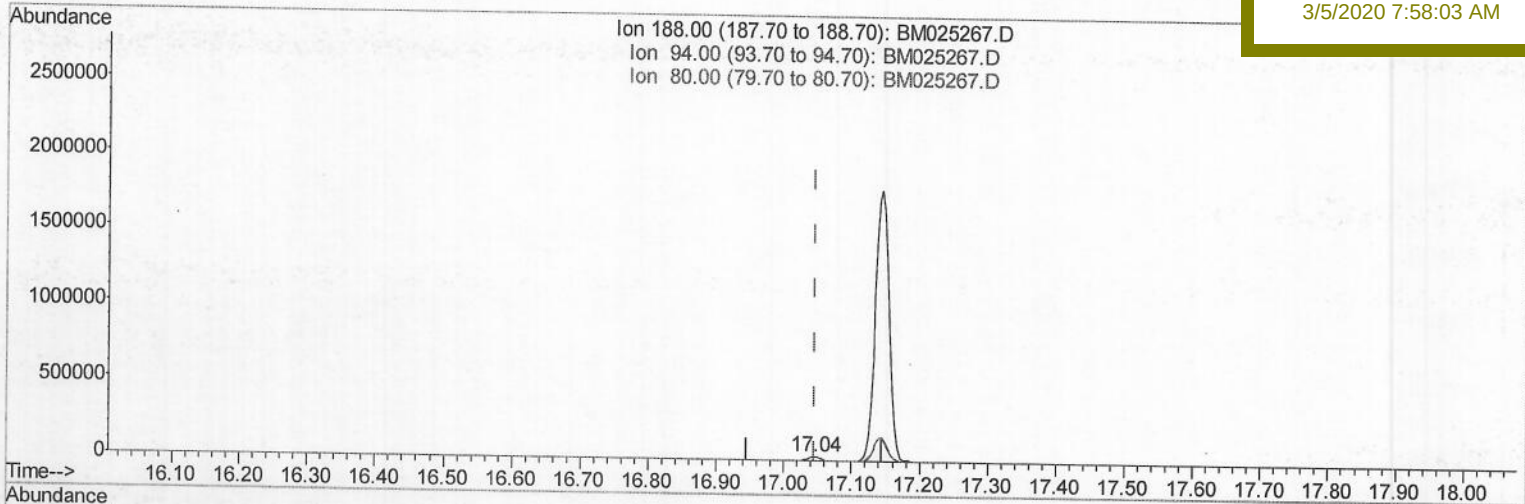

(10) Phenanthrene-d10 (I)

17.044min (-0.002) 0.40ng/ul m > 5v 03/05/20

response 33718

Ion	Exp%	Act%
188.00	100	100
94.00	26.60	7.94#
80.00	22.60	9.21#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030320\
Data File : BM025267.D
Acq On : 05 Mar 2020 01:24
Operator : CG/JU
Sample : L1708-02
Misc :
ALS Vial : 63 Sample Multiplier: 1

Quant Time: Mar 05 04:25:24 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 05 00:55:12 2020
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
C0C98

Manual Integrations
APPROVED

mohammad
3/5/2020 7:58:03 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.68	152	4493	0.40	ng/ul	0.00
2) Naphthalene-d8	10.44	136	19338	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.30	164	14294	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.04	188	33718m)	0.40	ng/ul	0.00
16) Chrysene-d12	21.23	240	30951	0.40	ng/ul	0.00
20) Perylene-d12	23.42	264	28175	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.04	152	9946	0.27	ng/ul	0.00
14) Fluoranthene-d10	19.07	212	32636	0.30	ng/ul	0.00

Target Compounds Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

03/05/20