


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030320\
 Data File : BM025268.D
 Acq On : 05 Mar 2020 02:00
 Operator : CG/JU
 Sample : L1708-04
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Quant Time: Mar 05 04:26:48 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 05 00:55:12 2020
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 C0CE0

Manual Integrations
 APPROVED

mohammad
 3/5/2020 7:58:06 AM

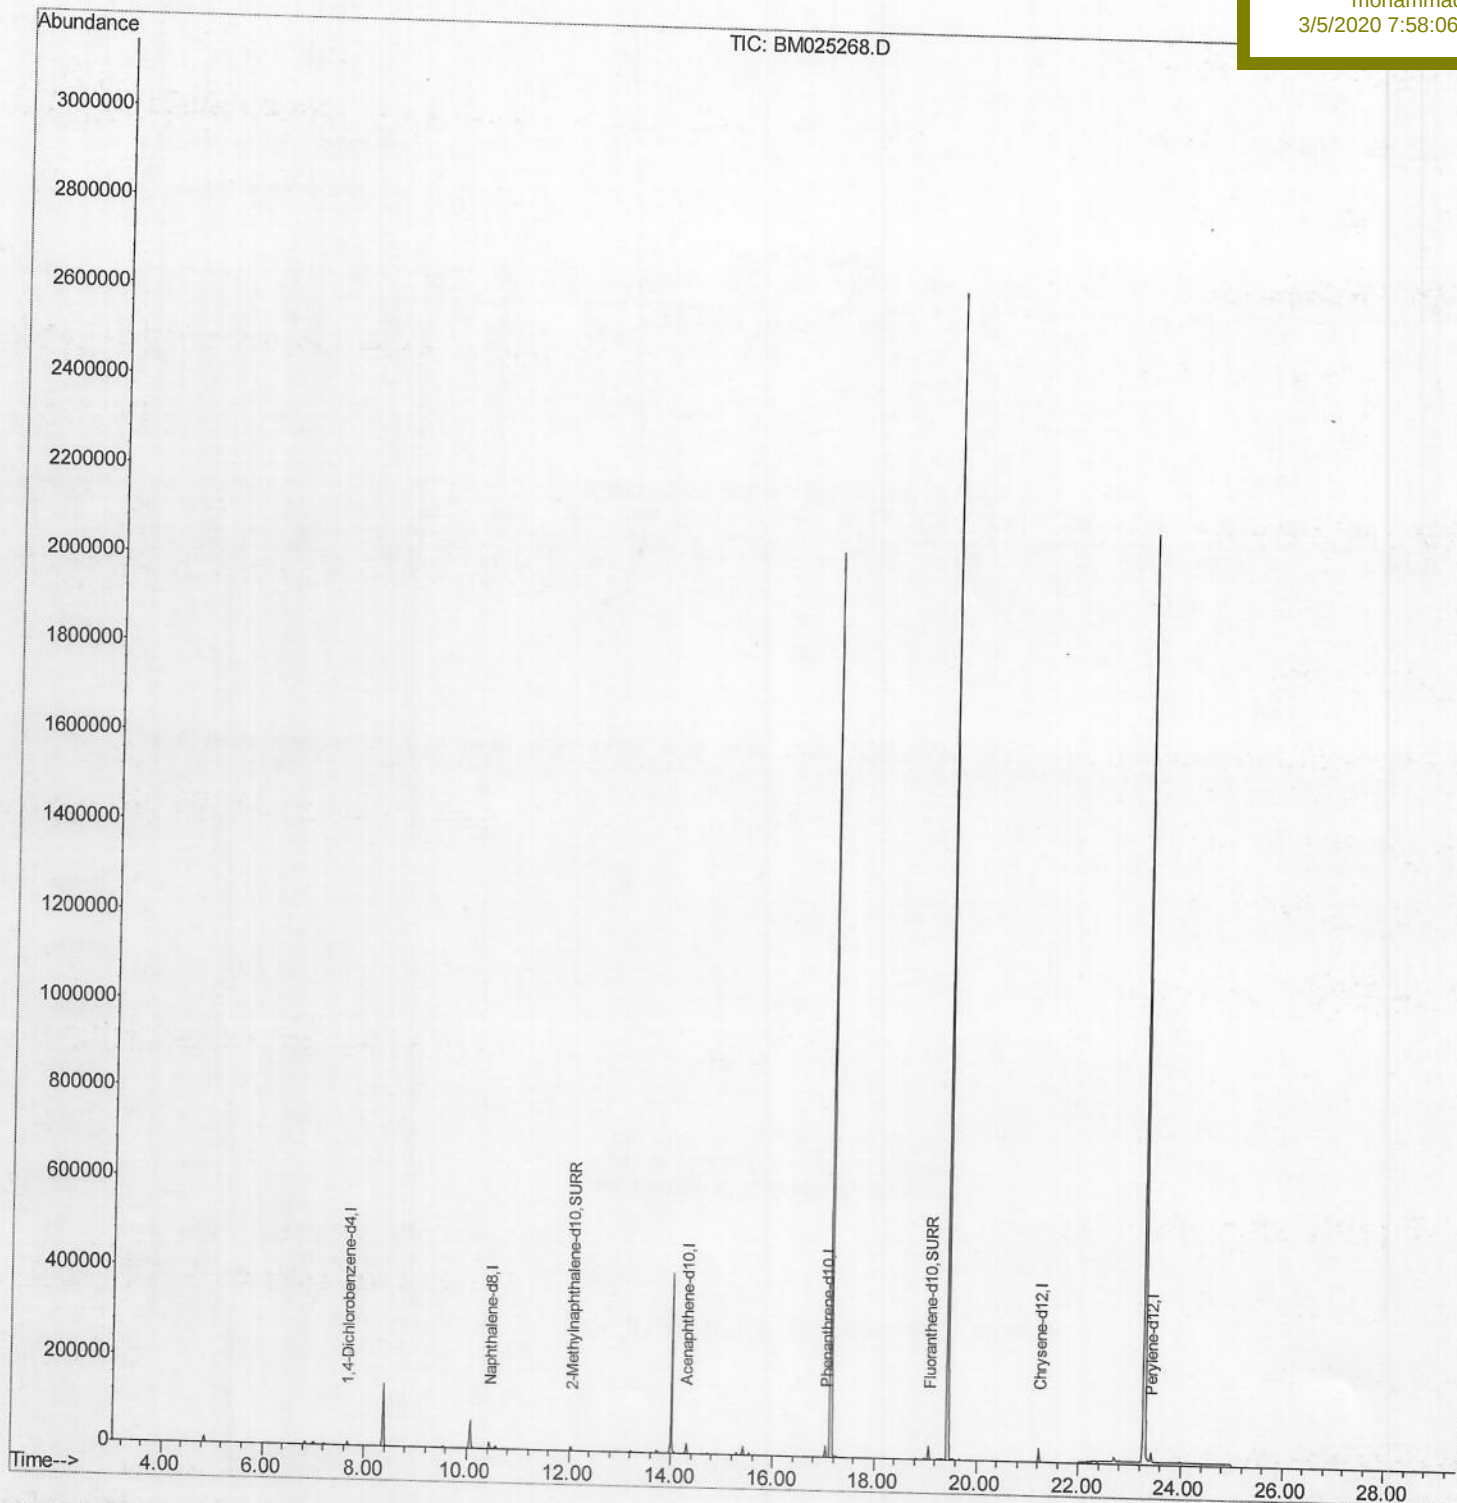

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030320\
 Data File : BM025268.D
 Acq On : 05 Mar 2020 02:00
 Operator : CG/JU
 Sample : L1708-04
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Quant Time: Mar 05 04:25:45 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 05 00:55:12 2020
 Response via : Initial Calibration

Instrument :
 BNA_M
ClientSampleId :
 C0CE0

Manual Integrations
APPROVED

mohammad
 3/5/2020 7:58:06 AM

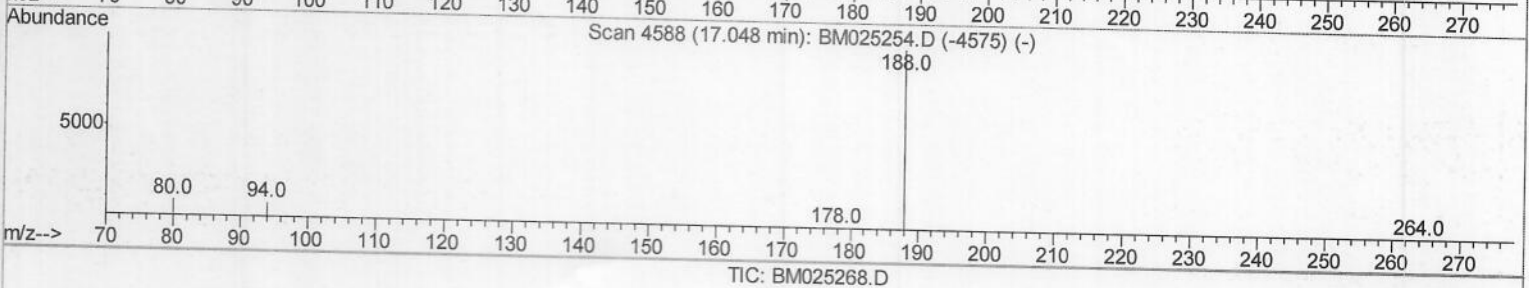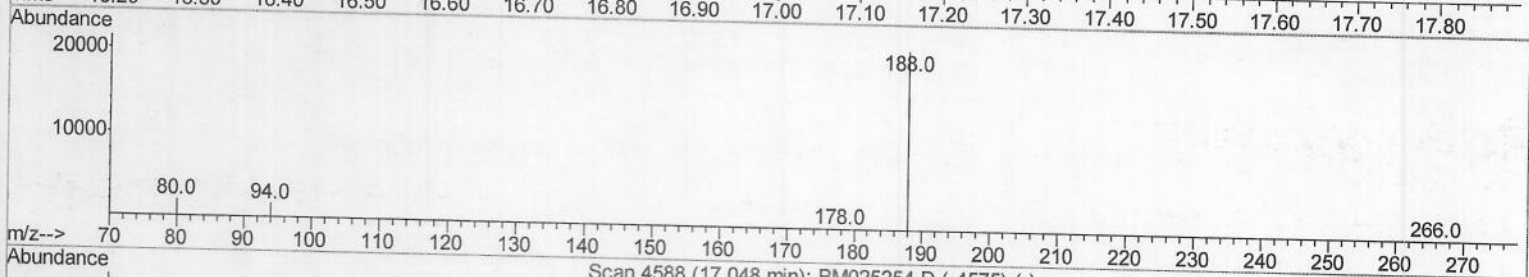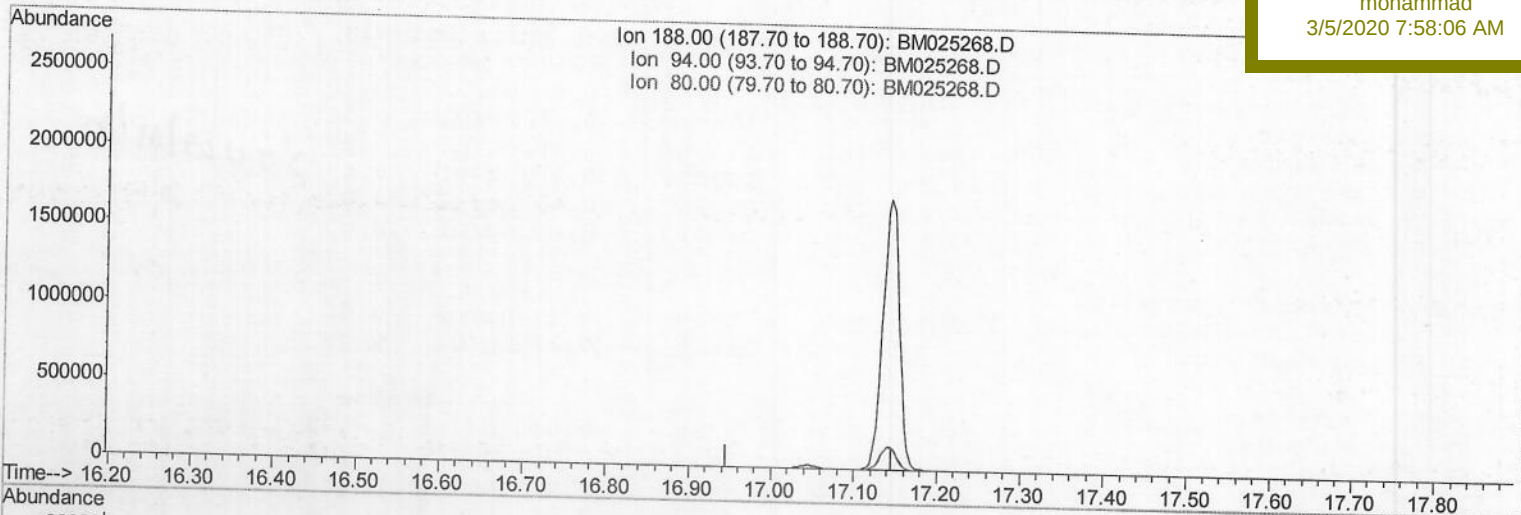

(10) Phenanthrene-d10 (I)

17.046min (-17.046) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	26.60	0.00#
80.00	22.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030320\
 Data File : BM025268.D
 Acq On : 05 Mar 2020 02:00
 Operator : CG/JU
 Sample : L1708-04
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Quant Time: Mar 05 04:25:45 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 05 00:55:12 2020
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 C0CE0

Manual Integrations
 APPROVED

mohammad
 3/5/2020 7:58:06 AM

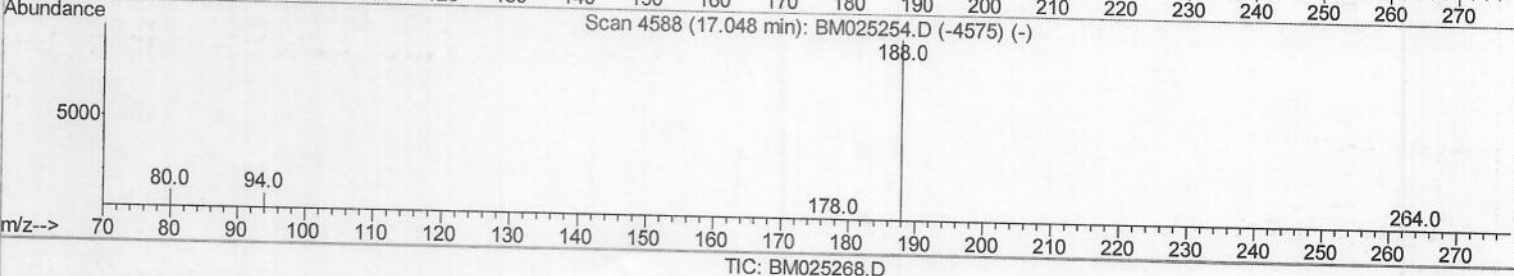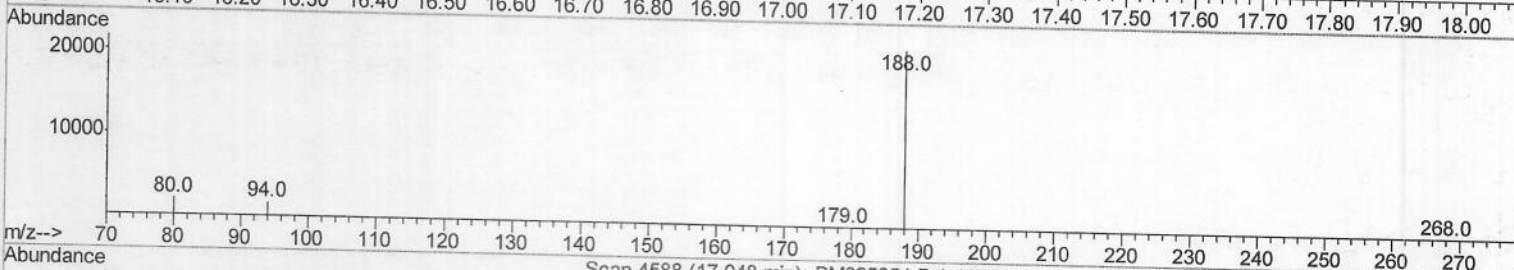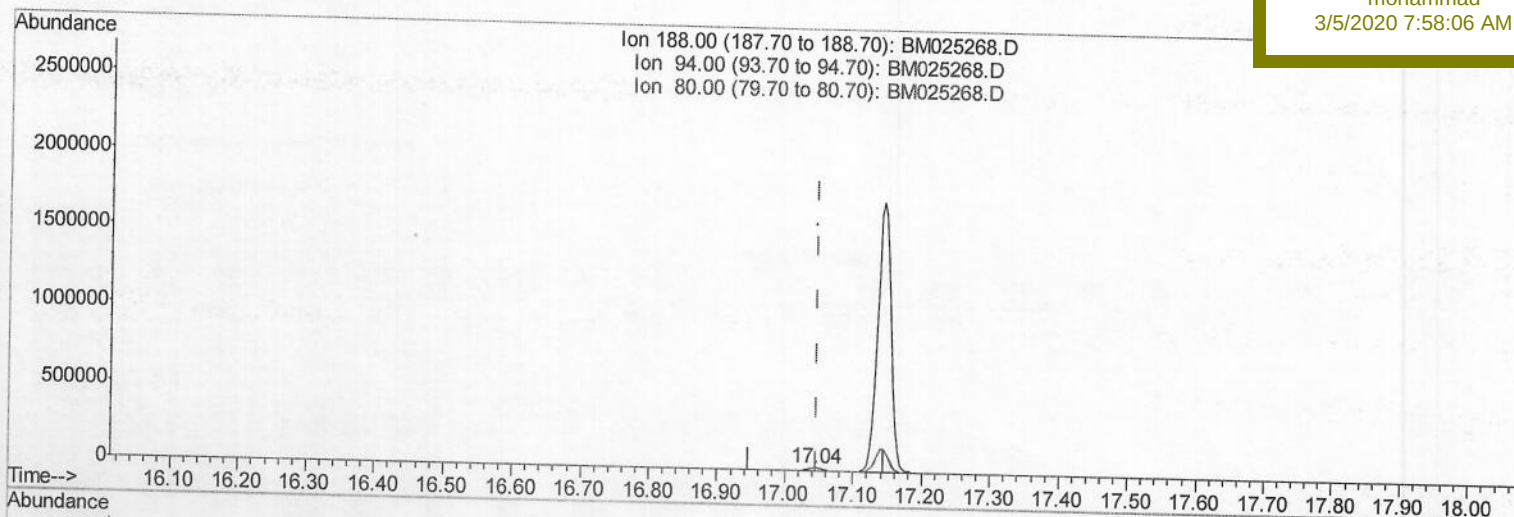

(10) Phenanthrene-d10 (I)

17.043min (-0.004) 0.40ng/ul m>Ju 03/05/20

response 29194

Ion	Exp%	Act%
188.00	100	100
94.00	26.60	7.90#
80.00	22.60	9.54#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030320\
Data File : BM025268.D
Acq On : 05 Mar 2020 02:00
Operator : CG/JU
Sample : L1708-04
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0CE0

Manual Integrations
APPROVED

mohammad
3/5/2020 7:58:06 AM

Quant Time: Mar 05 04:26:48 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 05 00:55:12 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.68	152	3829	0.40	ng/ul	0.00
2) Naphthalene-d8	10.44	136	16638	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.30	164	12460	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.04	188	29194m	0.40	ng/ul	0.00
16) Chrysene-d12	21.23	240	29251	0.40	ng/ul	0.00
20) Perylene-d12	23.42	264	27756	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.04	152	9831	0.32	ng/ul	0.00
14) Fluoranthene-d10	19.07	212	32258	0.34	ng/ul	0.00

Target Compounds Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

50
03/05/20