

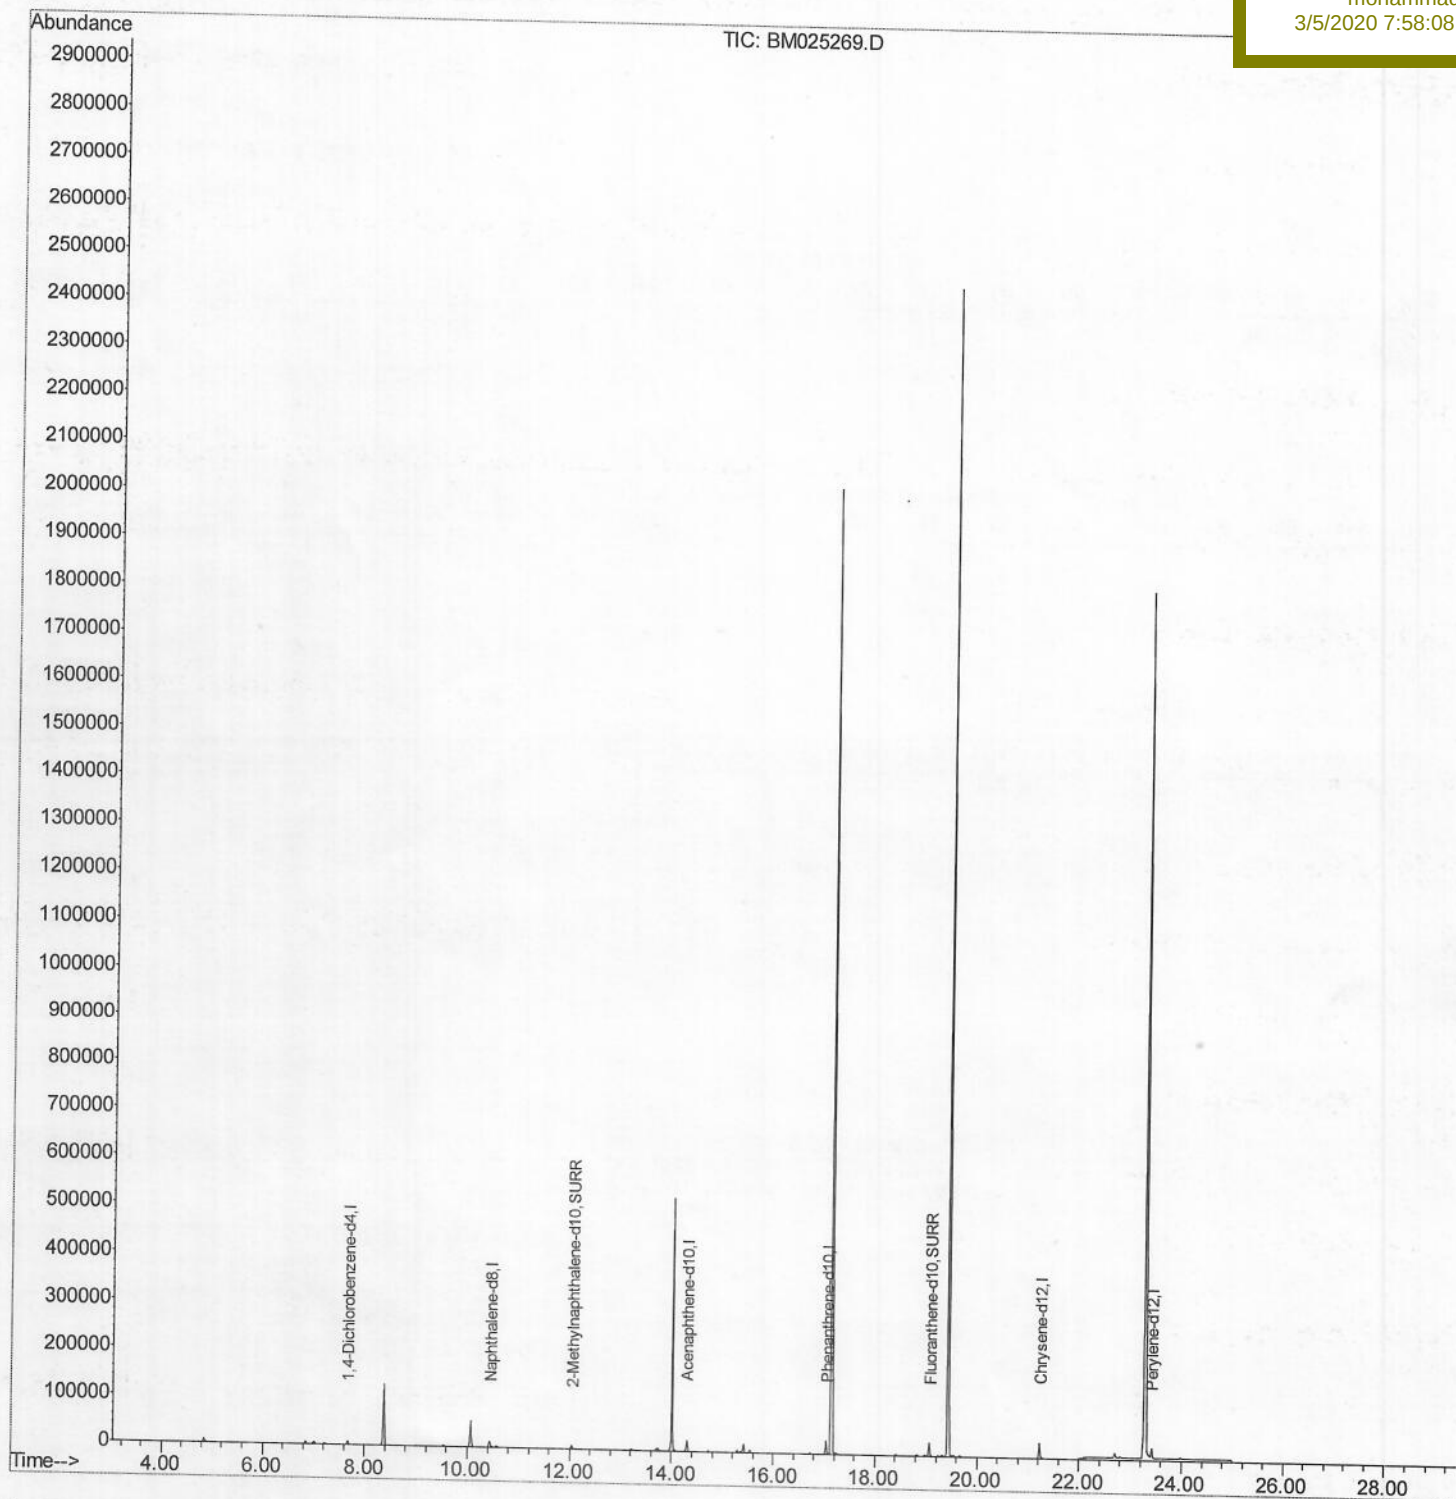
Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030320\
Data File : BM025269.D
Acq On : 05 Mar 2020 02:36
Operator : CG/JU
Sample : L1708-03
Misc :
ALS Vial : 65 Sample Multiplier: 1

Quant Time: Mar 05 04:28:06 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 05 00:55:12 2020
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
C0CA0

Manual Integrations
APPROVED

mohammad
3/5/2020 7:58:08 AM



Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030320\
Data File : BM025269.D
Acq On : 05 Mar 2020 02:36
Operator : CG/JU
Sample : L1708-03
Misc :
ALS Vial : 65 Sample Multiplier: 1

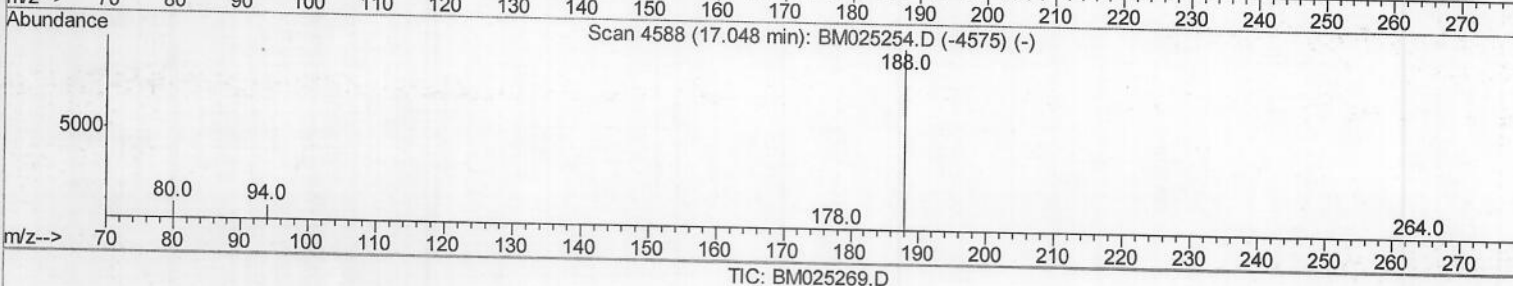
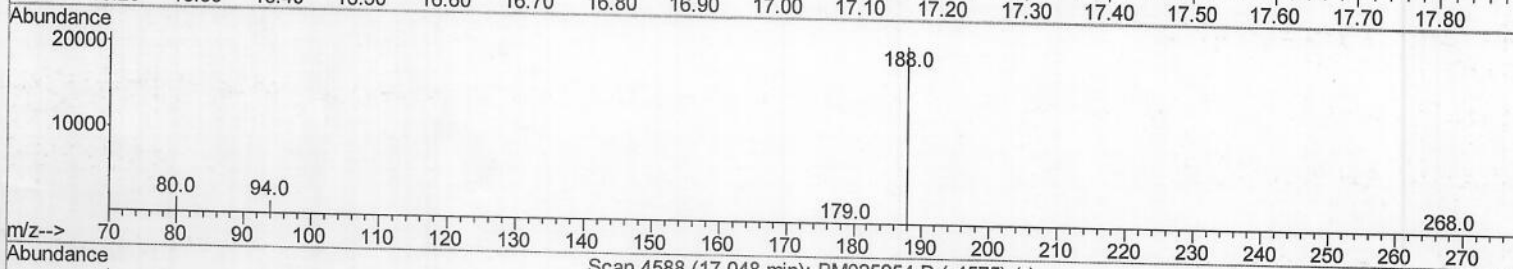
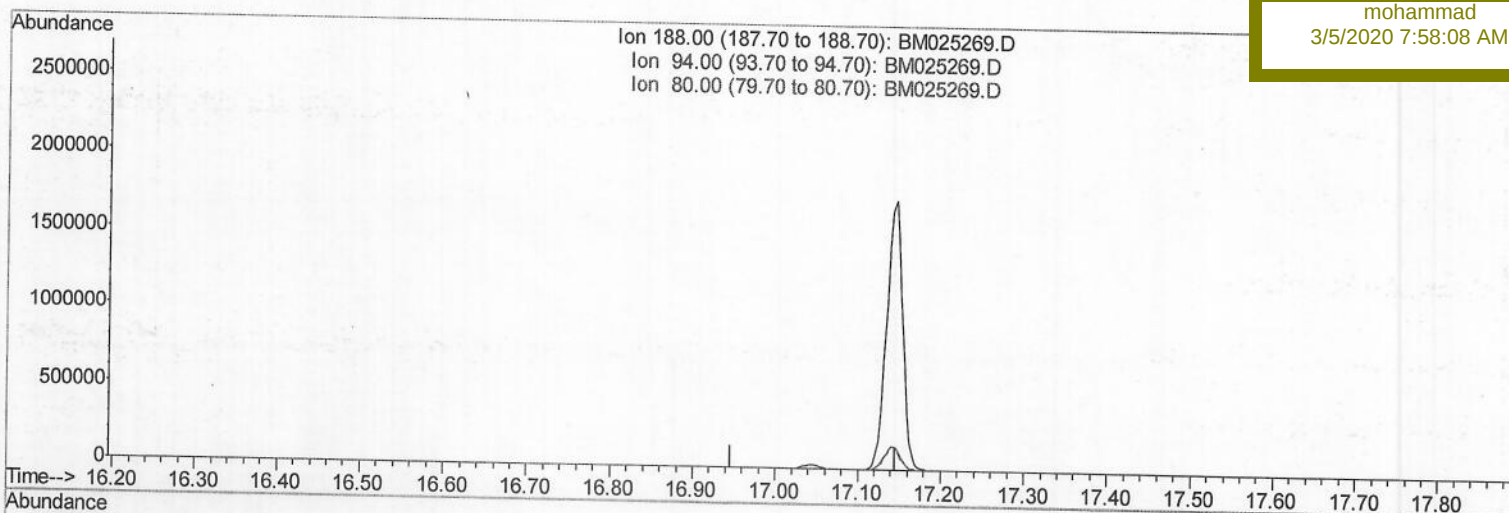
Quant Time: Mar 05 04:27:12 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 05 00:55:12 2020
Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :

C0CA0

Manual Integrations
APPROVEDmohammad
3/5/2020 7:58:08 AM

(10) Phenanthrene-d10 (I)

17.046min (-17.046) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	26.60	0.00#
80.00	22.60	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030320\

Data File : BM025269.D

Acq On : 05 Mar 2020 02:36

Operator : CG/JU

Sample : L1708-03

Misc :

ALS Vial : 65 Sample Multiplier: 1

Quant Time: Mar 05 04:27:12 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Thu Mar 05 00:55:12 2020

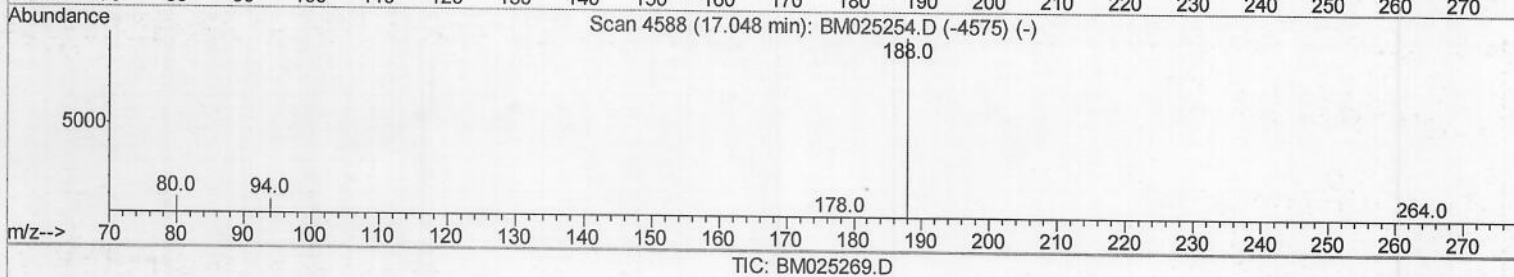
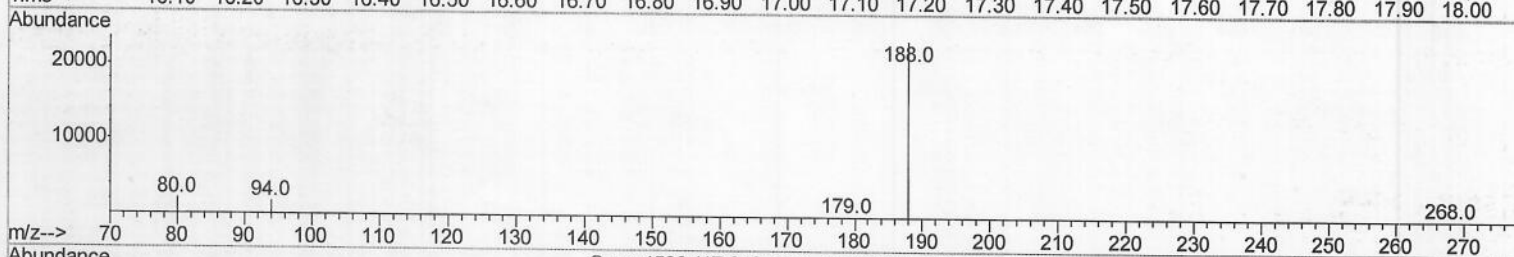
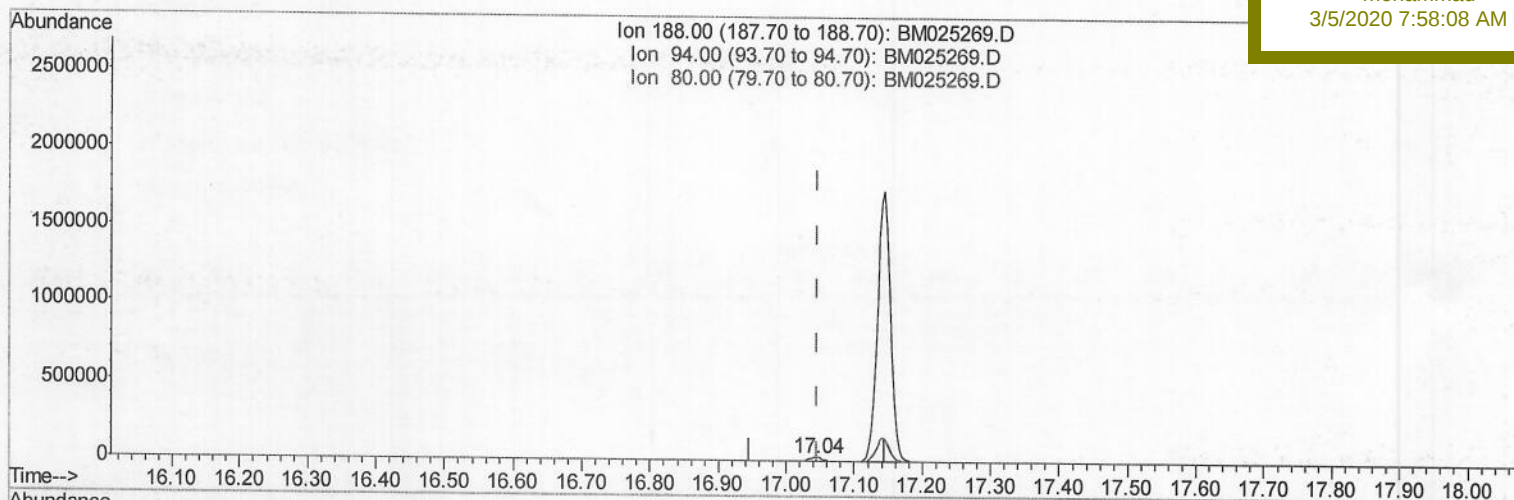
Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :

C0CA0

Manual Integrations
APPROVEDmohammad
3/5/2020 7:58:08 AM

(10) Phenanthrene-d10 (I)

17.044min (-0.002) 0.40ng/ul m > Ju 03105/20

response 30795

Ion	Exp%	Act%
188.00	100	100
94.00	26.60	7.60#
80.00	22.60	9.04#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030320\
Data File : BM025269.D
Acq On : 05 Mar 2020 02:36
Operator : CG/JU
Sample : L1708-03
Misc :
ALS Vial : 65 Sample Multiplier: 1

Quant Time: Mar 05 04:28:06 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 05 00:55:12 2020
Response via : Initial Calibration

Instrument :
BNA_M
Client Sampled :
C0CA0

Manual Integrations
APPROVED

mohammad
3/5/2020 7:58:08 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.68	152	3888	0.40	ng/ul	0.00
2) Naphthalene-d8	10.44	136	17176	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.30	164	12853	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.04	188	30795m)	0.40	ng/ul	0.00
16) Chrysene-d12	21.23	240	29054	0.40	ng/ul	0.00
20) Perylene-d12	23.42	264	26528	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.04	152	9033	0.28	ng/ul	0.00
14) Fluoranthene-d10	19.07	212	30517	0.30	ng/ul	0.00

Target Compounds	Ovalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed