


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM030320\
Data File : BM025282.D
Acq On : 05 Mar 2020 11:01
Operator : CG/JU
Sample : L1543-02
Misc :
ALS Vial : 78 Sample Multiplier: 1

Quant Time: Mar 05 14:20:44 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 04 08:02:03 2020
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
DBD58

Manual Integrations
APPROVED

mohammad
3/5/2020 3:32:14 PM

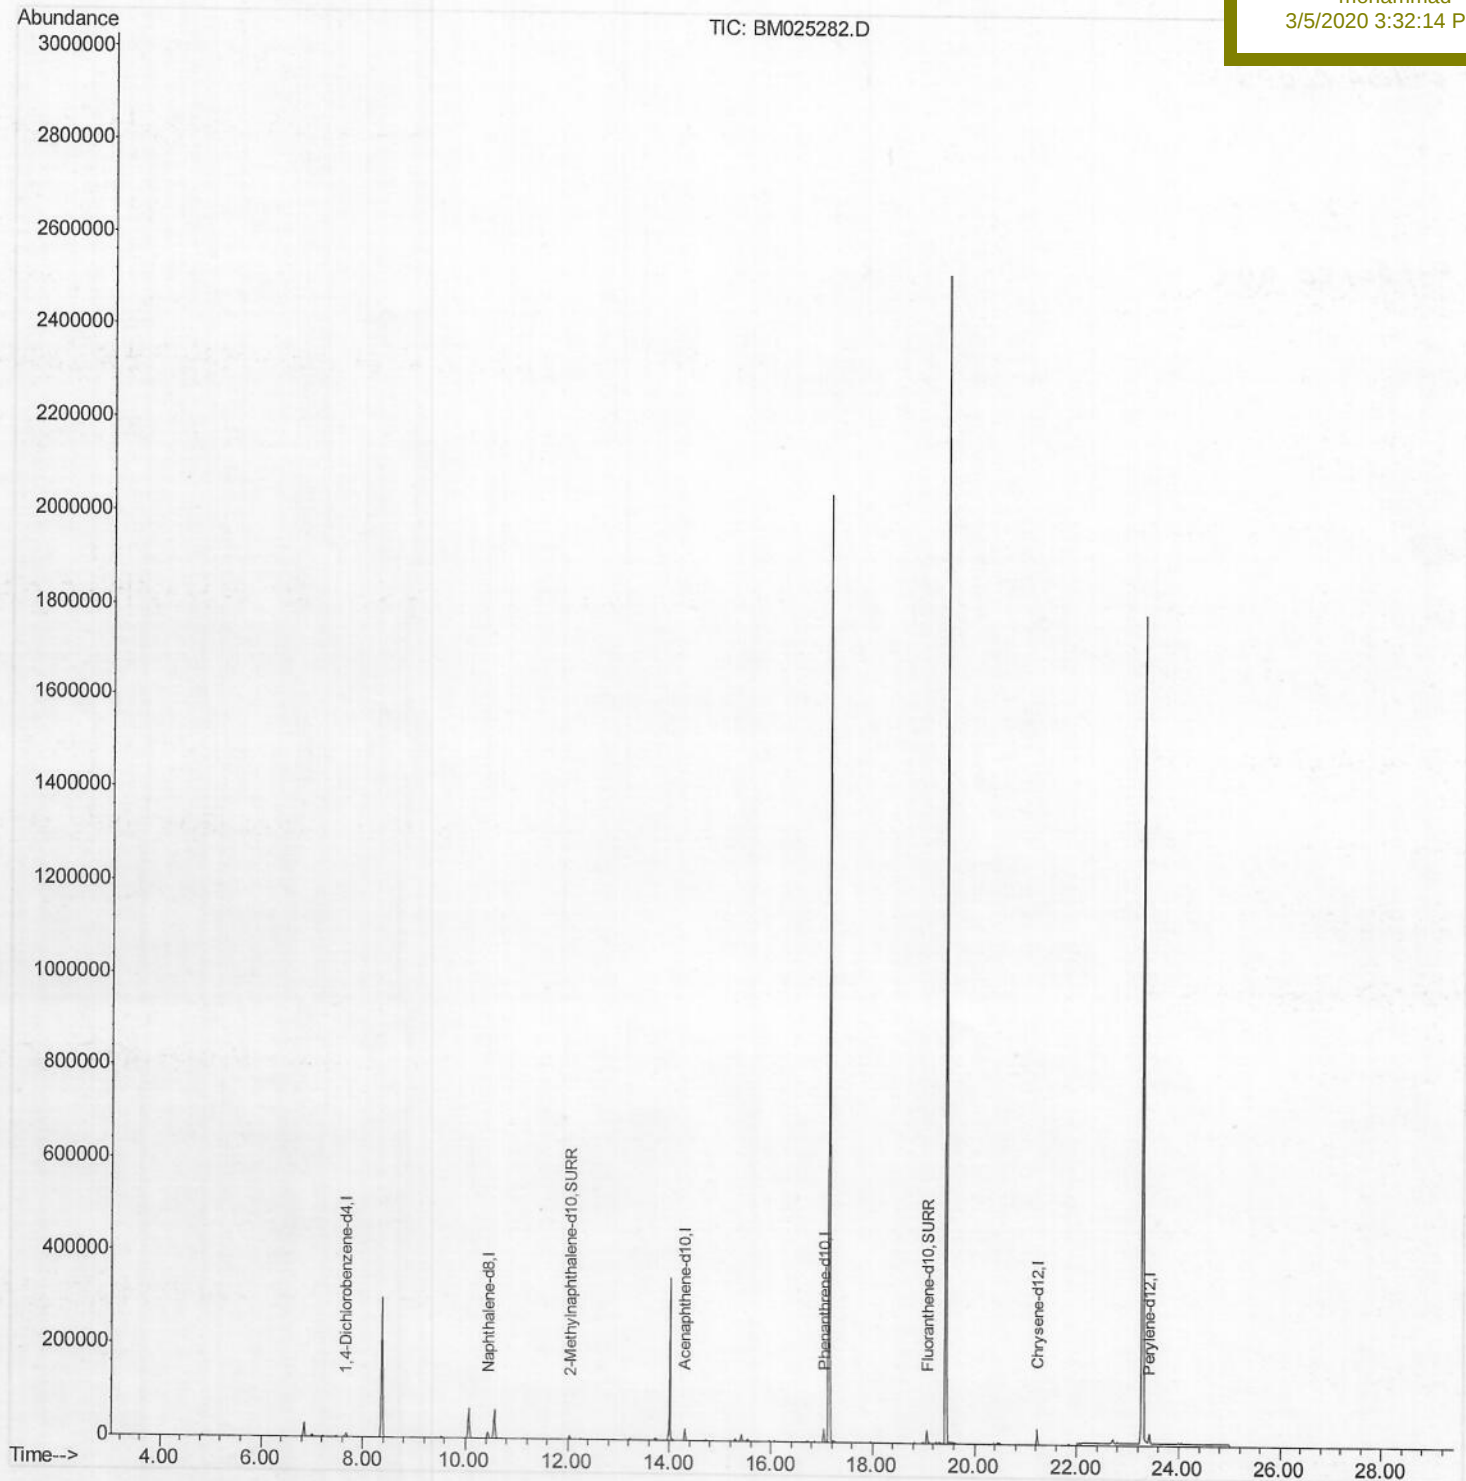

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM030320\
 Data File : BM025282.D
 Acq On : 05 Mar 2020 11:01
 Operator : CG/JU
 Sample : L1543-02
 Misc :
 ALS Vial : 78 Sample Multiplier: 1

Quant Time: Mar 05 14:19:51 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 04 08:02:03 2020
 Response via : Initial Calibration

Instrument :
 BNA_M
ClientSampleId :
 DBD58

Manual Integrations
APPROVED

mohammad
 3/5/2020 3:32:14 PM

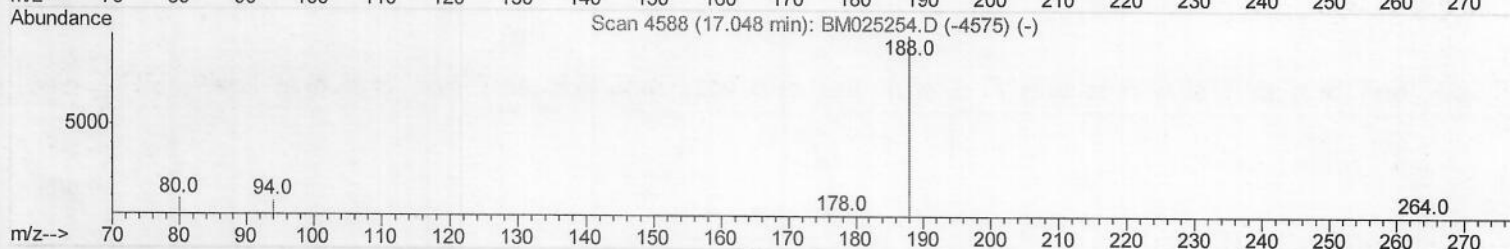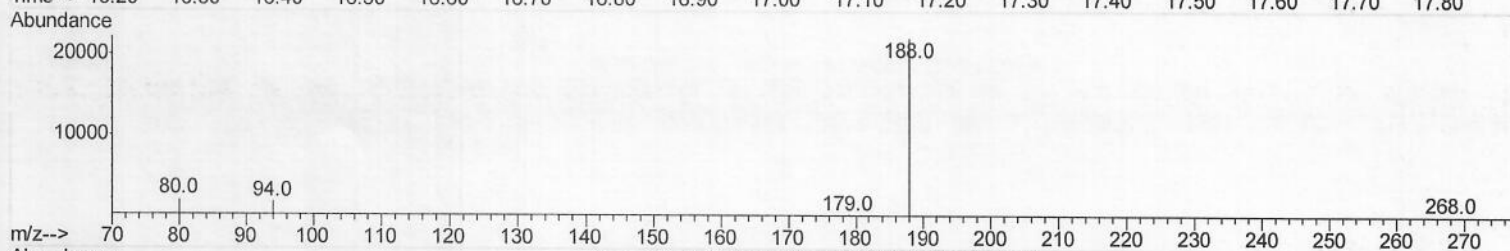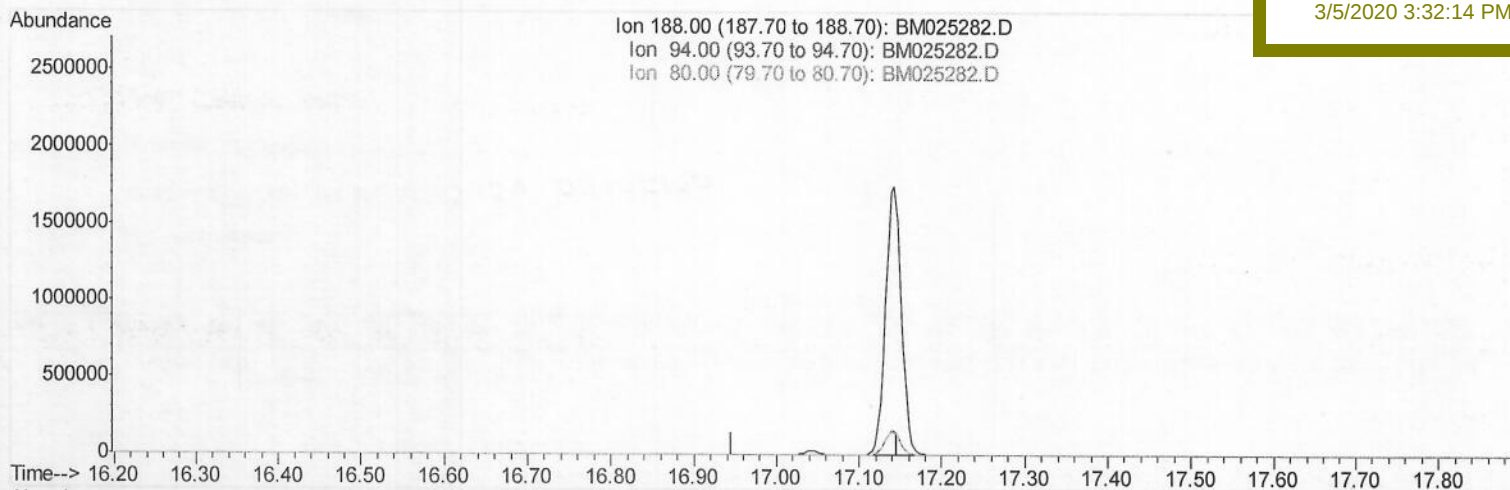

TIC: BM025282.D

(10) Phenanthrene-d10 (I)

17.046min (-17.046) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	26.60	0.00#
80.00	22.60	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM030320\

Data File : BM025282.D

Acq On : 05 Mar 2020 11:01

Operator : CG/JU

Sample : L1543-02

Misc :

ALS Vial : 78 Sample Multiplier: 1

Quant Time: Mar 05 14:19:51 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Wed Mar 04 08:02:03 2020




Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :

DBD58

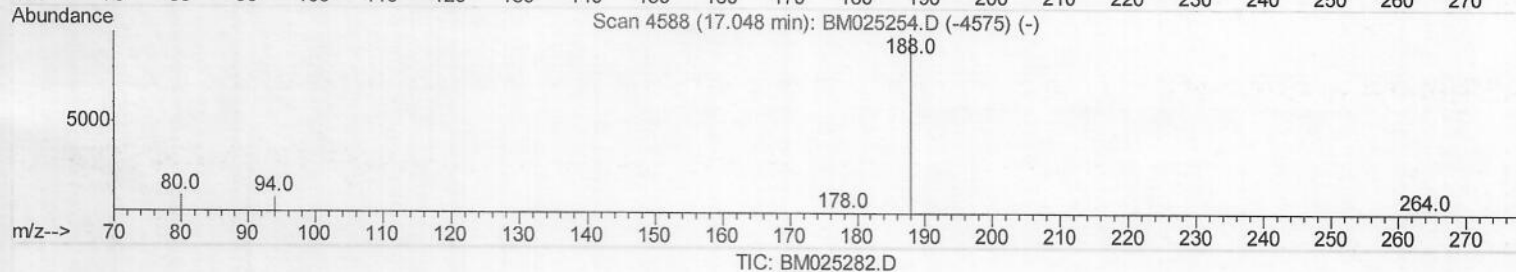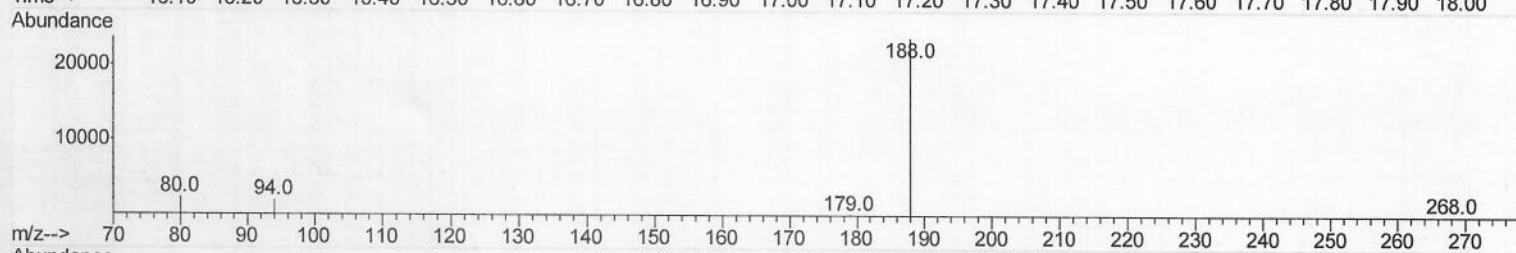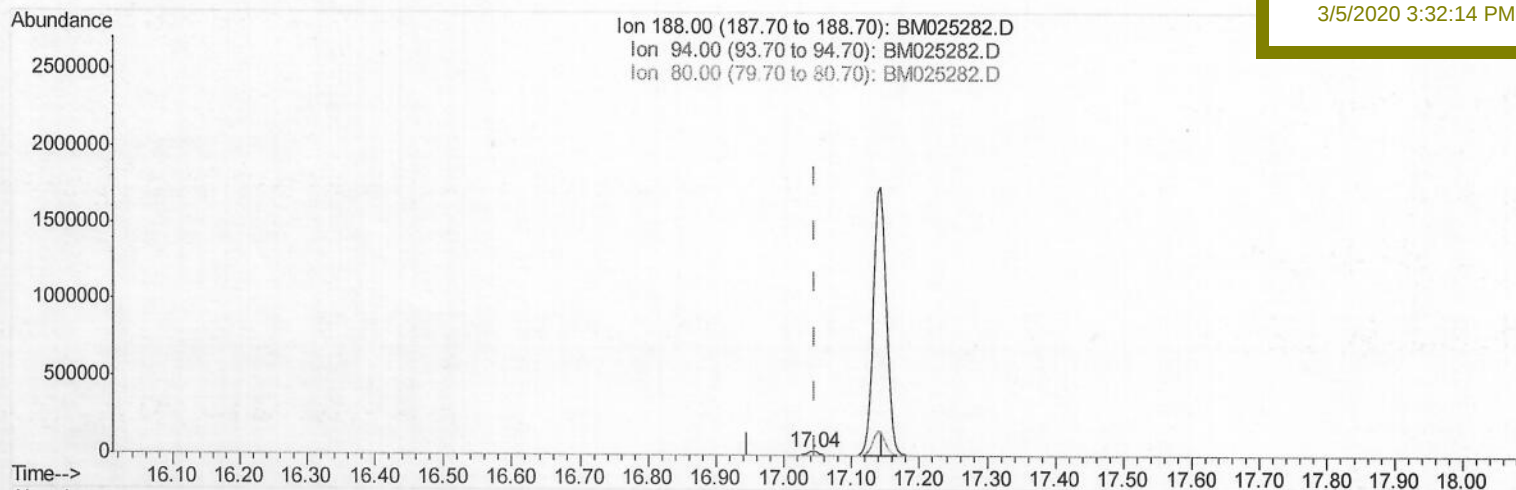Manual Integrations
APPROVEDmohammad
3/5/2020 3:32:14 PM

(10) Phenanthrene-d10 (I)

17.043min (-0.003) 0.40ng/ul m>JU 03/06/20

response 32104

Ion	Exp%	Act%
188.00	100	100
94.00	26.60	8.31#
80.00	22.60	9.69#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM030320\
 Data File : BM025282.D
 Acq On : 05 Mar 2020 11:01
 Operator : CG/JU
 Sample : L1543-02
 Misc :
 ALS Vial : 78 Sample Multiplier: 1

Quant Time: Mar 05 14:20:44 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 04 08:02:03 2020
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 DBD58

Manual Integrations
 APPROVED

mohammad
 3/5/2020 3:32:14 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.67	152	4029	0.40	ng/ul	0.00
2) Naphthalene-d8	10.44	136	17636	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.30	164	13311	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.04	188	32104m	0.40	ng/ul	0.00
16) Chrysene-d12	21.23	240	30071	0.40	ng/ul	0.00
20) Perylene-d12	23.42	264	27364	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.04	152	10520	0.32	ng/ul	0.00
14) Fluoranthene-d10	19.07	212	30694	0.29	ng/ul	0.00

Target Compounds Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

JU 03/06/20