

Quantitation Report (QT Reviewed)


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030320\
 Data File : BM025294.D
 Acq On : 05 Mar 2020 18:56
 Operator : CG/JU
 Sample : L1543-14
 Misc :
 ALS Vial : 90 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBD96

Manual Integrations
 APPROVED

mohammad
 3/6/2020 10:15:01 PM

Quant Time: Mar 06 03:00:24 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 04 08:02:03 2020
 Response via : Initial Calibration

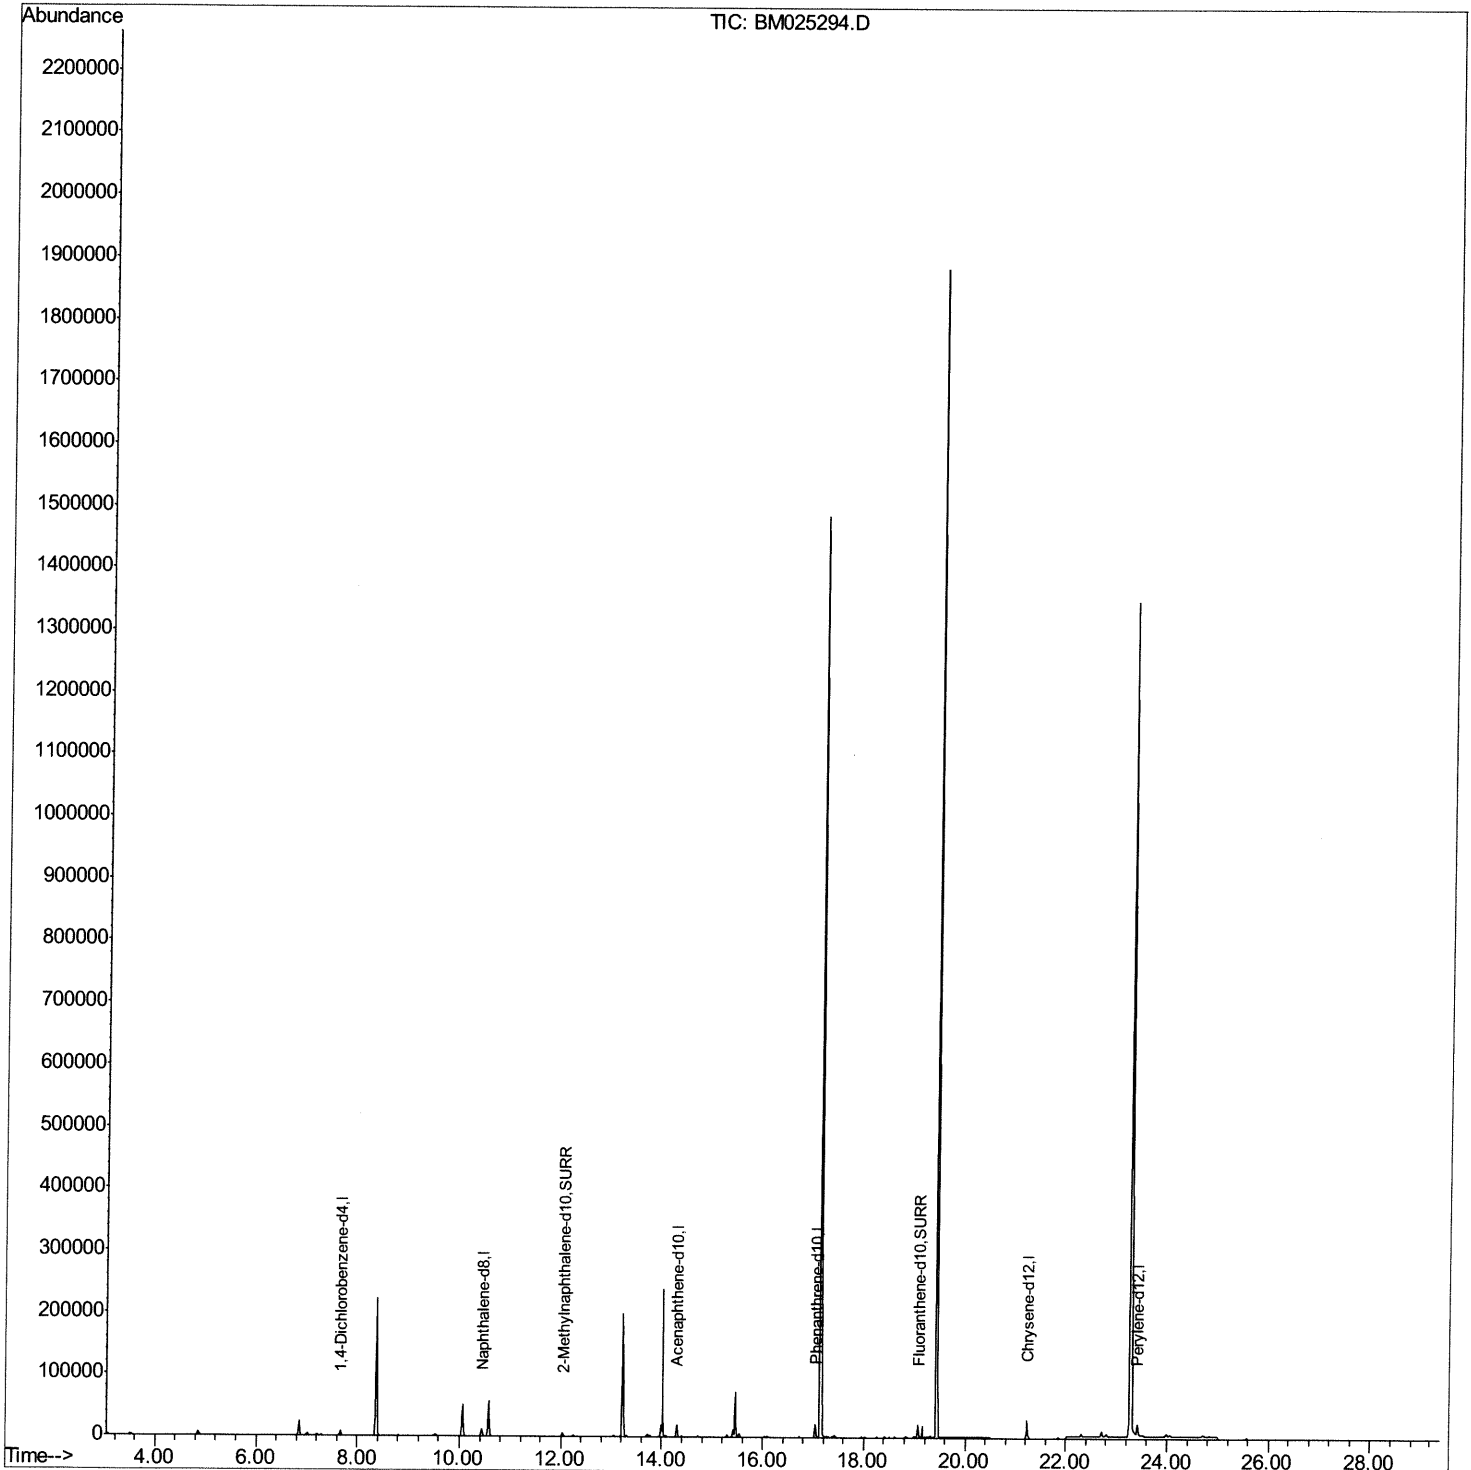

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030320\
 Data File : BM025294.D
 Acq On : 05 Mar 2020 18:56
 Operator : CG/JU
 Sample : L1543-14
 Misc :
 ALS Vial : 90 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBD96

Manual Integrations
 APPROVED

mohammad
 3/6/2020 10:15:01 PM

Quant Time: Mar 06 02:45:46 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 04 08:02:03 2020
 Response via : Initial Calibration

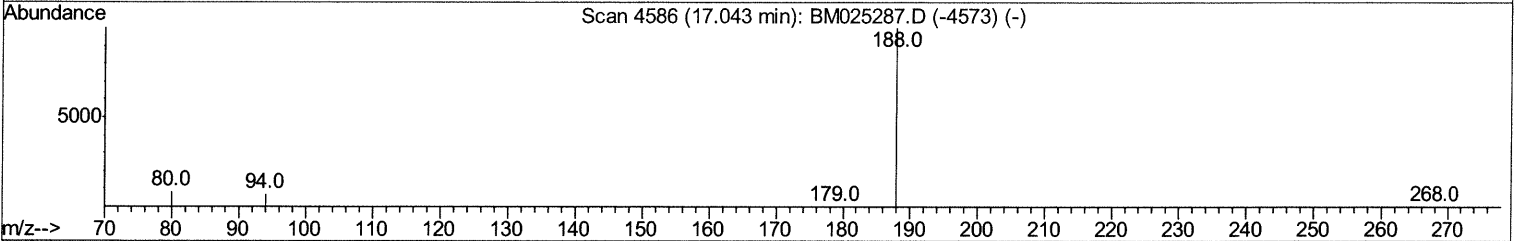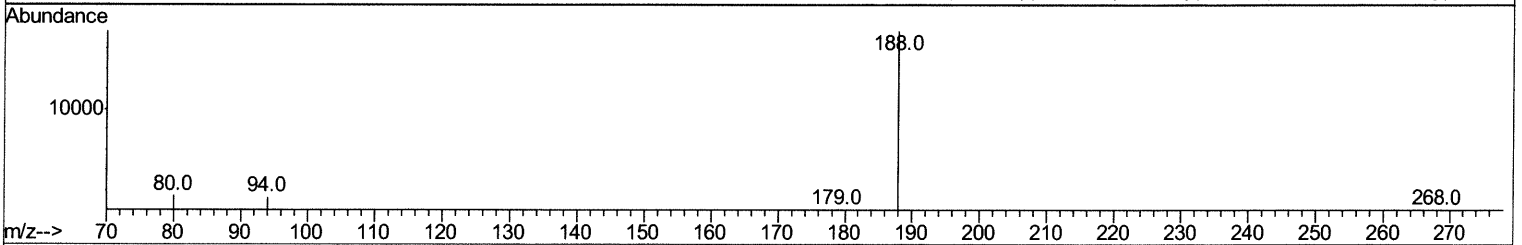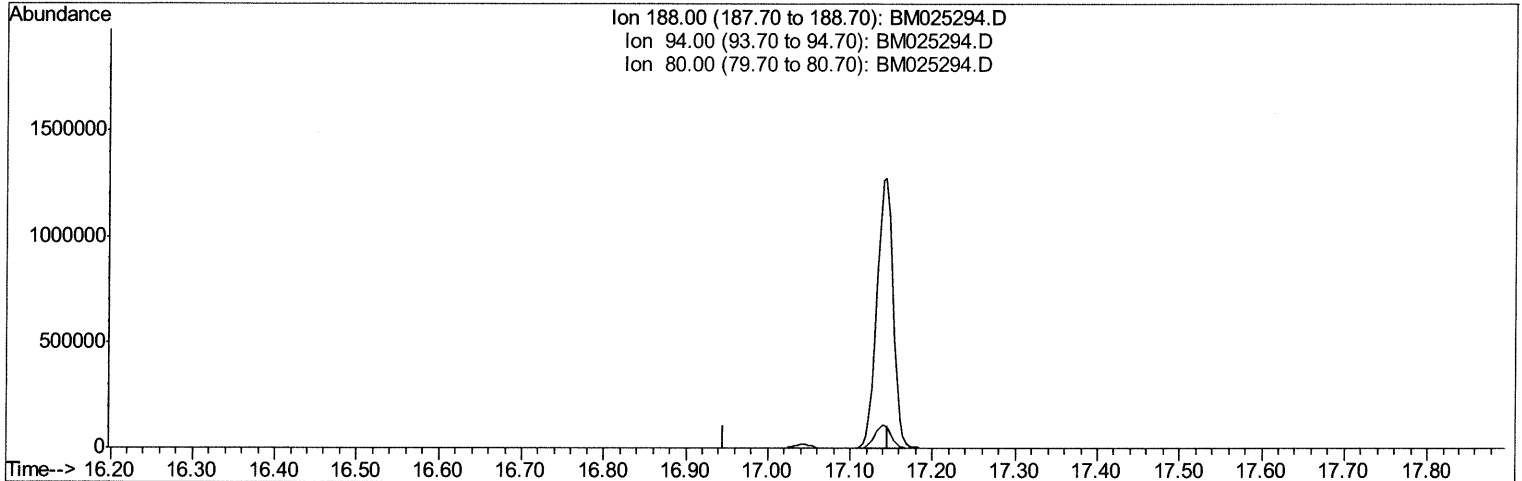

TIC: BM025294.D

(10) Phenanthrene-d10 (I)
 17.046min (-17.046) 0.00ng/ul
 response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	26.60	0.00#
80.00	22.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030320\
 Data File : BM025294.D
 Acq On : 05 Mar 2020 18:56
 Operator : CG/JU
 Sample : L1543-14
 Misc :
 ALS Vial : 90 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBD96

Manual Integrations
 APPROVED

mohammad
 3/6/2020 10:15:01 PM

Quant Time: Mar 06 02:45:46 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 04 08:02:03 2020
 Response via : Initial Calibration

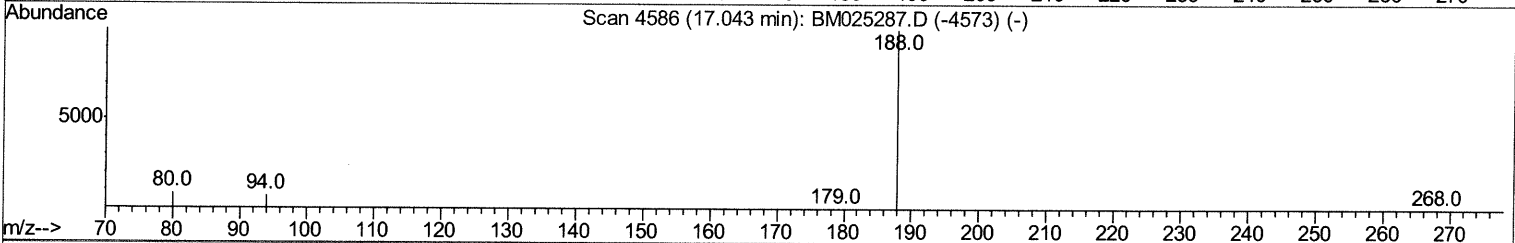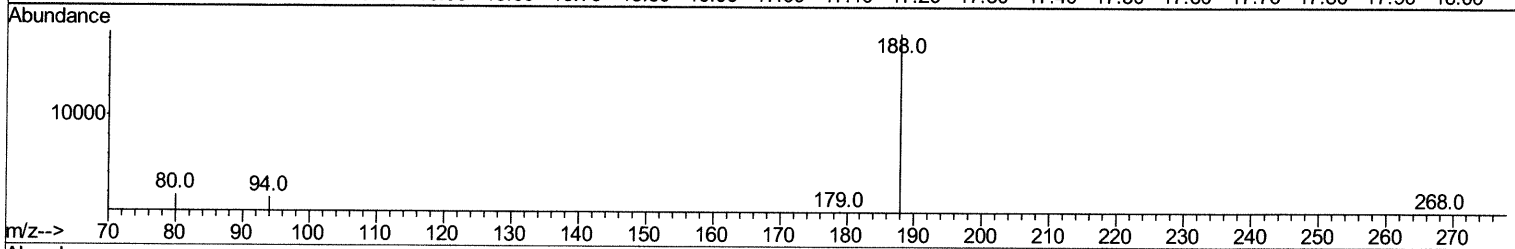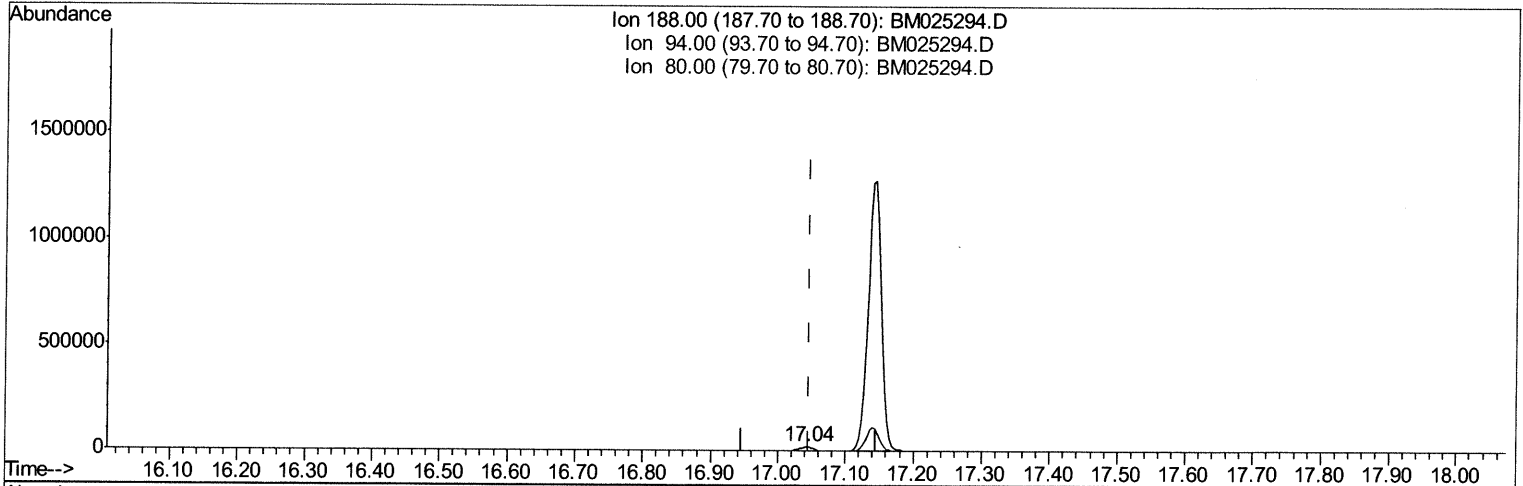

TIC: BM025294.D

(10) Phenanthrene-d10 (I)

17.043min (-0.003) 0.40ng/ul m 2003/06/20

response 25905

Ion	Exp%	Act%
188.00	100	100
94.00	26.60	7.86#
80.00	22.60	9.24#
0.00	0.00	0.00

Quantitation Report (QT Reviewed)

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030320\
Data File : BM025294.D
Acq On : 05 Mar 2020 18:56
Operator : CG/JU
Sample : L1543-14
Misc :
ALS Vial : 90 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBD96

Manual Integrations
APPROVED

mohammad
3/6/2020 10:15:01 PM

Quant Time: Mar 06 03:00:24 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 04 08:02:03 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.67	152	3407	0.40	ng/ul	0.00
2) Naphthalene-d8	10.44	136	14787	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.30	164	10920	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.04	188	25905m>	0.40	ng/ul	> 0.00
16) Chrysene-d12	21.23	240	25024	0.40	ng/ul	0.00
20) Perylene-d12	23.42	264	22861	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.04	152	7990	0.29	ng/ul	0.00
14) Fluoranthene-d10	19.07	212	23056	0.27	ng/ul	0.00

Target Compounds Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Tu 03/06/20