

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030320\
 Data File : BM025266.D
 Acq On : 05 Mar 2020 00:48
 Operator : CG/JU
 Sample : L1708-05
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0CE2

Manual Integrations
 APPROVED

mohammad
 3/5/2020 7:58:00 AM

Quant Time: Mar 05 01:31:44 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 05 00:55:12 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.68	152	4052	0.40	ng/ul	0.00
2) Naphthalene-d8	10.44	136	17401	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.30	164	13018	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.04	188	29776m	0.40	ng/ul	0.00
16) Chrysene-d12	21.23	240	25000	0.40	ng/ul	0.00
20) Perylene-d12	23.42	264	22872	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.04	152	10364	0.32	ng/ul	0.00
14) Fluoranthene-d10	19.07	212	30215	0.31	ng/ul	0.00
Target Compounds						
3) Naphthalene	10.49	128	1069	0.020	ng/ul	Ovalue 97

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030320\
Data File : BM025266.D
Acq On : 05 Mar 2020 00:48
Operator : CG/JU
Sample : L1708-05
Misc :
ALS Vial : 62 Sample Multiplier: 1




Instrument :
BNA_M
ClientSampleId :
C0CE2

Manual Integrations
APPROVED

mohammad
3/5/2020 7:58:00 AM

Quant Time: Mar 05 01:31:44 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 05 00:55:12 2020
Response via : Initial Calibration

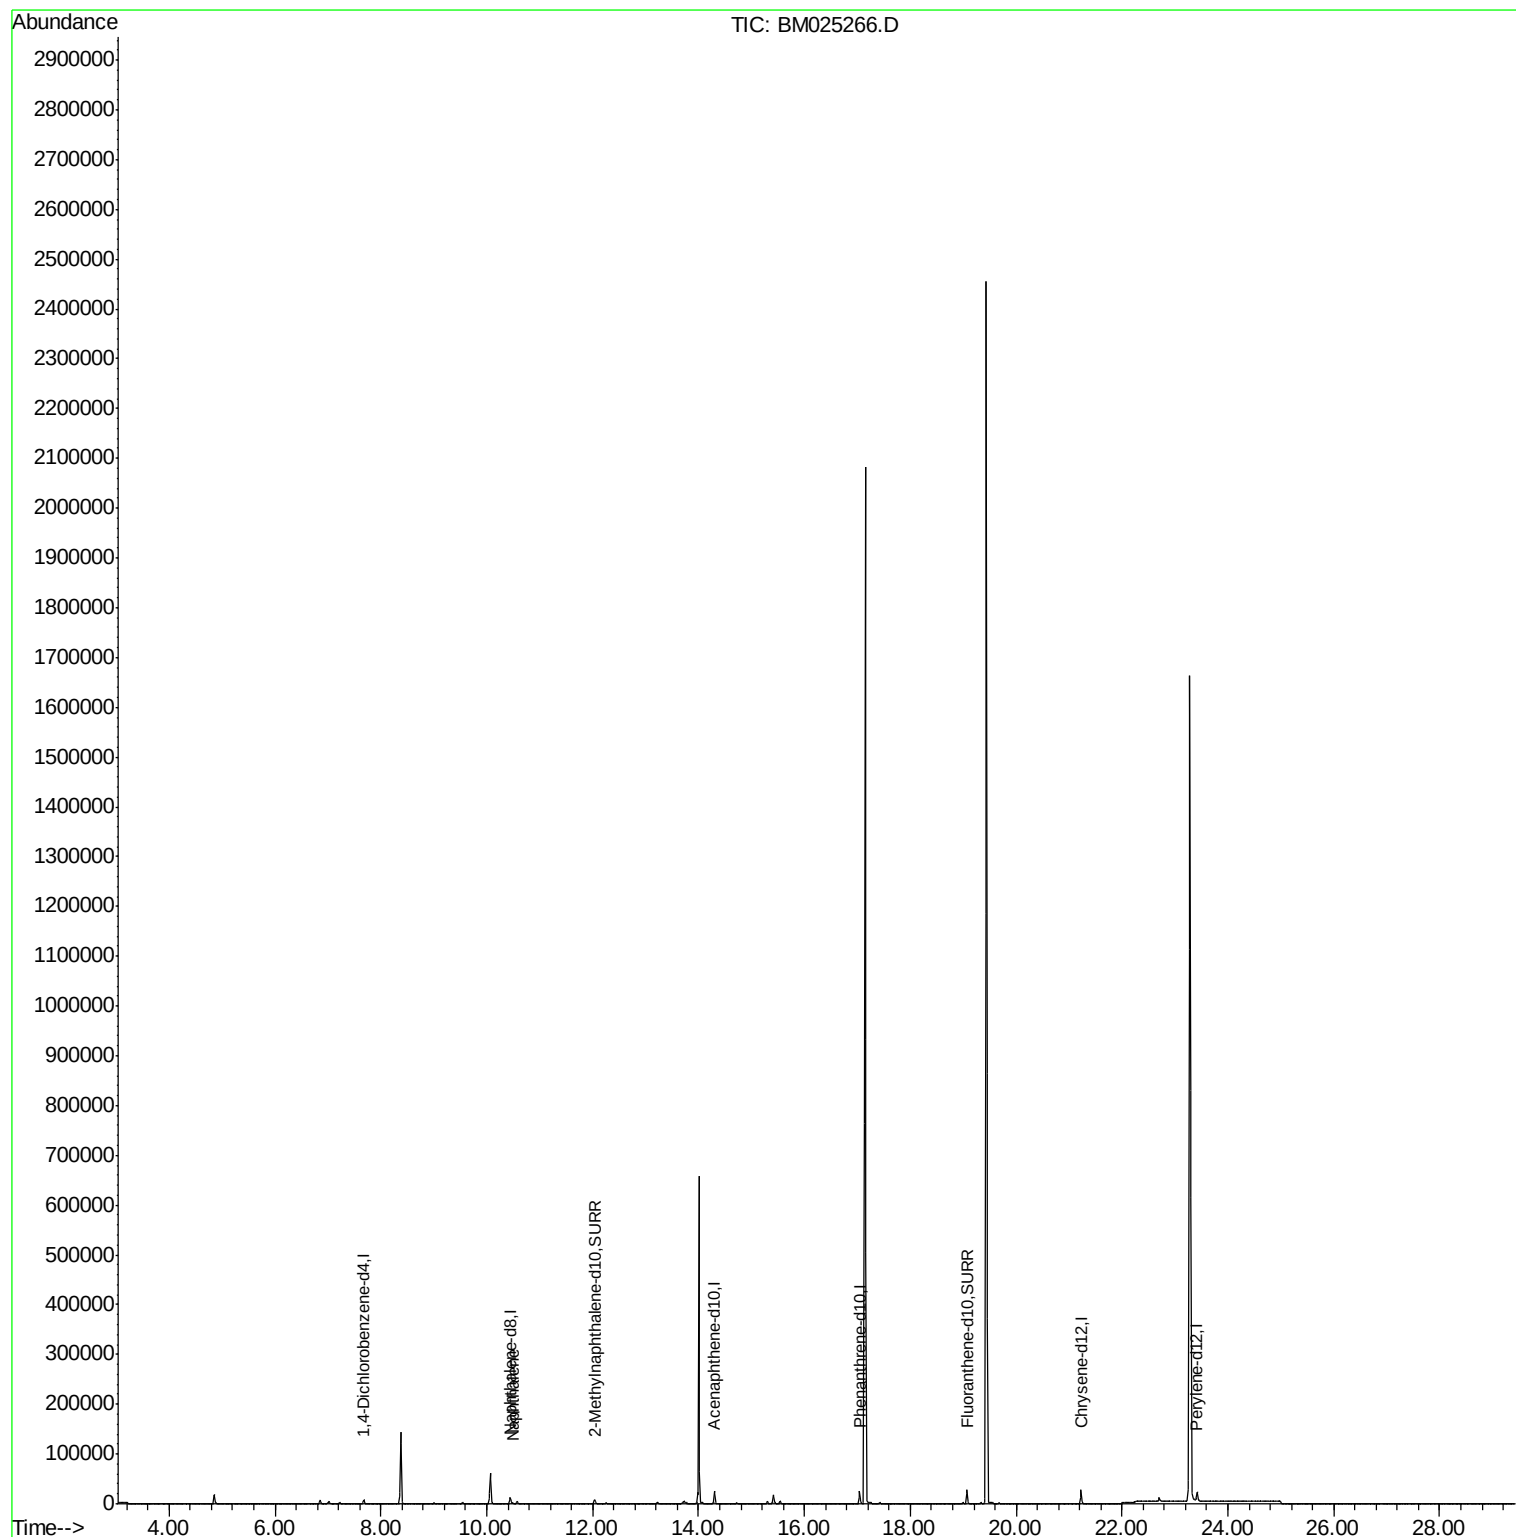

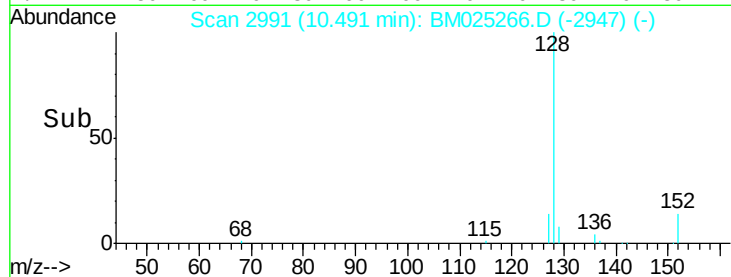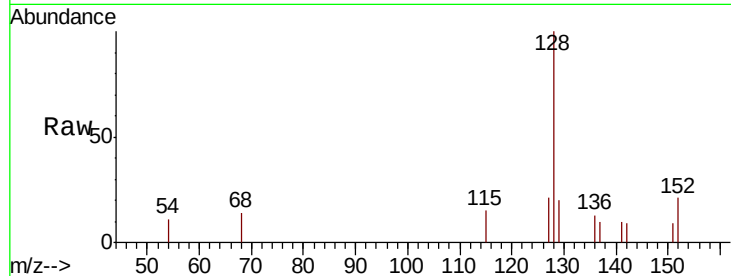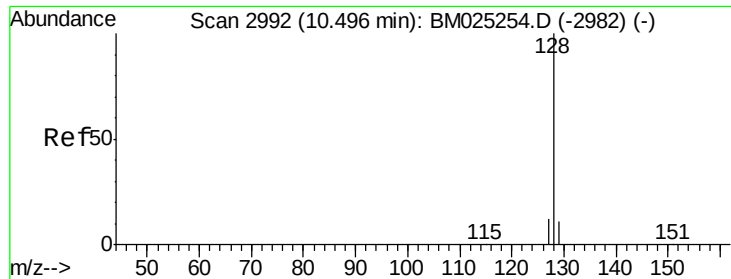

#3

Naphthalene

Concen: 0.020 ng/ul

RT: 10.49 min Scan# 2991

Delta R.T. -0.00 min

Lab File: BM025266.D

Acq: 05 Mar 2020 00:48

Tot Ion:	128	Resp:	1069
Ion Ratio	Lower	Upper	
128	100		
129	19.7	17.0	25.6
127	21.0	15.7	23.5

Instrument :

BNA_M

ClientSampleId :

C0CE2

Manual Integrations
APPROVED

mohammad
3/5/2020 7:58:00 AM

