

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030320\
 Data File : BM025311.D
 Acq On : 06 Mar 2020 10:59
 Operator : CG/JU
 Sample : L1568-07
 Misc :
 ALS Vial : 109 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBDB0

Quant Time: Mar 06 11:39:46 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 04 08:02:03 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.67	152	4121	0.40	ng/ul	0.00
2) Naphthalene-d8	10.44	136	17338	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.30	164	12257	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.04	188	29803	0.40	ng/ul	0.00
16) Chrysene-d12	21.23	240	26356	0.40	ng/ul	0.00
20) Perylene-d12	23.42	264	23795	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.04	152	4511	0.14	ng/ul	0.00
14) Fluoranthene-d10	19.07	212	12656	0.13	ng/ul	0.00
Target Compounds						
12) Phenanthrene	17.08	178	1928	0.020	ng/ul	Ovalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030320\
Data File : BM025311.D
Acq On : 06 Mar 2020 10:59
Operator : CG/JU
Sample : L1568-07
Misc :
ALS Vial : 109 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBDB0

Quant Time: Mar 06 11:39:46 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 04 08:02:03 2020
Response via : Initial Calibration

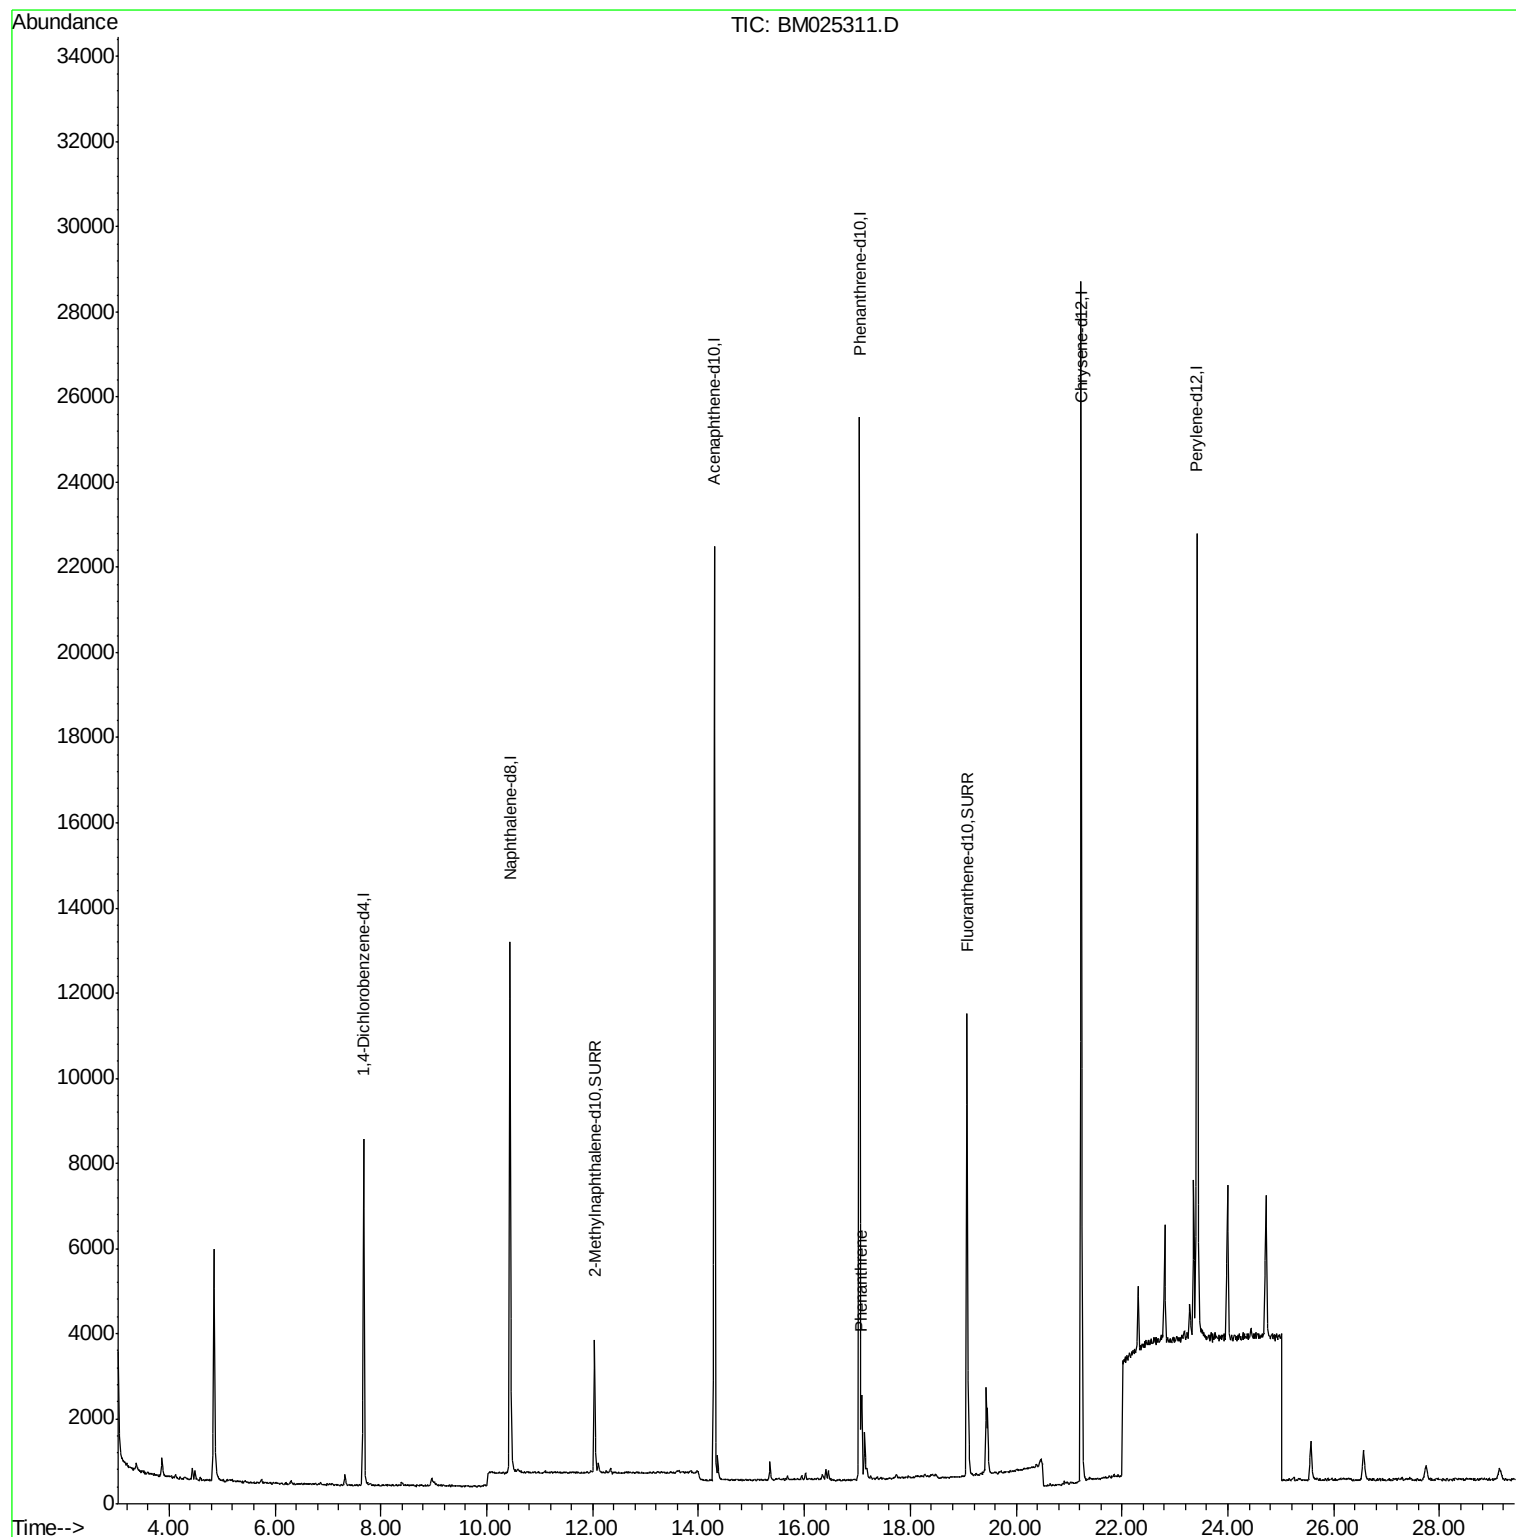

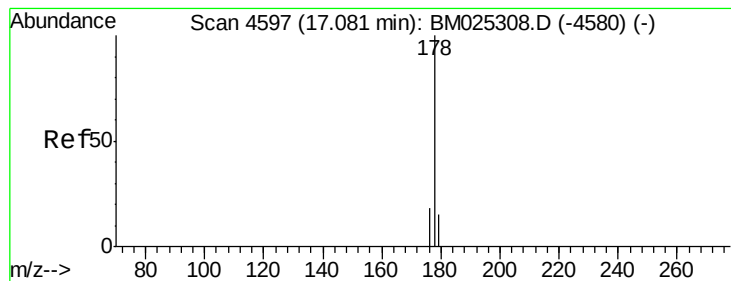

#12

Phenanthrene

Concen: 0.020 ng/ul

RT: 17.08 min Scan# 4597

Delta R.T. -0.01 min

Lab File: BM025311.D


Acq: 06 Mar 2020 10:59

Instrument :

BNA_M

ClientSampleId :

DBDB0

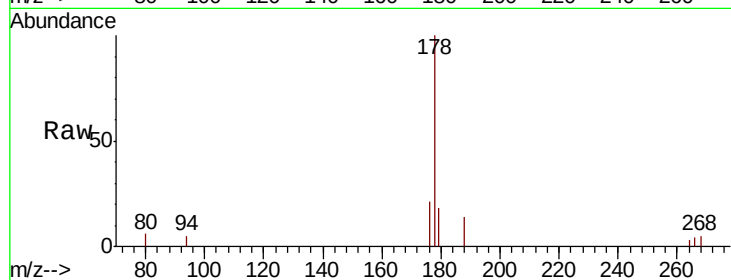

Tot Ion:178 Resp: 1928

Ion Ratio Lower Upper

178 100

179 18.3 14.0 21.0

176 20.6 16.6 24.8

