

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030321\
 Data File : BM028969.D
 Acq On : 03 Mar 2021 10:09
 Operator : CG/JU
 Sample : M1505-05
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM022721MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.140	25	26	28	rVB	224	152	0.12%	0.022%
2	3.170	28	31	33	rBB	203	257	0.20%	0.037%
3	3.187	33	34	36	rBV	174	180	0.14%	0.026%
4	3.317	55	56	59	rBB	195	190	0.15%	0.028%
5	3.352	59	62	63	rBB	189	185	0.14%	0.027%
6	3.423	71	74	75	rBB	205	134	0.10%	0.019%
7	3.470	78	82	83	rBB	157	164	0.13%	0.024%
8	3.887	150	153	154	rBB	409	429	0.34%	0.062%
9	7.763	807	812	822	rBB	48803	75724	59.22%	10.970%
10	10.569	1282	1289	1298	rBB	61841	100936	78.94%	14.623%
11	14.428	1940	1945	1951	rBB	87664	121045	94.67%	17.536%
12	17.175	2406	2412	2418	rBV	95552	127861	100.00%	18.524%
13	17.310	2433	2435	2437	rBB	346	233	0.18%	0.034%
14	17.539	2471	2474	2475	rBB	174	170	0.13%	0.025%
15	17.580	2479	2481	2483	rBV	176	234	0.18%	0.034%
16	17.604	2483	2485	2488	rVB	362	299	0.23%	0.043%
17	17.633	2489	2490	2492	rBV	329	244	0.19%	0.035%
18	17.651	2492	2493	2495	rVB	340	186	0.15%	0.027%
19	17.680	2495	2498	2499	rBV	214	238	0.19%	0.034%
20	17.704	2501	2502	2504	rBB	215	133	0.10%	0.019%
21	17.751	2509	2510	2512	rBV	343	229	0.18%	0.033%
22	17.886	2531	2533	2534	rVB	230	157	0.12%	0.023%
23	17.916	2534	2538	2540	rBV	334	475	0.37%	0.069%
24	17.975	2544	2548	2549	rVV	214	248	0.19%	0.036%
25	17.986	2549	2550	2553	rVV	220	167	0.13%	0.024%
26	18.051	2556	2561	2562	rVV	226	217	0.17%	0.031%
27	18.157	2576	2579	2580	rVB	271	188	0.15%	0.027%
28	18.175	2580	2582	2583	rBV	238	245	0.19%	0.035%
29	18.204	2585	2587	2589	rVV	273	190	0.15%	0.028%
30	18.380	2616	2617	2619	rBV	226	228	0.18%	0.033%
31	18.422	2622	2624	2626	rBV2	241	277	0.22%	0.040%
32	18.457	2628	2630	2632	rVB	233	130	0.10%	0.019%
33	18.498	2635	2637	2640	rBV	299	247	0.19%	0.036%
34	18.598	2650	2654	2655	rBV	185	190	0.15%	0.028%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030321\
 Data File : BM028969.D
 Acq On : 03 Mar 2021 10:09
 Operator : CG/JU
 Sample : M1505-05
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM022721MA.M
 Title : SVOA CALIBRATION

35	18.616	2655	2657	2660	rVV	189	173	0.14%	0.025%
36	18.645	2660	2662	2663	rVB	221	155	0.12%	0.022%
37	18.692	2666	2670	2675	rBV	259	370	0.29%	0.054%
38	18.727	2675	2676	2680	rBV	178	196	0.15%	0.028%
39	18.775	2683	2684	2687	rVB	371	237	0.19%	0.034%
40	18.810	2689	2690	2692	rVB	230	147	0.11%	0.021%
41	18.833	2692	2694	2695	rVB	251	133	0.10%	0.019%
42	18.845	2695	2696	2697	rBV	214	137	0.11%	0.020%
43	18.892	2702	2704	2705	rBV	223	157	0.12%	0.023%
44	18.963	2714	2716	2719	rBV	254	302	0.24%	0.044%
45	18.986	2719	2720	2722	rVB	415	207	0.16%	0.030%
46	19.016	2723	2725	2727	rBV	398	303	0.24%	0.044%
47	19.039	2727	2729	2731	rBV	382	305	0.24%	0.044%
48	19.057	2731	2732	2734	rBV	484	330	0.26%	0.048%
49	19.080	2734	2736	2740	rVB	456	541	0.42%	0.078%
50	19.122	2741	2743	2744	rBV	399	231	0.18%	0.033%
51	19.151	2744	2748	2751	rBV	357	550	0.43%	0.080%
52	19.180	2751	2753	2755	rVB	229	196	0.15%	0.028%
53	19.198	2755	2756	2759	rBV	403	328	0.26%	0.048%
54	19.222	2759	2760	2762	rVB	548	365	0.29%	0.053%
55	19.251	2762	2765	2766	rBV	630	515	0.40%	0.075%
56	19.269	2766	2768	2769	rBV	325	211	0.17%	0.031%
57	19.310	2774	2775	2778	rBV	512	602	0.47%	0.087%
58	19.333	2778	2779	2782	rBV2	351	195	0.15%	0.028%
59	19.398	2786	2790	2791	rBV2	499	699	0.55%	0.101%
60	19.422	2793	2794	2796	rBV2	431	349	0.27%	0.051%
61	19.451	2796	2799	2801	rVB2	695	684	0.53%	0.099%
62	19.469	2801	2802	2803	rBV	480	325	0.25%	0.047%
63	19.574	2819	2820	2821	rBV	246	172	0.13%	0.025%
64	19.645	2831	2832	2834	rBV	432	279	0.22%	0.040%
65	19.710	2841	2843	2845	rBV2	496	567	0.44%	0.082%
66	19.957	2884	2885	2886	rBV2	498	238	0.19%	0.034%
67	20.033	2895	2898	2900	rBV3	546	671	0.52%	0.097%
68	20.080	2904	2906	2907	rVV2	555	318	0.25%	0.046%
69	20.380	2955	2957	2960	rBV3	991	1503	1.18%	0.218%
70	20.592	2992	2993	2995	rBV2	957	575	0.45%	0.083%
71	21.339	3115	3120	3125	rBV	103736	120057	93.90%	17.393%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030321\
Data File : BM028969.D
Acq On : 03 Mar 2021 10:09
Operator : CG/JU
Sample : M1505-05
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SVOC-GPC-BLANK

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM022721MA.M
Title : SVOA CALIBRATION

72	23.533	3487	3493	3500	rVB2	69982	124750	97.57%	18.073%
----	--------	------	------	------	------	-------	--------	--------	---------


Sum of corrected areas: 690255

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030321\
Data File : BM028969.D
Acq On : 03 Mar 2021 10:09
Operator : CG/JU
Sample : M1505-05
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM022721MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

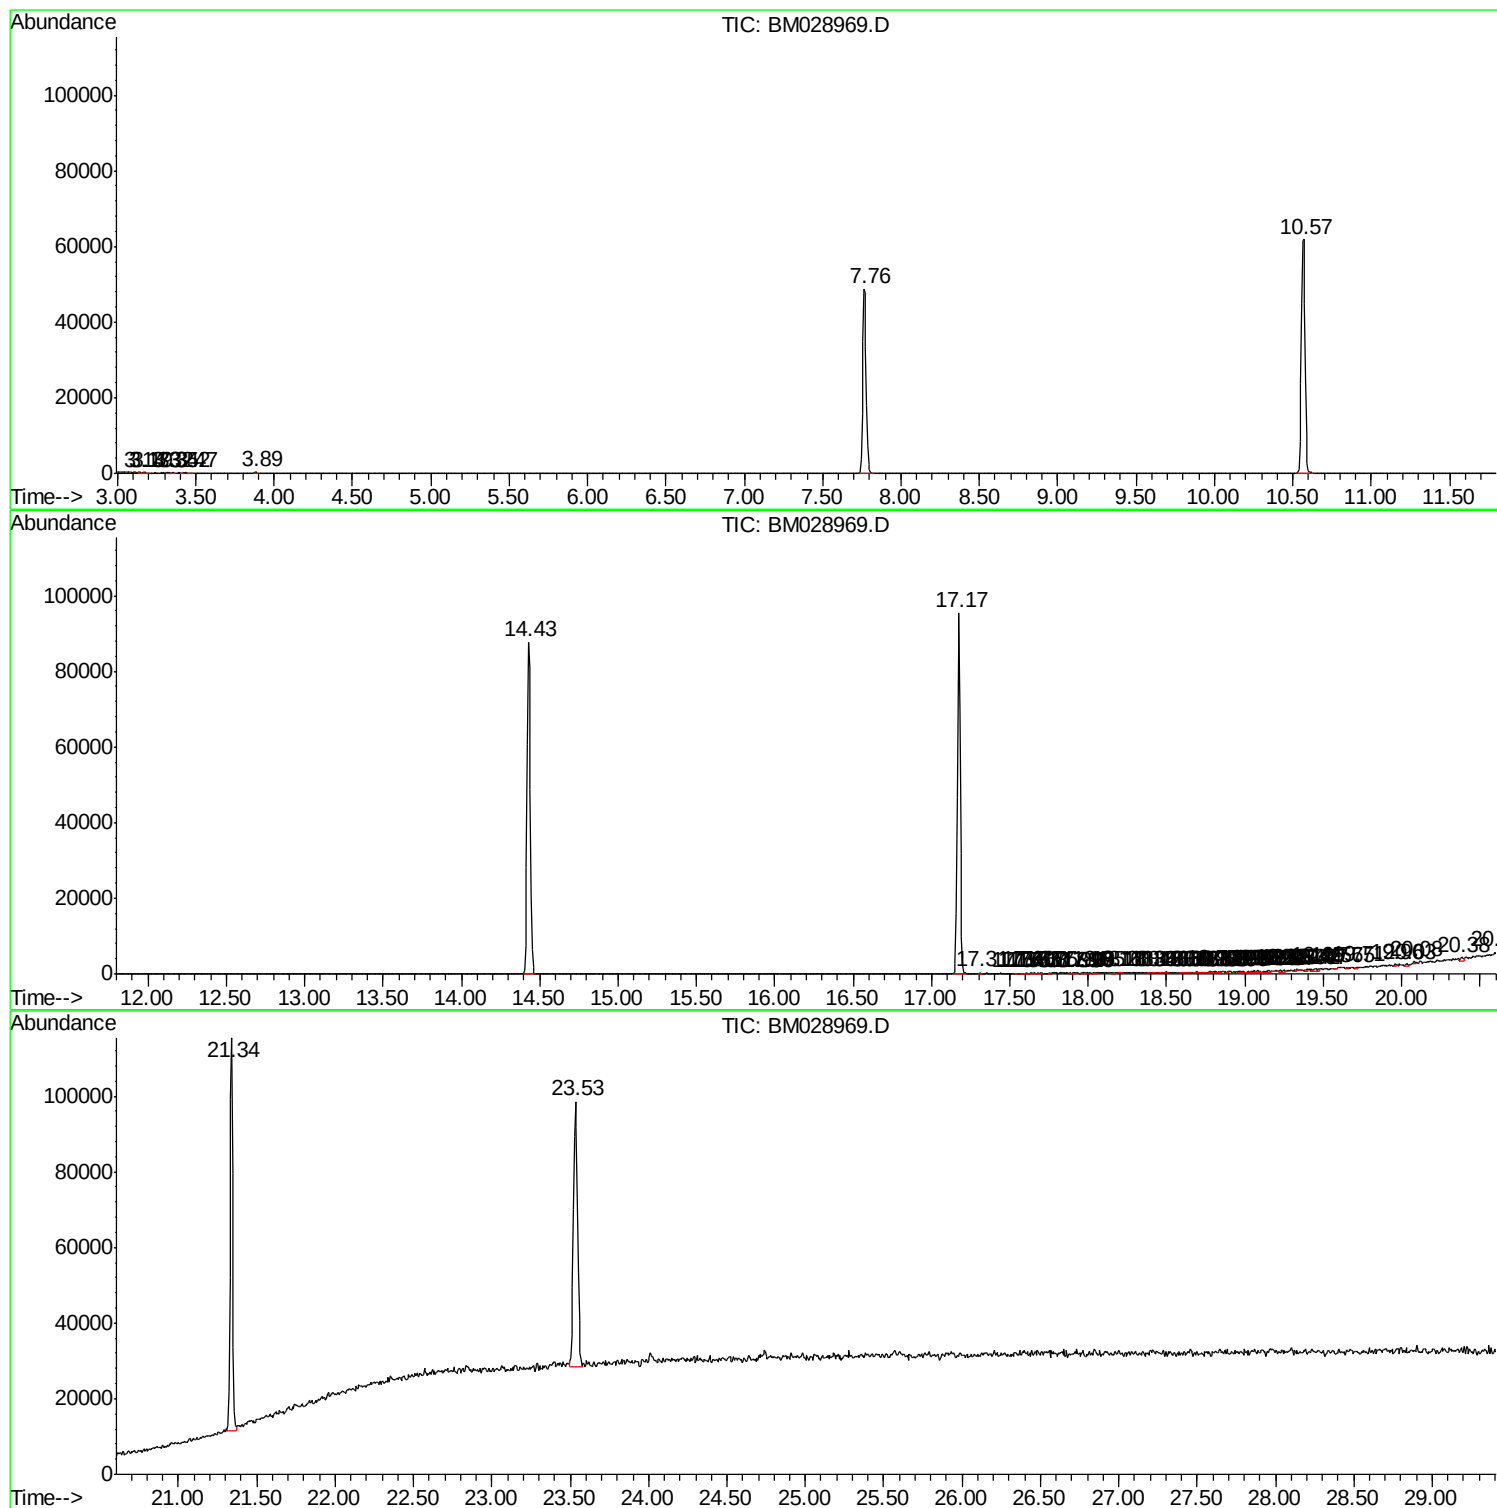

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM030321\
Data File : BM028969.D
Acq On : 03 Mar 2021 10:09
Operator : CG/JU
Sample : M1505-05
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM022721MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM030321\
Data File : BM028969.D
Acq On : 03 Mar 2021 10:09
Operator : CG/JU
Sample : M1505-05
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM022721MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc