

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030321\
 Data File : BM028970.D
 Acq On : 03 Mar 2021 10:45
 Operator : CG/JU
 Sample : M1505-10
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SVOC-GPC2-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM022721MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.169	29	31	32	rVB	225	156	0.11%	0.022%
2	3.187	32	34	36	rBV	263	242	0.18%	0.034%
3	3.252	42	45	48	rVB	244	236	0.17%	0.033%
4	3.281	48	50	51	rBV	206	153	0.11%	0.022%
5	3.634	109	110	113	rVB	227	233	0.17%	0.033%
6	3.881	150	152	155	rBB	404	351	0.25%	0.050%
7	4.046	178	180	183	rBB	176	235	0.17%	0.033%
8	7.769	807	813	821	rBB	47643	74380	53.93%	10.520%
9	10.563	1282	1288	1299	rBB	61420	102065	74.01%	14.436%
10	14.427	1940	1945	1952	rBB	91035	127383	92.36%	18.017%
11	17.174	2406	2412	2418	rBV	101992	137913	100.00%	19.506%
12	17.521	2470	2471	2473	rBV	157	164	0.12%	0.023%
13	17.721	2503	2505	2507	rBB	179	176	0.13%	0.025%
14	17.739	2507	2508	2511	rBB	211	191	0.14%	0.027%
15	17.768	2511	2513	2514	rBV	175	168	0.12%	0.024%
16	17.815	2520	2521	2523	rBV	192	182	0.13%	0.026%
17	17.857	2526	2528	2531	rVB	193	249	0.18%	0.035%
18	17.880	2531	2532	2536	rBV	204	319	0.23%	0.045%
19	17.910	2536	2537	2540	rVB	235	239	0.17%	0.034%
20	17.992	2548	2551	2552	rBV	183	233	0.17%	0.033%
21	18.668	2662	2666	2668	rBV	145	138	0.10%	0.020%
22	18.727	2675	2676	2680	rVB	243	186	0.13%	0.026%
23	18.768	2680	2683	2684	rBV	315	243	0.18%	0.034%
24	18.986	2718	2720	2722	rBV	230	184	0.13%	0.026%
25	19.068	2731	2734	2735	rBV	213	156	0.11%	0.022%
26	19.086	2735	2737	2739	rVB	237	171	0.12%	0.024%
27	19.127	2741	2744	2745	rBV	563	432	0.31%	0.061%
28	19.139	2745	2746	2748	rBV	244	207	0.15%	0.029%
29	19.157	2748	2749	2750	rVB	447	158	0.11%	0.022%
30	19.180	2750	2753	2755	rBV	250	236	0.17%	0.033%
31	19.198	2755	2756	2757	rBV	373	181	0.13%	0.026%
32	19.221	2757	2760	2762	rVB	443	353	0.26%	0.050%
33	19.274	2768	2769	2771	rBV	297	270	0.20%	0.038%
34	19.292	2771	2772	2773	rVV	296	138	0.10%	0.020%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030321\
 Data File : BM028970.D
 Acq On : 03 Mar 2021 10:45
 Operator : CG/JU
 Sample : M1505-10
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SVOC-GPC2-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM022721MA.M
 Title : SVOA CALIBRATION

35	19.345	2778	2781	2784	rBV2	499	784	0.57%	0.111%
36	19.374	2784	2786	2787	rVB	301	200	0.15%	0.028%
37	19.421	2791	2794	2798	rBV2	489	762	0.55%	0.108%
38	19.509	2807	2809	2811	rVB2	257	183	0.13%	0.026%
39	19.557	2814	2817	2819	rBV2	310	400	0.29%	0.057%
40	19.574	2819	2820	2821	rBV	341	192	0.14%	0.027%
41	19.592	2821	2823	2825	rVV3	304	270	0.20%	0.038%
42	19.627	2828	2829	2832	rBV2	253	226	0.16%	0.032%
43	19.715	2843	2844	2846	rBV	398	277	0.20%	0.039%
44	19.780	2853	2855	2858	rVB3	439	288	0.21%	0.041%
45	19.857	2867	2868	2869	rBV	529	200	0.15%	0.028%
46	19.951	2883	2884	2885	rBV	474	172	0.12%	0.024%
47	20.080	2904	2906	2908	rBV2	764	720	0.52%	0.102%
48	20.168	2919	2921	2925	rBV2	766	1018	0.74%	0.144%
49	20.221	2928	2930	2931	rBV	866	605	0.44%	0.086%
50	21.339	3115	3120	3125	rBV	108154	127615	92.53%	18.050%
51	23.533	3487	3493	3500	rBV2	69895	124781	90.48%	17.649%


Sum of corrected areas: 707014

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030321\
Data File : BM028970.D
Acq On : 03 Mar 2021 10:45
Operator : CG/JU
Sample : M1505-10
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM022721MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

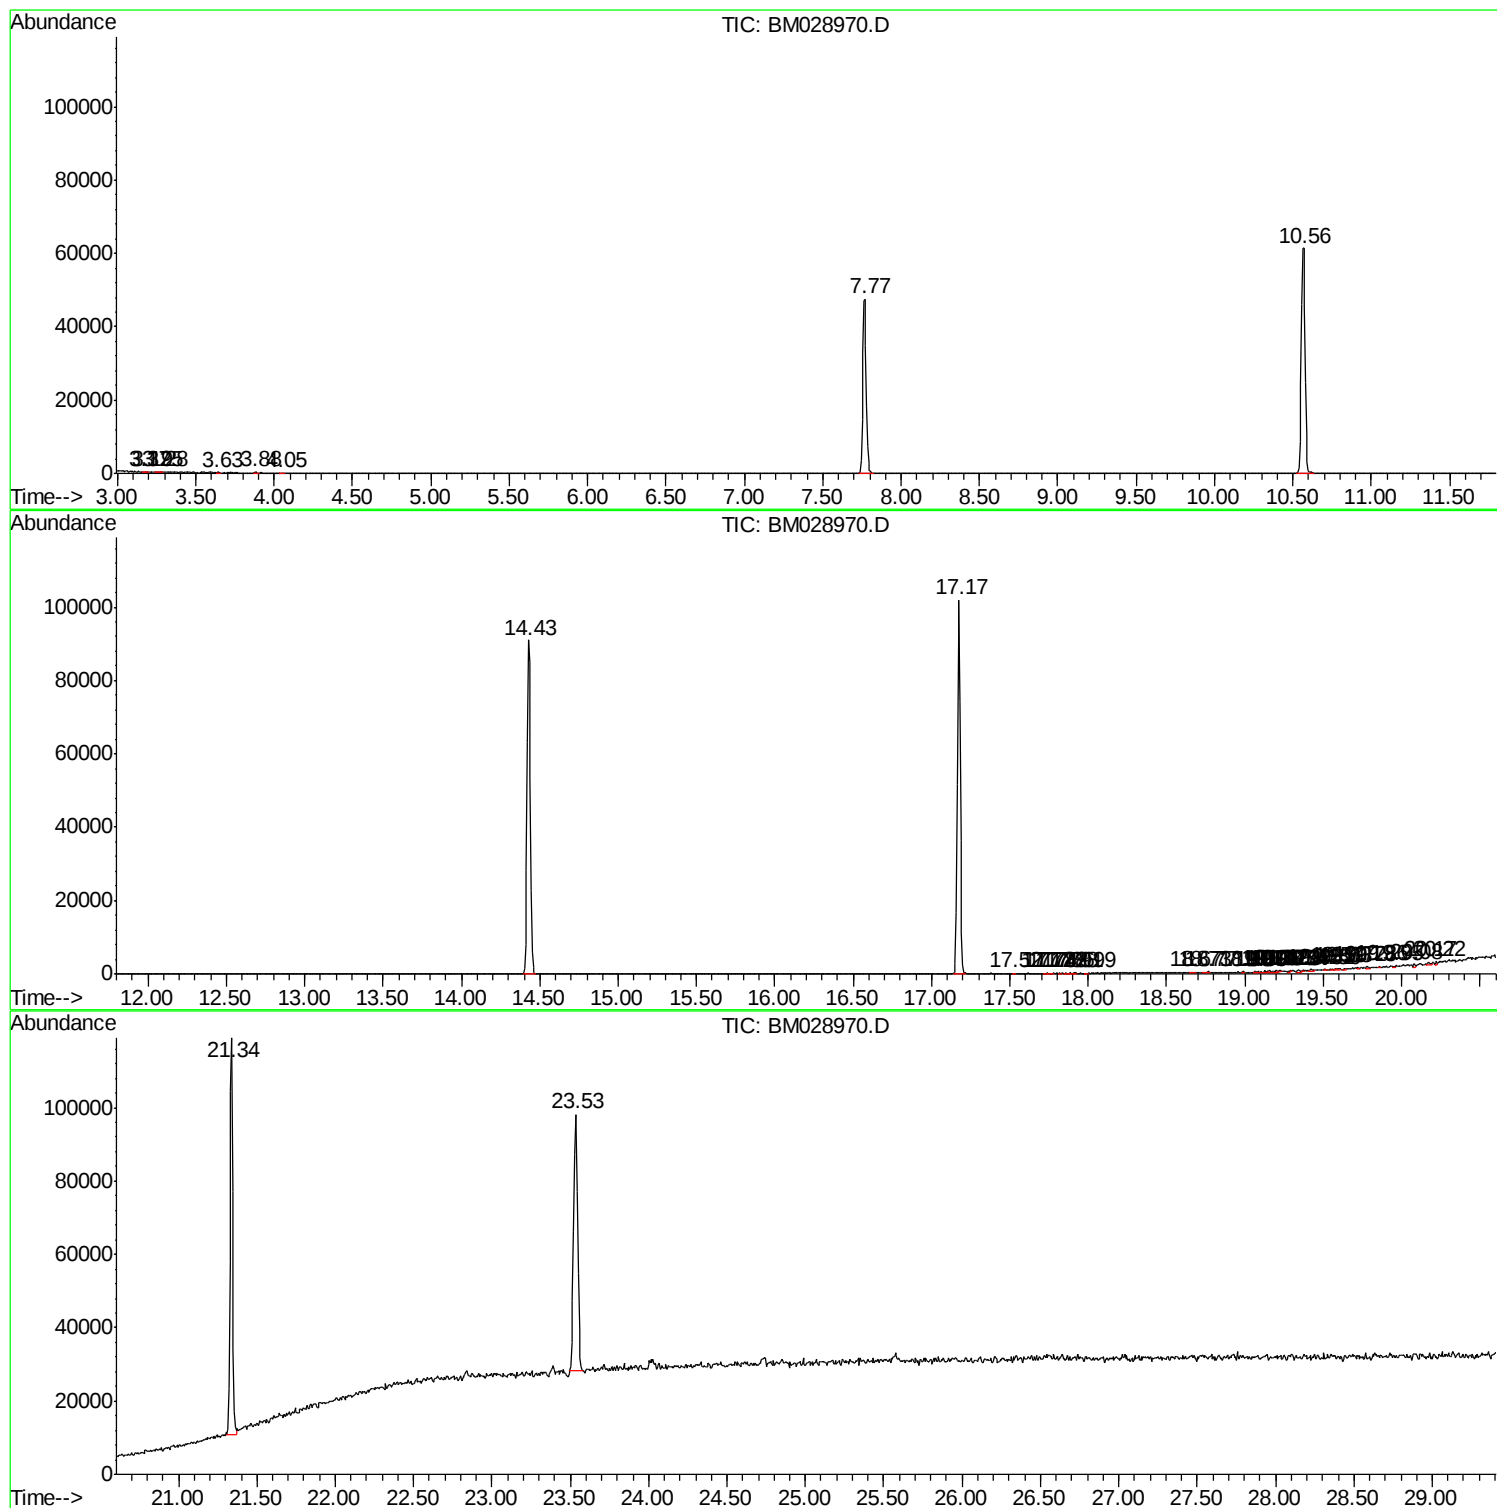

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM030321\
Data File : BM028970.D
Acq On : 03 Mar 2021 10:45
Operator : CG/JU
Sample : M1505-10
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM022721MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM030321\
Data File : BM028970.D
Acq On : 03 Mar 2021 10:45
Operator : CG/JU
Sample : M1505-10
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM022721MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc