


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM030321\
 Data File : BM028967.D
 Acq On : 03 Mar 2021 08:56
 Operator : CG/JU
 Sample : DFTPP39
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP39

Integration File: LSCINT.P

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM022721MA.M
 Title : SVOA CALIBRATION
 Last Update : Wed Mar 03 10:15:41 2021

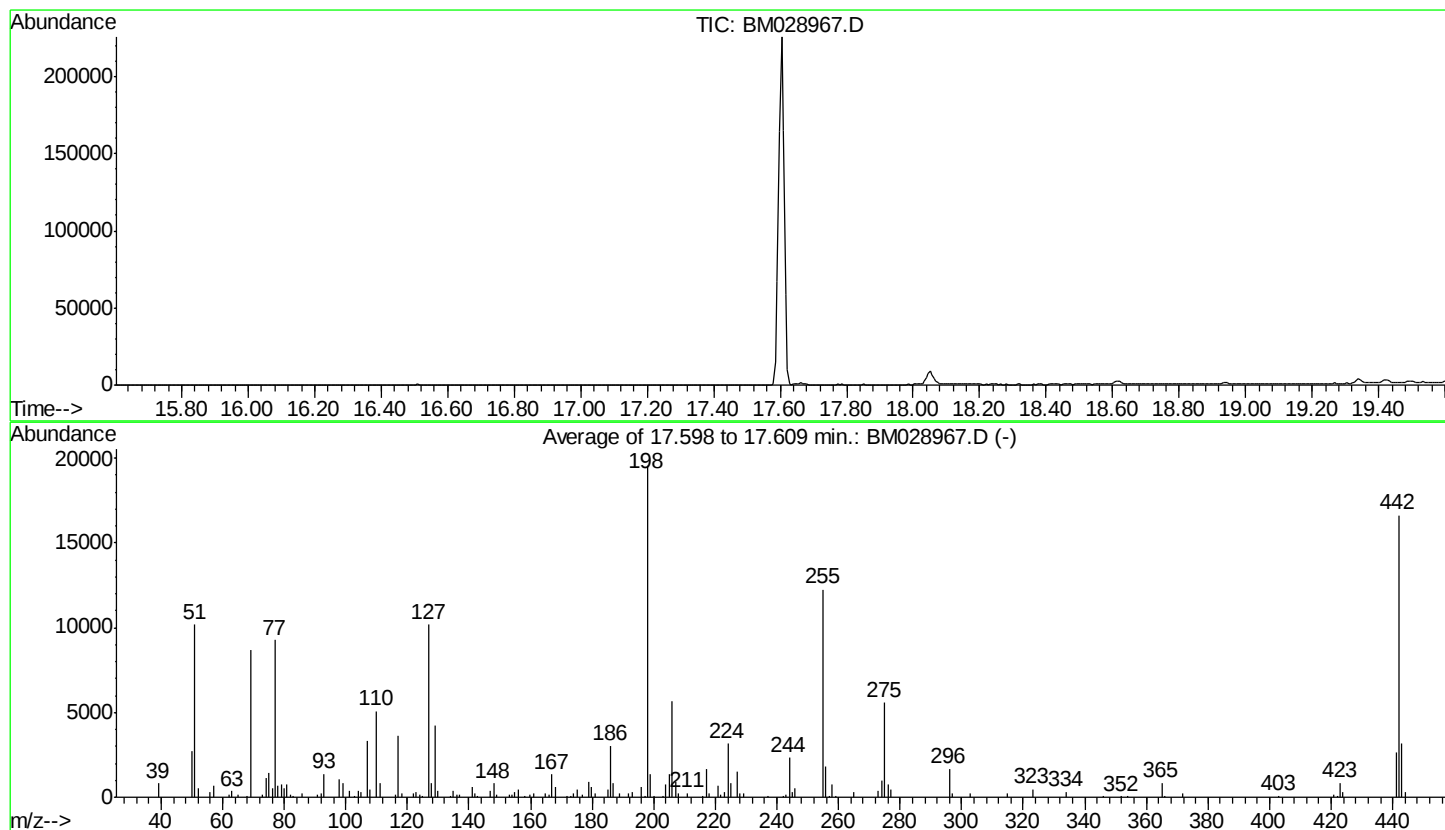

AutoFind: Scans 2484, 2485, 2486; Background Corrected with Scan 2479

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.0	10169	PASS
68	69	0.00	2	0.8	67	PASS
69	198	0.00	100	44.3	8653	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.0	10174	PASS
197	198	0.00	2	0.3	67	PASS
198	198	100	100	100.0	19549	PASS
199	198	5	9	7.1	1382	PASS
275	198	10	60	28.5	5562	PASS
365	198	1	100	4.3	839	PASS
441	198	0.01	100	13.4	2619	PASS
442	198	50	100	84.9	16606	PASS
443	442	15	24	19.2	3193	PASS

m/z	Abundance
44.00	183.0

Instrument :
BNA_M
ClientSampleId :
DFTPP39

m/z	Abundance
39.00	858.0
43.90	180.0
50.00	2881.0
51.00	10509.0
52.00	531.0
56.00	268.0
57.00	725.0
61.90	165.0
63.00	367.0
65.00	176.0
69.00	9235.0
73.00	184.0
74.00	1093.0
75.00	1376.0
76.00	557.0
77.00	9562.0
78.00	659.0
79.00	731.0
80.00	588.0
81.00	650.0
82.00	192.0
85.90	284.0
90.90	184.0
91.90	204.0
93.00	1402.0
98.00	1086.0
98.90	873.0
101.00	363.0
103.90	405.0
104.90	265.0
107.00	3314.0
107.90	465.0
110.00	4810.0
111.00	794.0
116.00	190.0
117.00	3404.0
118.00	213.0
122.00	236.0
123.00	297.0
124.00	188.0
127.00	9801.0
128.00	762.0
129.00	3974.0
129.90	334.0
135.00	363.0
135.90	162.0
137.00	180.0
141.00	584.0
141.90	214.0
146.90	333.0
148.00	817.0
148.90	160.0
152.90	176.0
154.90	293.0
155.90	395.0
159.90	226.0
161.00	262.0
164.90	218.0
166.00	150.0
167.00	1355.0
168.00	566.0
174.00	164.0
175.00	447.0
176.80	185.0
178.90	751.0
179.90	549.0
181.00	219.0
184.90	381.0
186.00	2633.0
186.90	683.0
189.00	213.0
191.90	218.0
193.00	339.0
195.90	499.0
197.90	17400.0
198.90	1254.0
202.90	167.0
204.00	700.0
205.00	1274.0
206.00	4904.0
207.00	842.0
207.90	209.0
211.00	222.0
216.90	1463.0
217.90	181.0
220.90	583.0
222.90	270.0
224.00	2541.0
225.00	655.0
227.00	1352.0
228.00	198.0
229.00	214.0

Instrument :
BNA_M
ClientSampleId :
DFTPP39

244.00	1908.0
245.00	278.0
246.00	491.0
255.00	10116.0
256.00	1431.0
258.00	620.0
264.90	284.0
273.00	306.0
273.90	801.0
275.00	4265.0
276.00	626.0
276.90	409.0
296.00	1270.0
296.90	173.0
303.00	162.0
315.00	153.0
323.00	373.0
333.90	257.0
365.00	587.0
371.90	200.0
423.00	550.0
423.90	247.0
441.00	1775.0
442.00	10938.0
443.00	2240.0
444.00	255.0

Instrument :
BNA_M
ClientSampleId :
DFTPP39

m/z	Abundance
39.00	957.0
43.90	162.0
50.00	3213.0
51.10	12181.0
52.00	611.0
56.00	422.0
57.00	824.0
61.90	201.0
63.00	416.0
65.00	187.0
67.90	201.0
69.00	10198.0
73.00	181.0
74.00	1372.0
75.00	1812.0
76.00	664.0
77.00	11060.0
78.00	875.0
79.00	962.0
80.00	692.0
80.90	1031.0
82.00	280.0
83.00	182.0
86.00	304.0
90.90	207.0
91.90	294.0
93.00	1703.0
98.00	1315.0
99.00	973.0
100.90	440.0
102.90	183.0
103.90	391.0
105.00	372.0
107.00	4013.0
108.00	526.0
110.00	6334.0
111.00	965.0
116.00	225.0
117.00	4487.0
118.00	296.0
121.90	313.0
123.00	390.0
123.90	228.0
124.90	157.0
127.00	12282.0
127.90	1035.0
129.00	5153.0
129.90	491.0
133.90	182.0
134.90	477.0
136.00	190.0
137.00	211.0
141.00	756.0
141.90	173.0
142.90	175.0
146.90	442.0
148.00	957.0
148.90	195.0
152.90	228.0
153.90	187.0
155.00	390.0
156.00	485.0
157.90	164.0
159.90	239.0
161.00	275.0
164.90	223.0
165.90	198.0
167.00	1553.0
168.00	766.0
171.90	156.0
173.00	172.0
174.00	292.0
174.90	560.0
176.80	274.0
178.90	1174.0
179.90	670.0
181.00	283.0
185.00	508.0
186.00	3901.0
187.00	1068.0
189.00	275.0
192.00	312.0
193.00	364.0
196.00	645.0
197.10	201.0
197.90	23576.0
198.90	1672.0
199.90	182.0
204.00	909.0
205.00	1542.0
206.00	6821.0
207.00	1024.0

Instrument :
BNA_M
ClientSampleId :
DFTPP39

207.90	285.0
211.00	280.0
215.90	200.0
216.90	2058.0
218.00	275.0
221.00	838.0
221.80	258.0
222.90	343.0
224.00	3841.0
225.00	1133.0
227.00	1799.0
228.00	256.0
229.00	305.0
237.00	238.0
241.90	181.0
243.00	189.0
244.00	2790.0
245.00	346.0
246.00	583.0
255.00	14728.0
255.90	2274.0
256.90	192.0
258.00	928.0
259.00	156.0
265.00	423.0
273.00	434.0
274.00	1126.0
275.00	6879.0
276.00	860.0
276.90	536.0
296.00	2062.0
297.00	319.0
302.90	233.0
314.90	249.0
323.00	590.0
334.00	418.0
346.00	154.0
352.00	211.0
364.90	1003.0
372.00	325.0
402.90	158.0
421.00	203.0
421.90	170.0
422.90	988.0
424.00	321.0
441.00	3094.0
442.00	19544.0
443.00	3645.0
444.00	390.0

Instrument :
BNA_M
ClientSampleId :
DFTPP39

m/z	Abundance
39.00	601.0
44.00	163.0
50.00	2156.0
51.00	7818.0
52.00	374.0
55.90	209.0
56.90	481.0
63.00	316.0
69.00	6528.0
74.00	895.0
75.00	1028.0
76.00	425.0
77.00	7170.0
78.00	430.0
79.00	595.0
79.90	390.0
81.00	639.0
91.90	165.0
93.00	1085.0
98.00	881.0
99.00	648.0
101.00	322.0
103.90	254.0
104.90	238.0
107.00	2550.0
107.90	400.0
110.00	4102.0
111.00	665.0
117.00	2910.0
118.00	185.0
122.00	230.0
122.90	262.0
127.00	8439.0
127.90	643.0
129.00	3646.0
130.00	299.0
134.90	371.0
141.00	580.0
142.00	195.0
147.00	300.0
148.00	673.0
152.90	166.0
153.90	169.0
155.00	188.0
156.10	442.0
161.00	212.0
165.00	223.0
167.00	1146.0
167.90	579.0
173.90	239.0
175.00	420.0
178.90	821.0
179.90	590.0
181.00	248.0
185.00	365.0
186.00	2605.0
187.00	771.0
188.90	266.0
191.90	250.0
193.00	283.0
195.90	643.0
197.90	17672.0
198.90	1220.0
203.00	169.0
204.00	713.0
205.00	1224.0
206.00	5292.0
207.00	766.0
208.00	183.0
210.90	251.0
217.00	1502.0
217.90	165.0
220.90	643.0
221.80	205.0
223.00	246.0
224.00	3090.0
225.00	637.0
227.00	1437.0
228.00	162.0
229.00	259.0
243.00	186.0
244.10	2305.0
245.00	272.0
246.00	535.0
255.00	11896.0
256.00	1773.0
257.90	781.0
265.00	296.0
272.90	330.0
274.00	954.0
275.00	5542.0
275.90	694.0

Instrument :
BNA_M
ClientSampleId :
DFTPP39

277.00	510.0
296.00	1728.0
297.00	251.0
303.00	207.0
315.00	247.0
323.00	427.0
333.90	292.0
353.90	175.0
364.90	929.0
365.90	170.0
372.00	265.0
403.00	167.0
421.00	155.0
423.00	980.0
423.80	236.0
441.00	2988.0
442.00	19336.0
443.00	3694.0
443.90	299.0

Instrument :
BNA_M
ClientSampleId :
DFTPP39